

DISCLAIMER

THE USE OF AND RELIANCE UPON THIS RECORDED-DATA BY THE HEREIN NAMED COMPANY (AND ANY OF ITS AFFILIATES, PARTNERS, REPRESENTATIVES, AGENTS, CONSULTANTS AND EMPLOYEES) IS SUBJECT TO THE TERMS AND CONDITIONS AGREED UPON BETWEEN SCHLUMBERGER AND THE COMPANY, INCLUDING: (a) RESTRICTIONS ON USE OF THE RECORDED-DATA; (b) DISCLAIMERS AND WAIVERS OF WARRANTIES AND REPRESENTATIONS REGARDING COMPANY'S USE OF AND RELIANCE UPON THE RECORDED-DATA; AND (c) CUSTOMER'S FULL AND SOLE RESPONSIBILITY FOR ANY INFERENCE DRAWN OR DECISION MADE IN CONNECTION WITH THE USE OF THIS RECORDED-DATA.

OTHER SERVICES1
 OS1:
 OS2: MSS
 OS3:
 OS4:
 OS5:

OTHER SERVICES2
 OS1:
 OS2:
 OS3:
 OS4:
 OS5:

REMARKS: RUN NUMBER 1
 Hole drilled with RCB coring bit and bottom hole assembly (BHA). 9 7/8 " BS
 Coring concluded approximately 24 hours prior to logging.
 Drill pipe set at a depth of 95mbsf with bit dropped at TD.
 Downlog run with corrections computed using bit size; uplogs corrected for actual hole size.
 Lower part of toolstring (MSS and HRLA) centralized using modified MCD inline centralizers.
 Upper part of toolstring (HLDS, APS, HNGS) eccentered using HLDS caliper and bowspring, as per toolsketch.
 APS minitron remained off during downlog to avoid GR interference / formation activation.
 Fluid type was barite+seawater gel mud, barite corrections applied.
 Depth originally recorded from drill floor; played back with sea floor as reference zero.
 All logs presented in measured depth below sea floor (MDBSF).
 Maximum observed temperature on the HRLA temperature was 13.5degC.
 Tools bridged before actual Driller TD at 307m below sea floor.
 Rig lowered pipe after main logging attempt but 2nd logging attempt did not get significantly further so no more data was acquired and remaining logging cancelled for this hole D.

REMARKS: RUN NUMBER 2

RUN 1

SERVICE ORDER #: _____
 PROGRAM VERSION: 19C0-187
 FLUID LEVEL: _____

LOGGED INTERVAL	START	STOP

RUN 2

SERVICE ORDER #: _____
 PROGRAM VERSION: _____
 FLUID LEVEL: _____

LOGGED INTERVAL	START	STOP

EQUIPMENT DESCRIPTION

RUN 1


SURFACE EQUIPMENT

SFT-281 1
 SFT-178 1
 GSR-U 616008
 WITM (EDTS)-A 1

RUN 2

DOWNHOLE EQUIPMENT

LEH-QT 301
 MDSB_EDTC 39.87
 Mud Tempe 38.54
 AH-369 CTEM 38.98
 Gamma Ray 36.91
 EDTC-B EFTB DIAG 38.54
 EDTH-B 8303 TelStatus
 EDTC-B 8317 EDTCB Ele 36.56

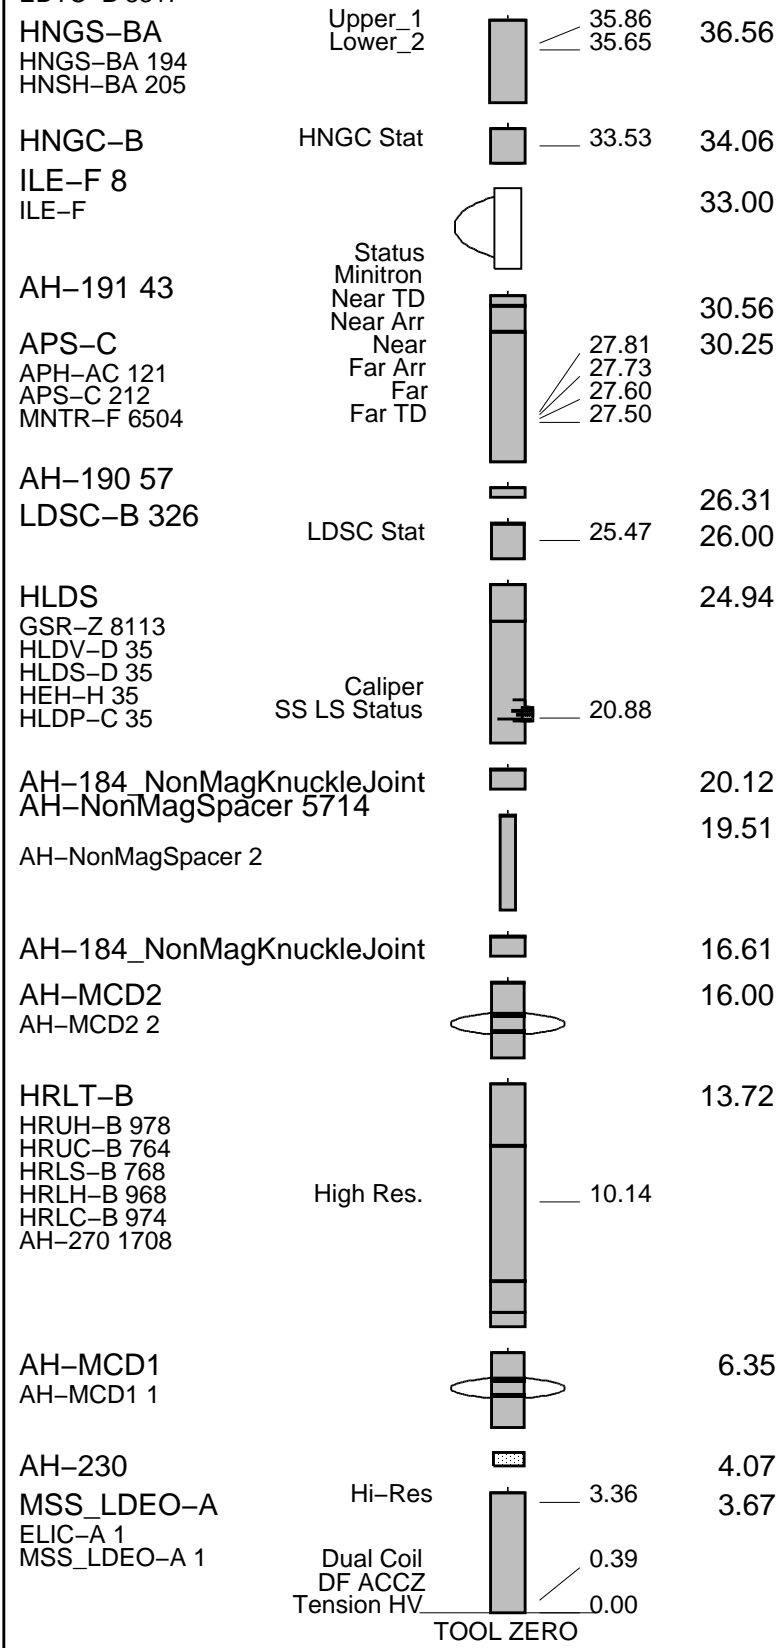


MAXIMUM STRING DIAMETER 3.75 IN
MEASUREMENTS RELATIVE TO TOOL ZERO
ALL LENGTHS IN METERS

Production String	(in)	(M)	Well Schematic	(M)	(in)	Casing String
	OD	ID		MD	MD	

Kelly Bushing Elevation
Derrick Floor Elevation

Mean Sea Level

-471
-471
-4700

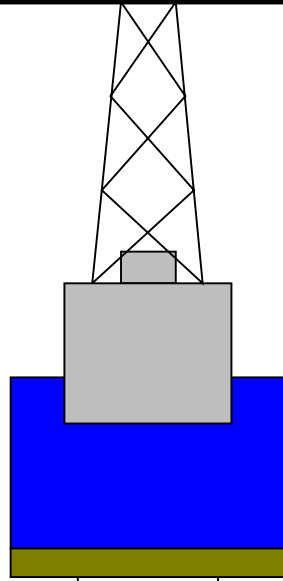

4.1

Sea Floor

0

4.1

Drill Pipe

95

Open Hole

9.875

Total Depth

897.8



Input DLIS Files

DEFAULT MSS_LDEO_HRLA_LDL_018LUP FN:26 PRODUCER 19-Jun-2014 00:41 5029.2 M 4689.2 M

Output DLIS Files

DEFAULT MSS_LDEO_HRLA_LDL_033PUP FN:46 PRODUCER 20-Jun-2014 18:21 312.4 M -27.7 M

OP System Version: 19C0-187

MSS_LDEO-A	19C0-187	HRLT-B	19C0-187
HLDS	19C0-187	LDSC-B	19C0-187
APS-C	19C0-187	HNGC-B	19C0-187
HNGS-BA	19C0-187	EDTC-B	SKK-5169-EDTCB

PIP SUMMARY

Time Mark Every 60 S

HRLT True Resistivity (RT_HRLT)		
0.2	(OHMM)	20
HRLT Resistivity 1 (RLA1)		HLDS Bulk Density Correction (DRH)
0.2	(OHMM)	20 -0.25 (G/C3) 0.25
HRLT Resistivity 2 (RLA2)		HLDS Long Spaced Photoelectric Effect (PEFL)
0.2	(OHMM)	20 0 (----) 10
HRLT Resistivity 3 (RLA3)		HLDS Bulk Density (RHOM)

Main Log

HNGS Spectroscopy Gamma Ray
(HSGR)
(GAPI) 100

0 100

Calibrated
Downhole
Force
(CDF)
(LBF)

3000 0

HRLT Resistivity 5 (RLA5)
(OHMM) 20

0.2 20

APS Array to Far Porosity (AFLU)
(PU) 0

100 0

HLDS Caliper (LCAL)
(IN) 20

0 20

Tension
(TENS)
(LBF)


10000 0


HRLT Resistivity 4 (RLA4)
(OHMM) 20


0.2 20



APS Corrected Standoff Porosity
(STPC)
(PU) 0




100 0

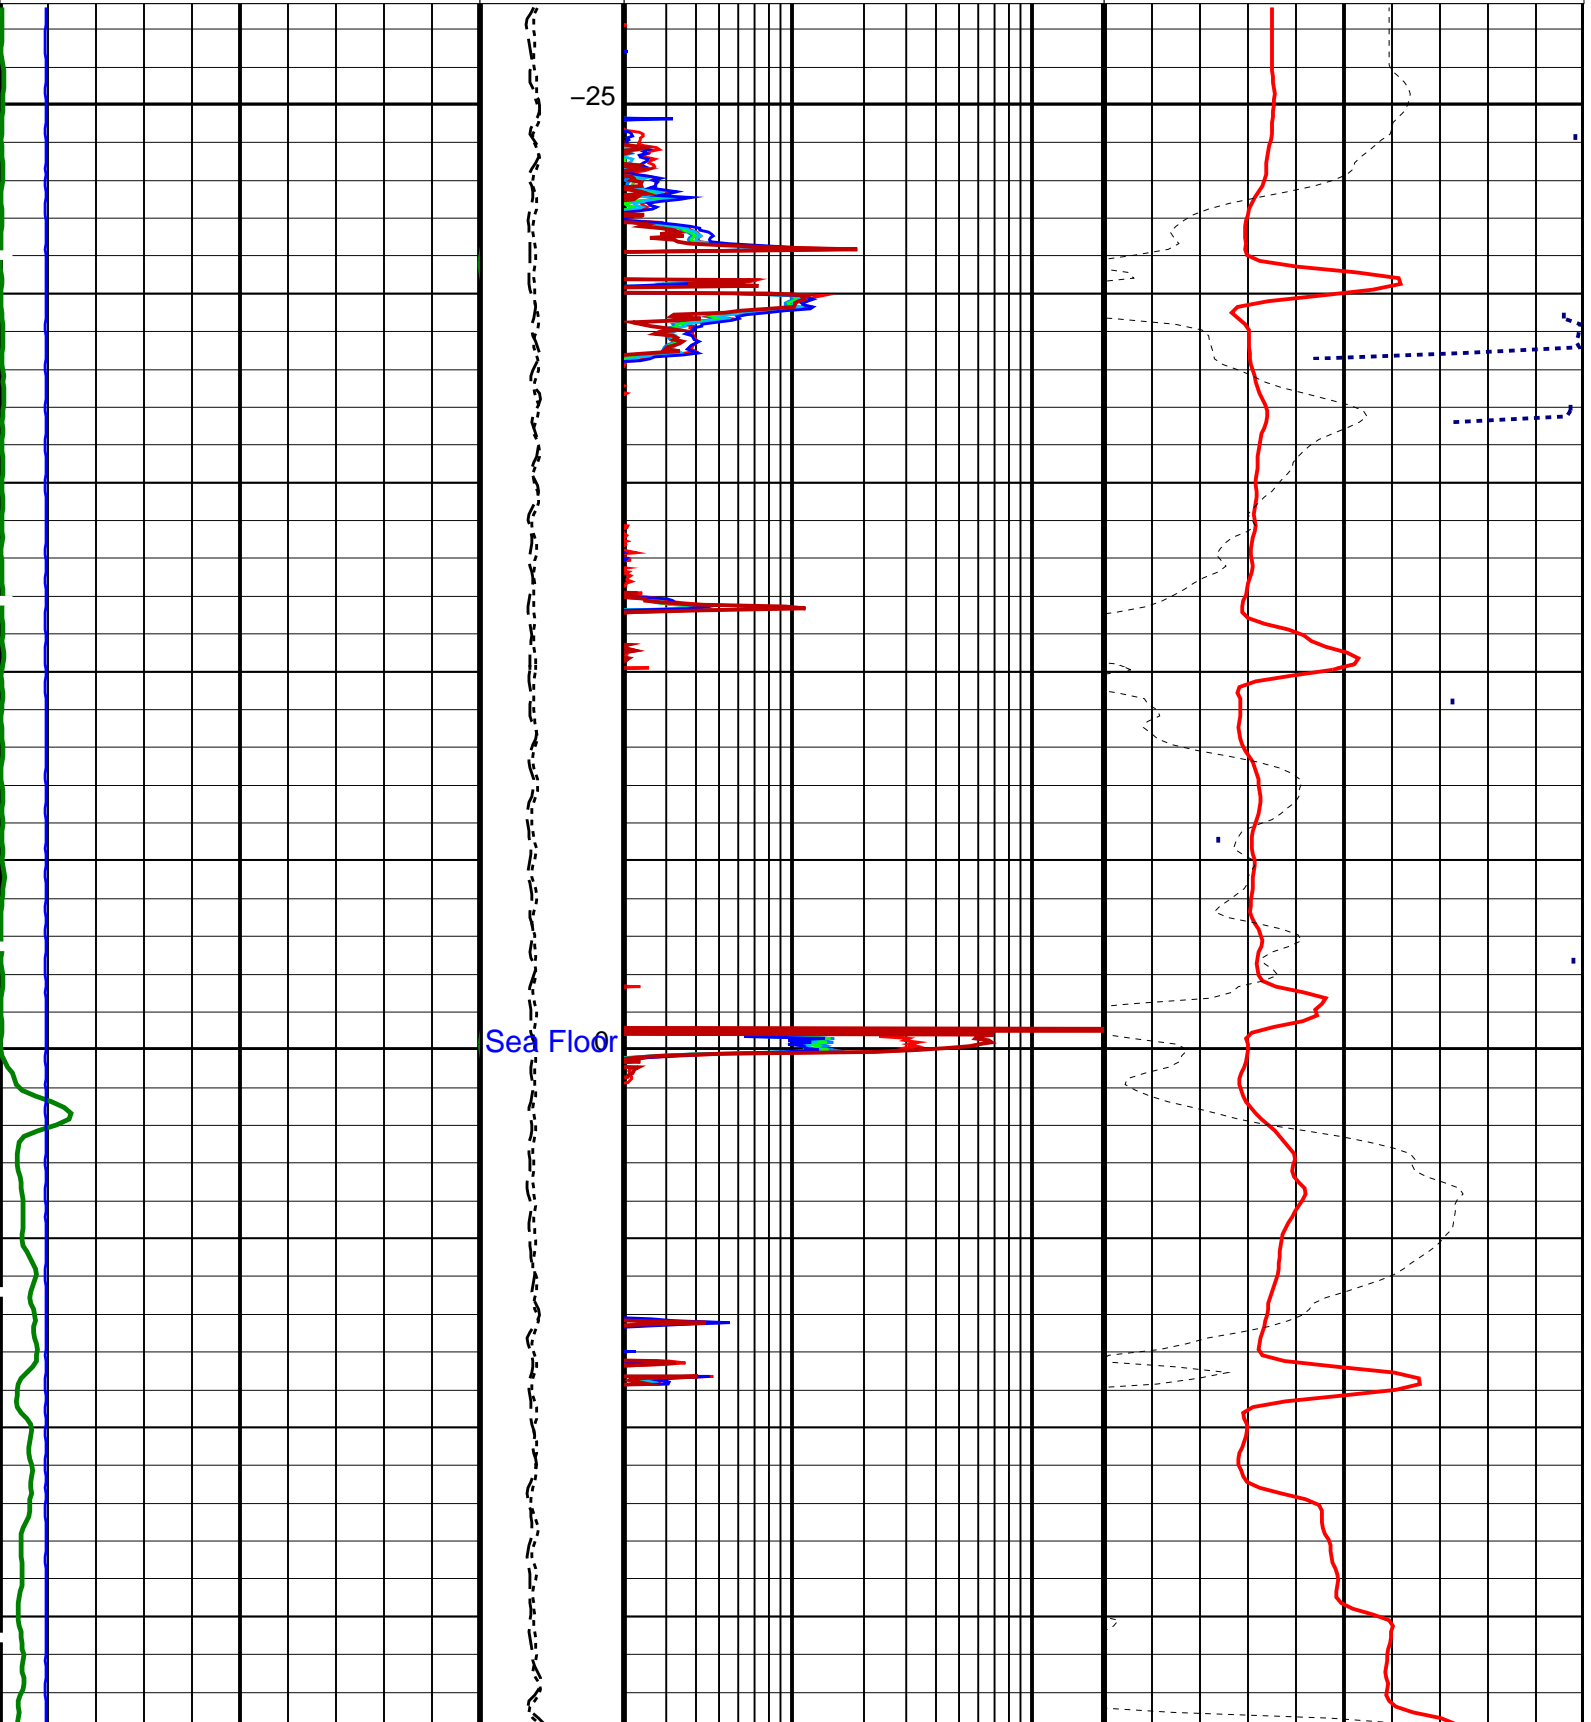


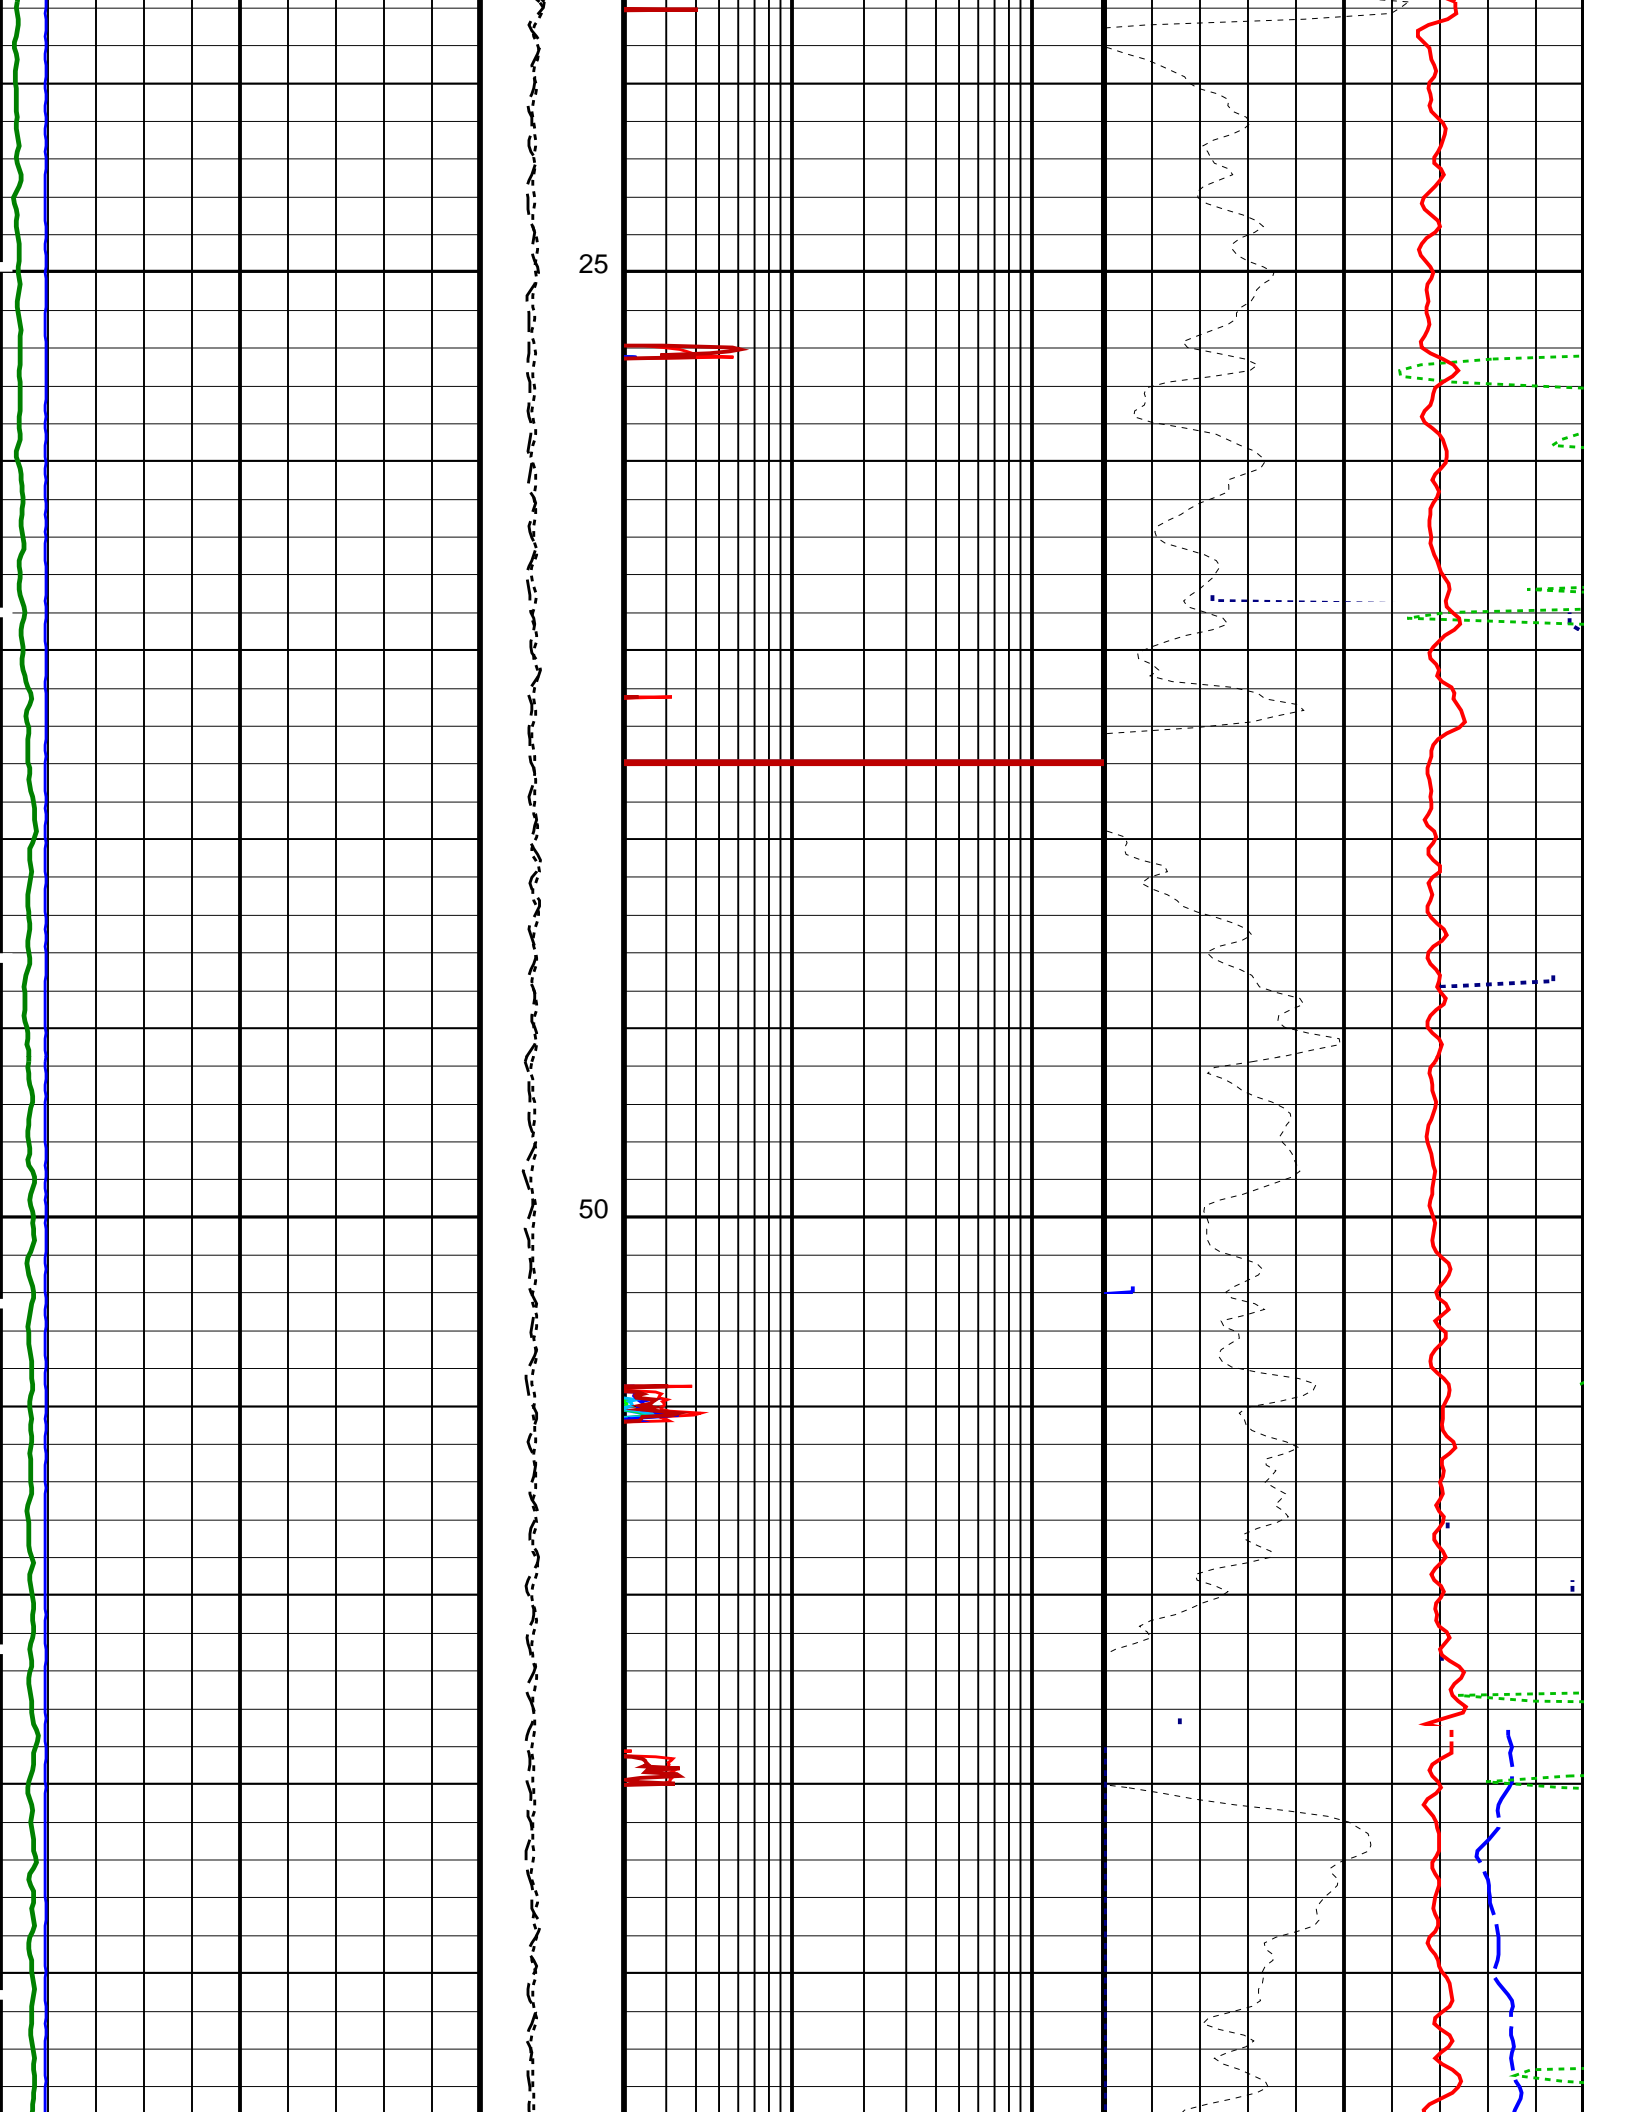


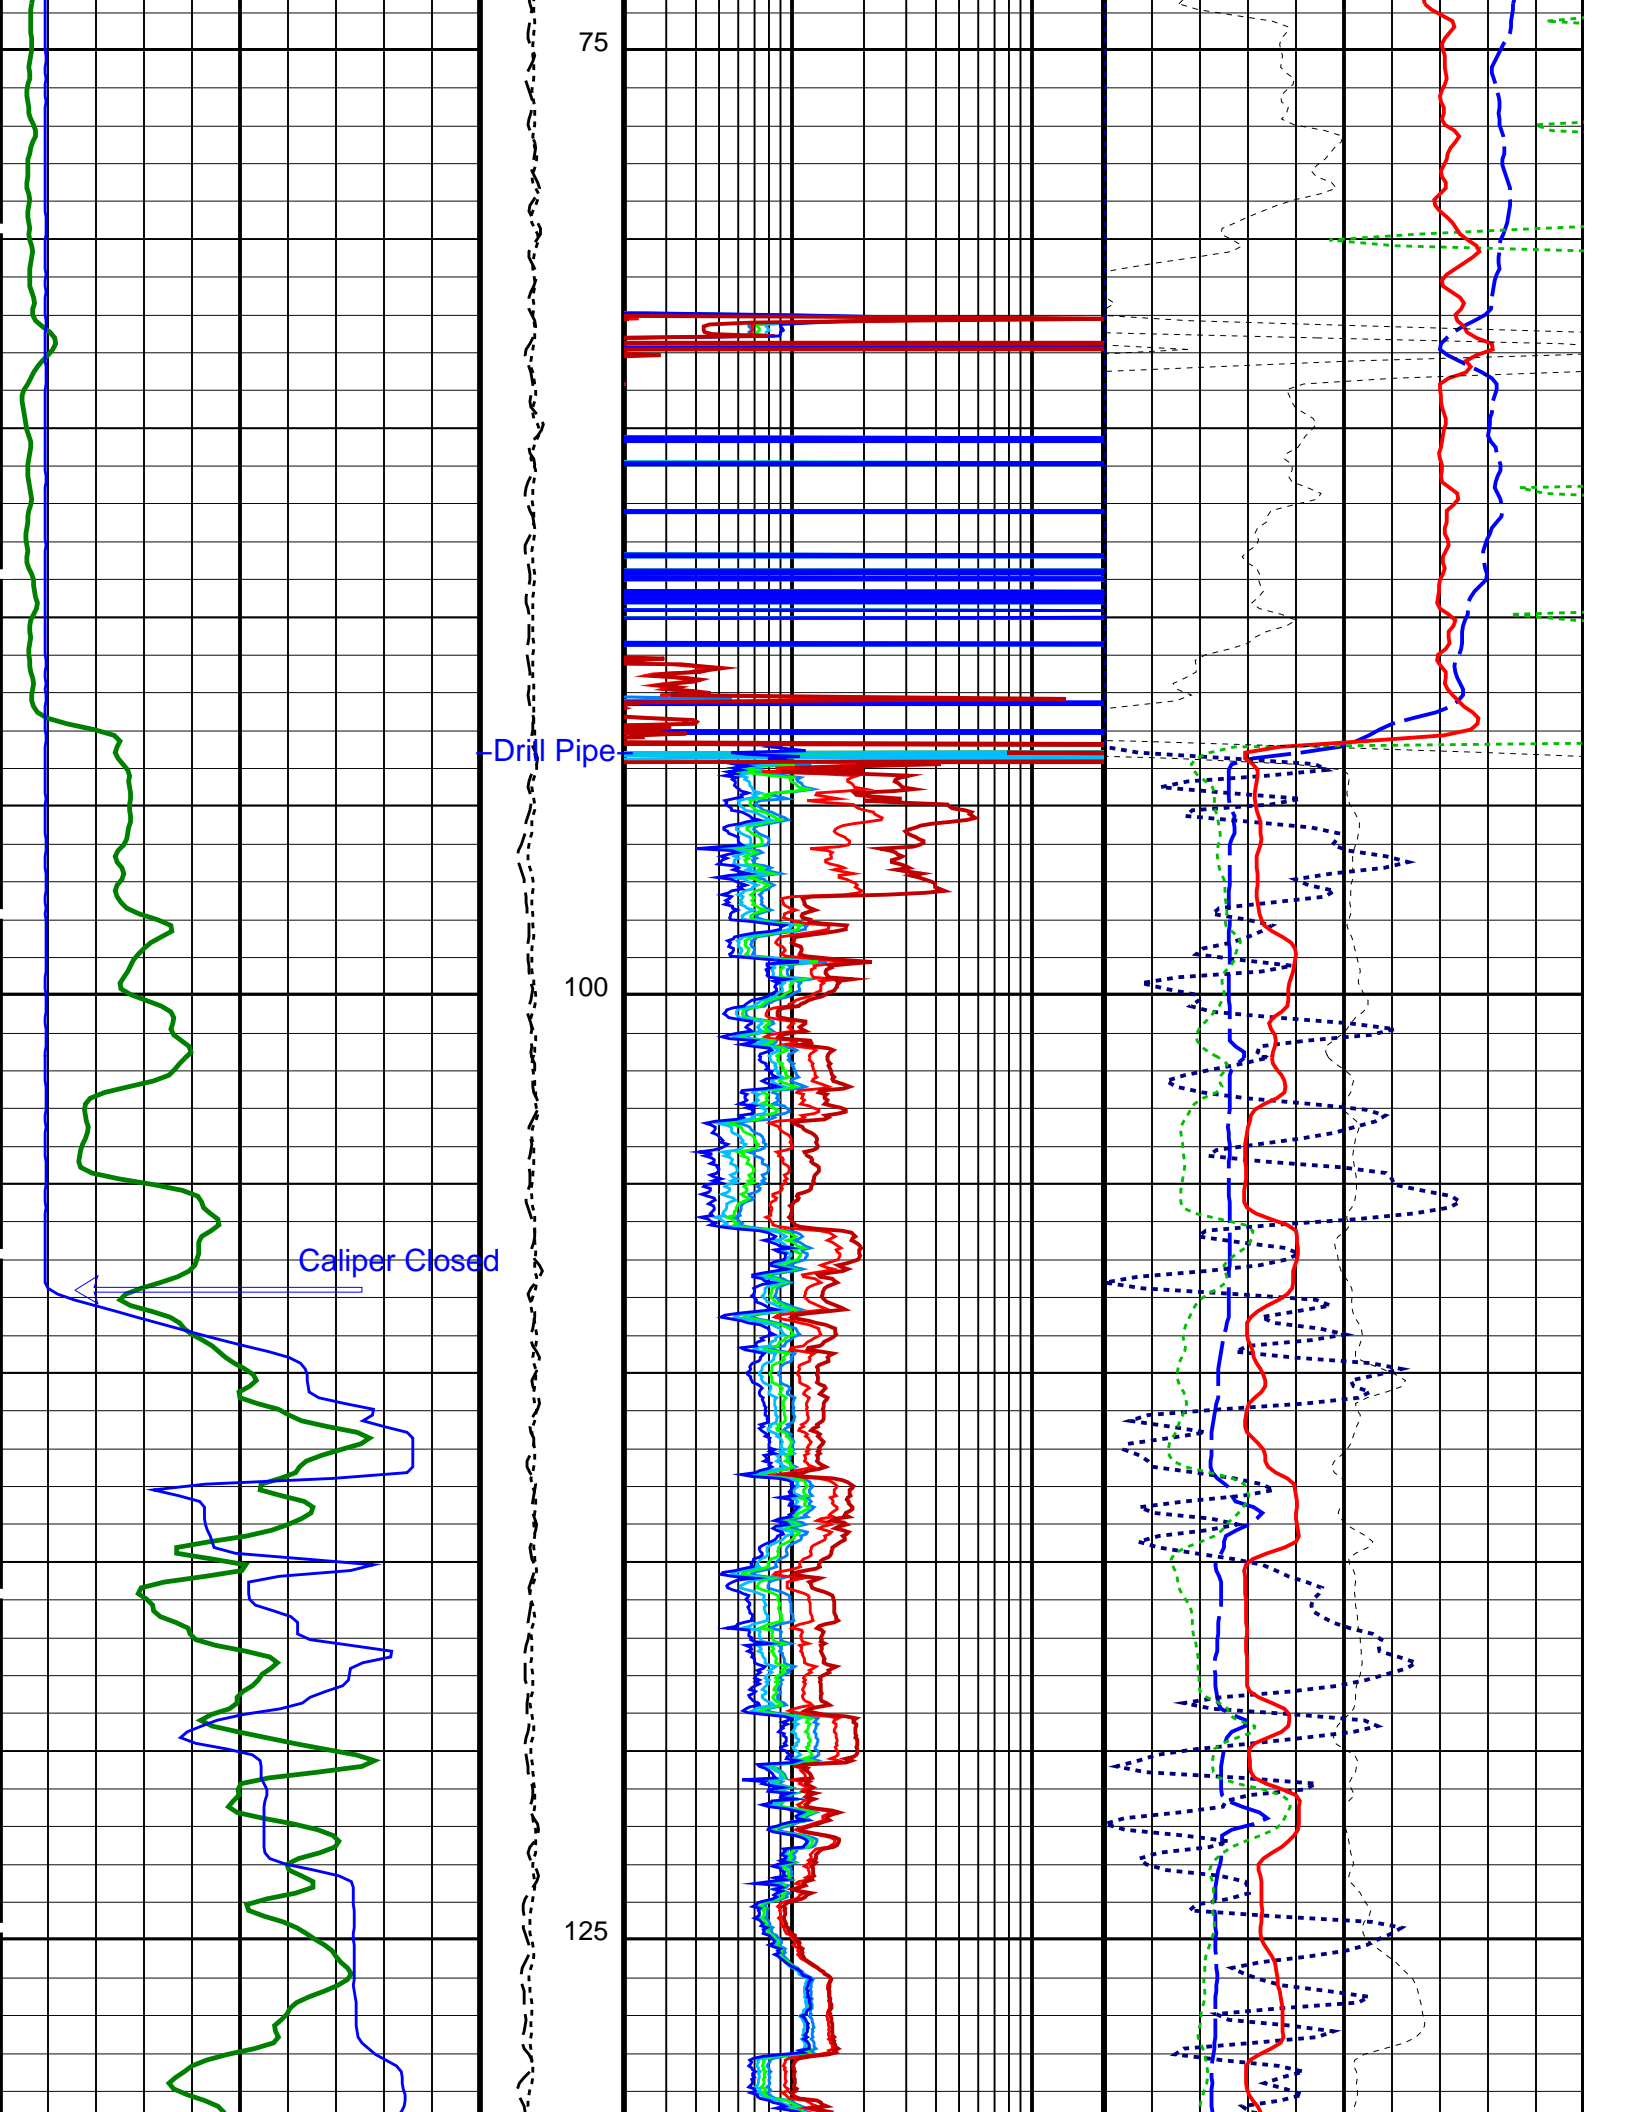

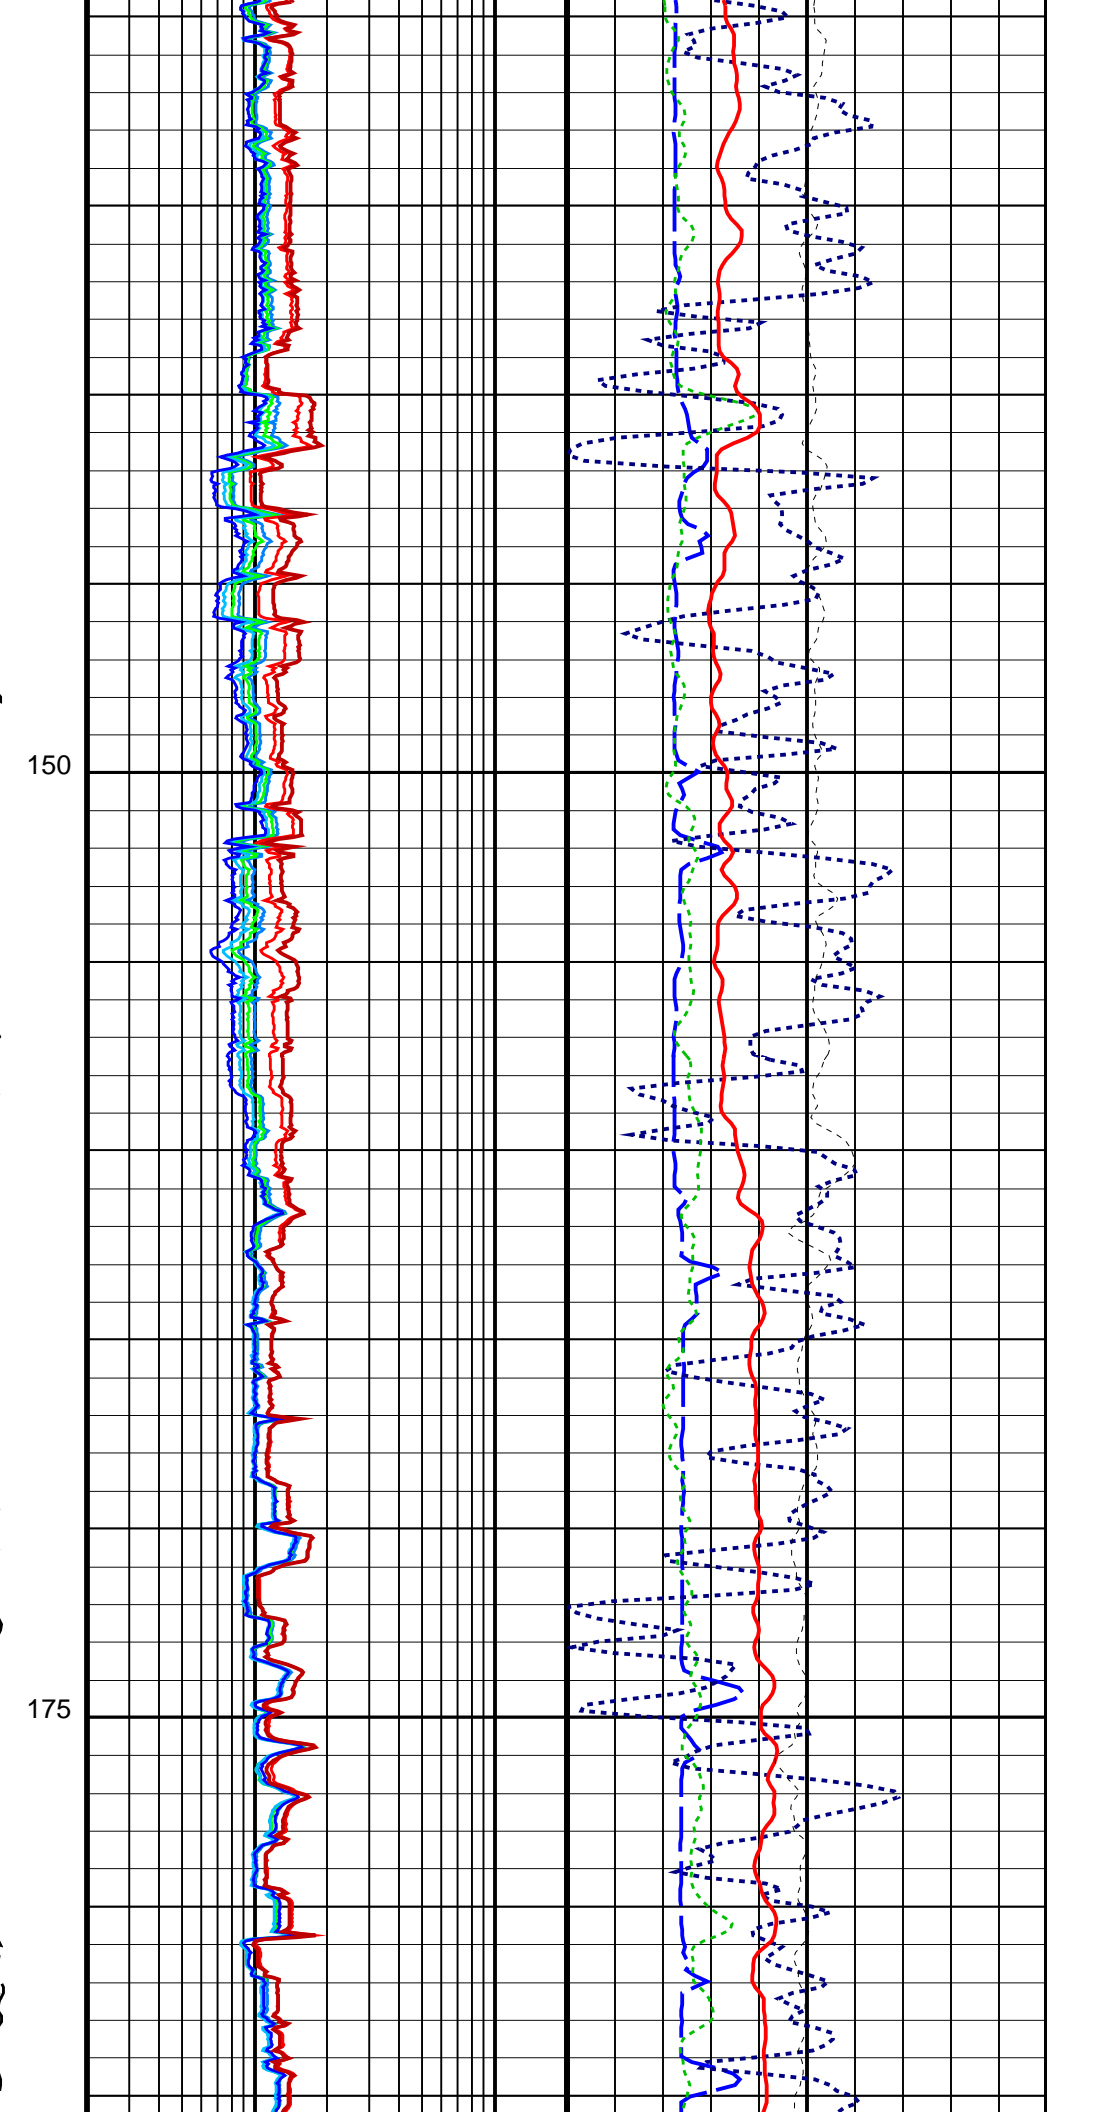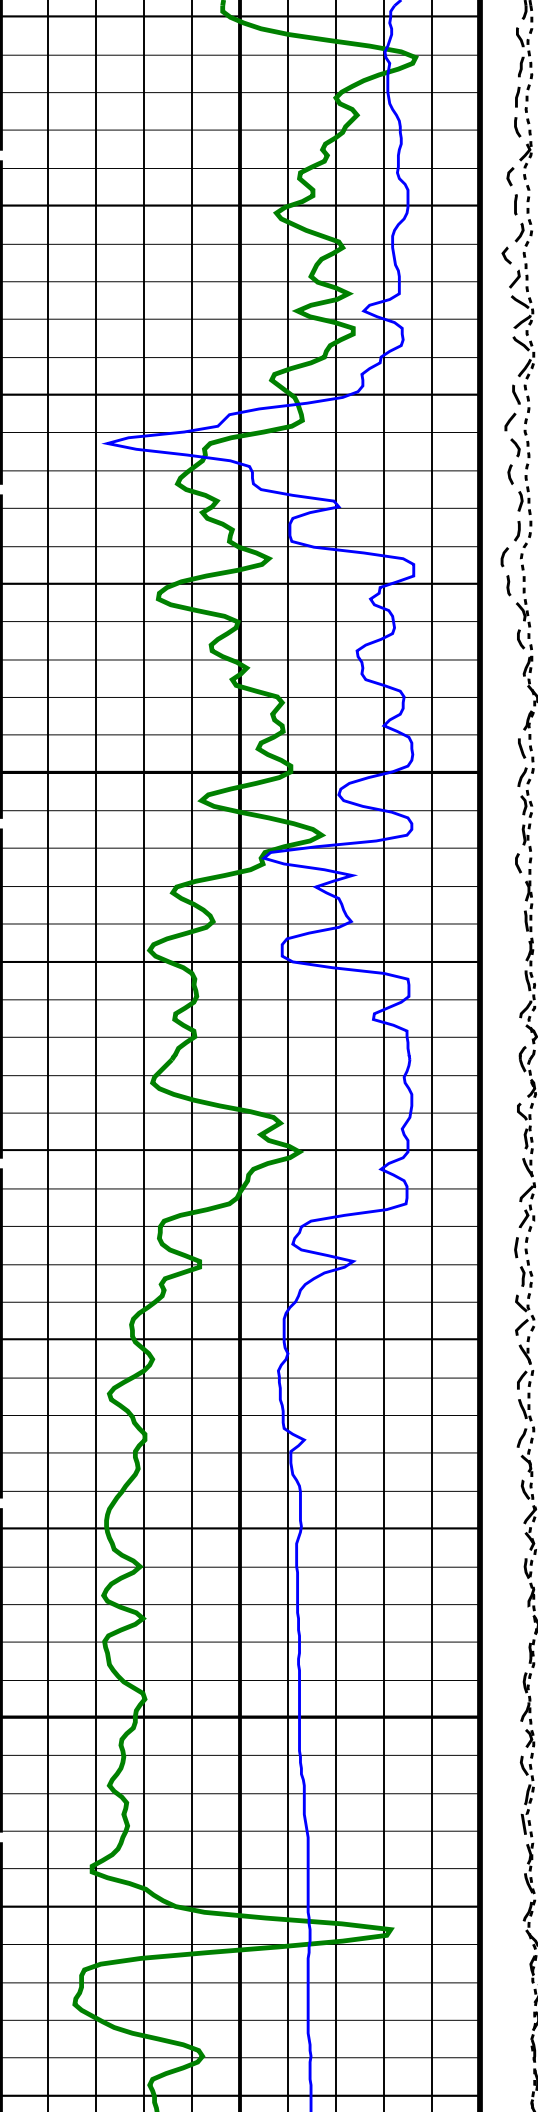

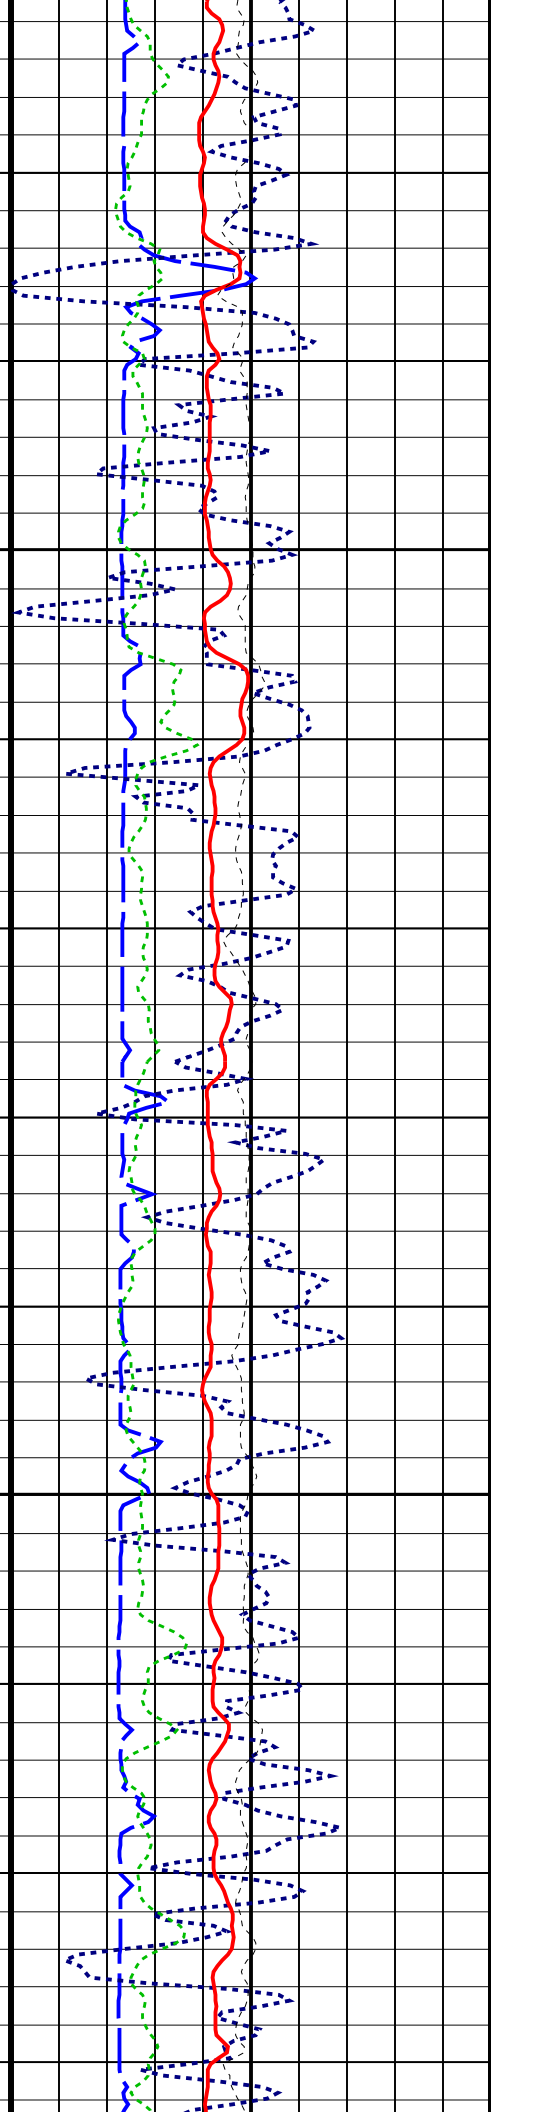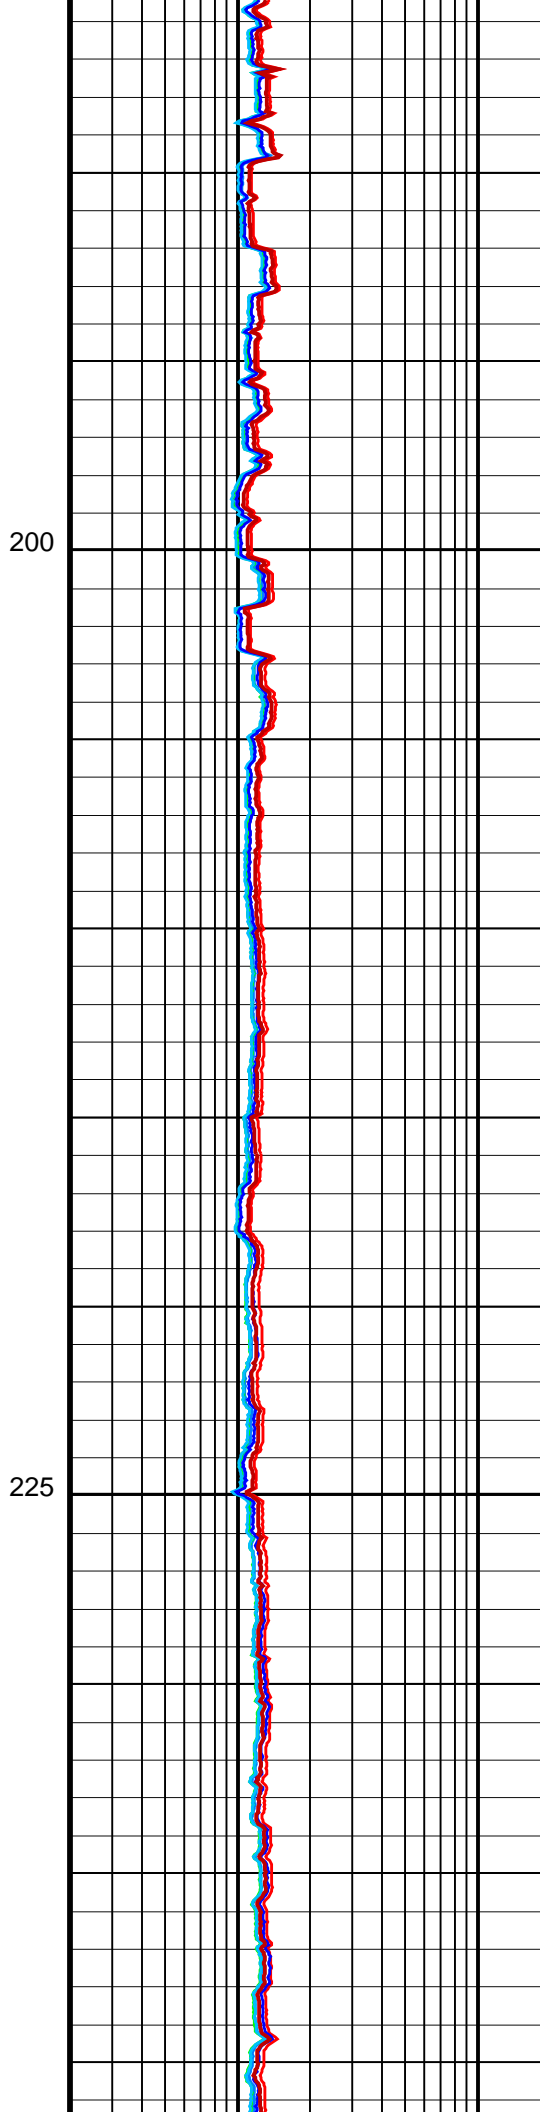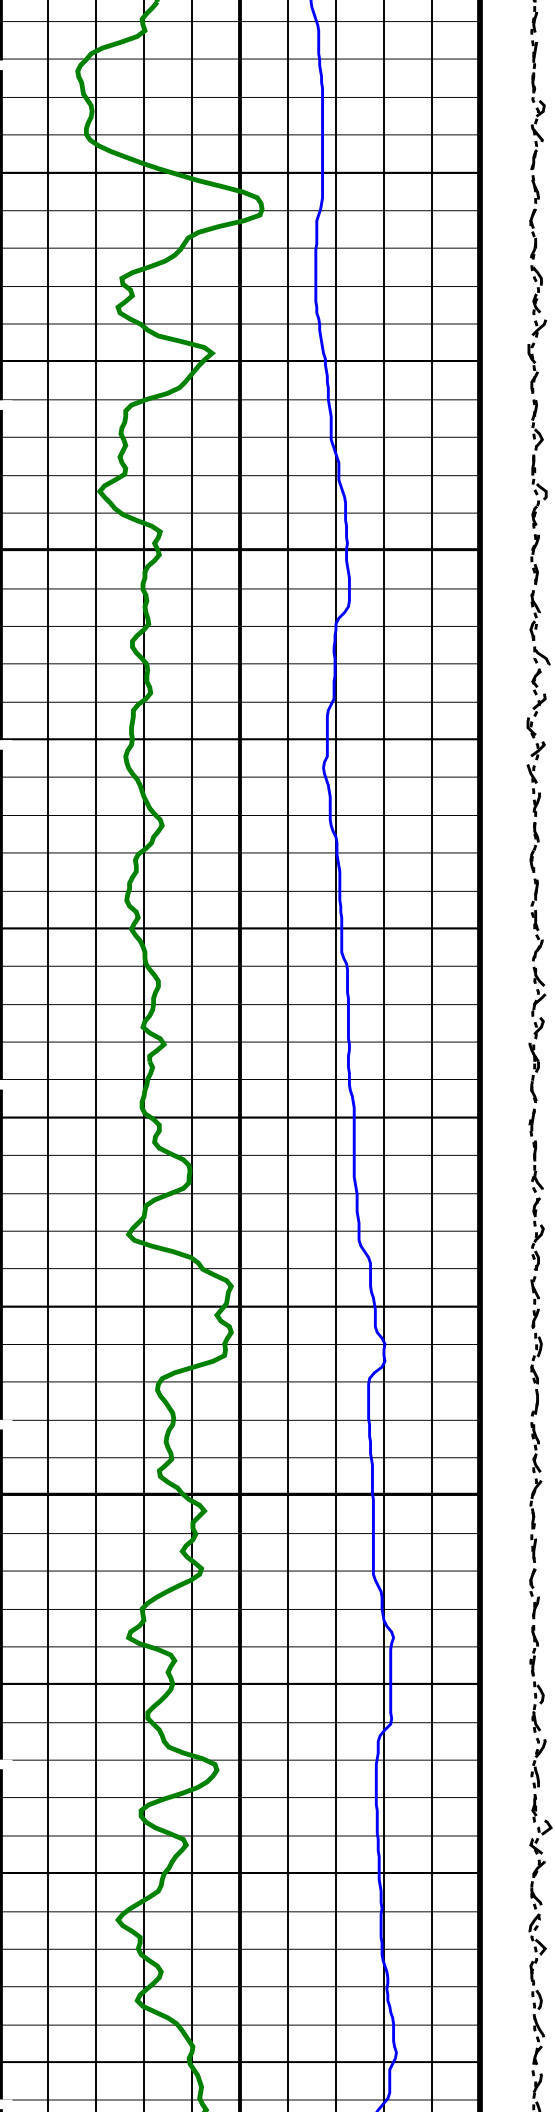

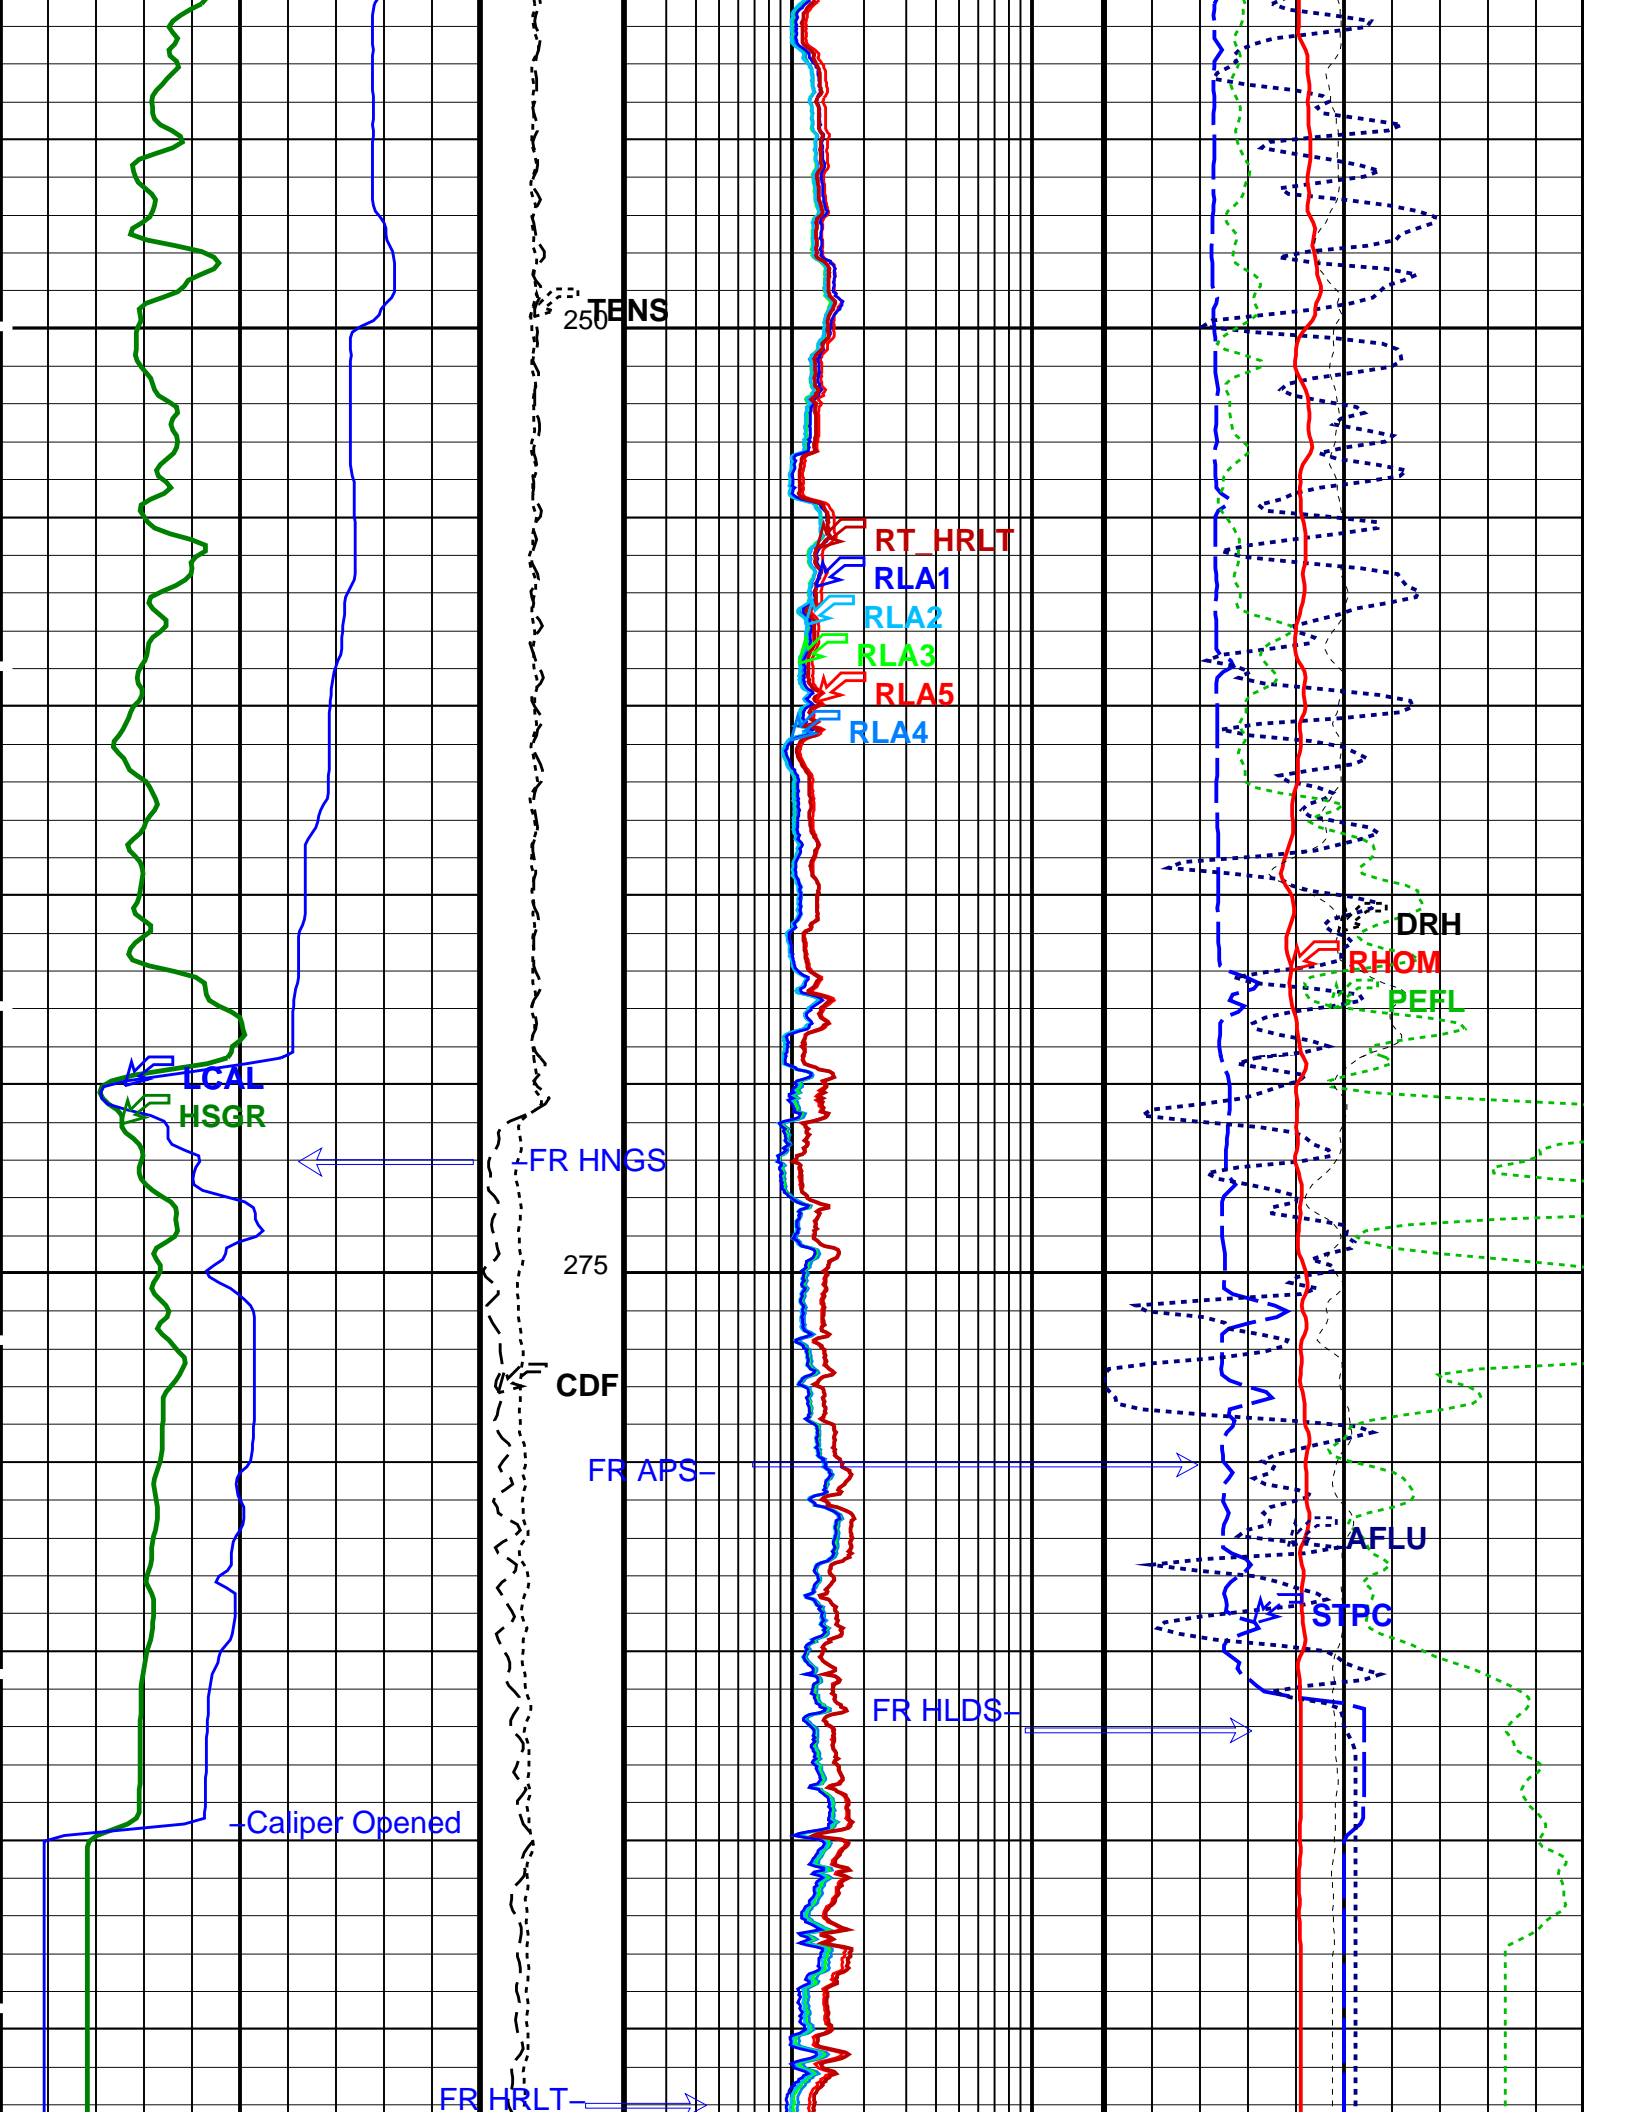

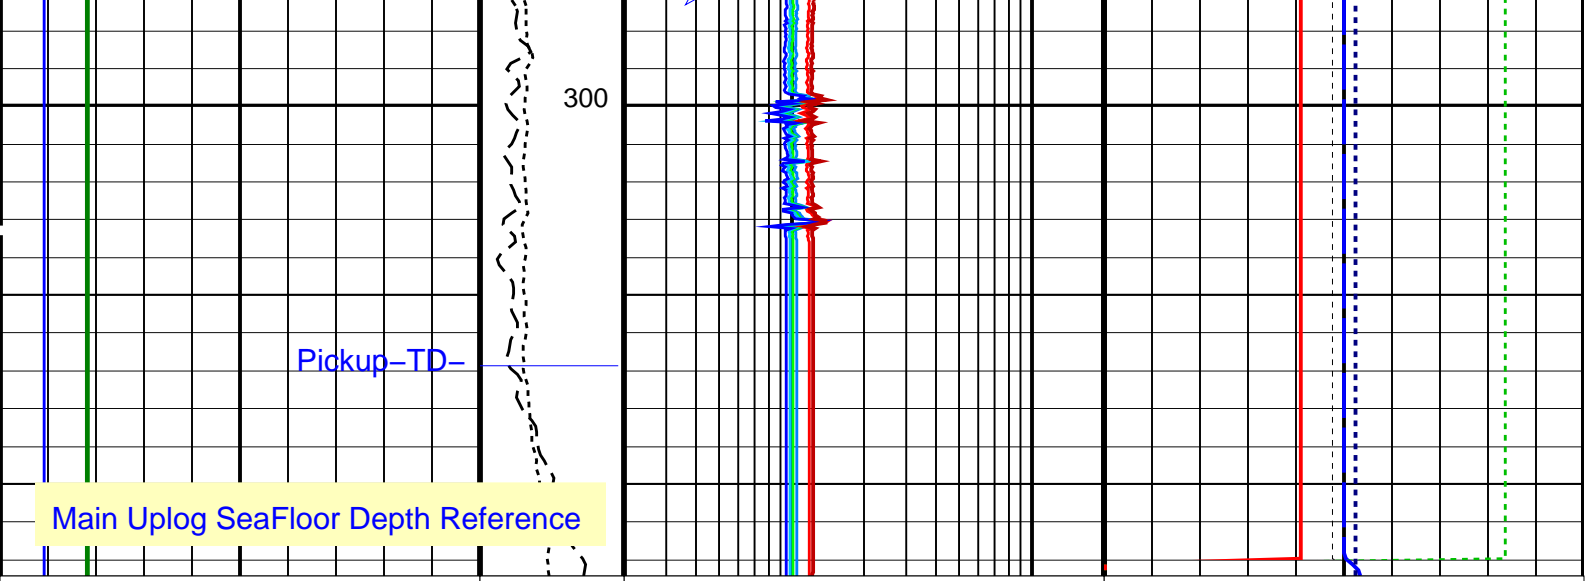

HLDS Caliper (LCAL) (IN)	Tension (TENS) (LBF)	HRLT Resistivity 4 (RLA4) (OHMM)	APS Corrected Standoff Porosity (STPC) (PU)
0 20	10000 0	0.2 20	100 0
HNGS Spectroscopy Gamma Ray (HSGR) (GAPI)	Calibrated Downhole Force (CDF) (LBF)	HRLT Resistivity 5 (RLA5) (OHMM)	APS Array to Far Porosity (AFLU) (PU)
0 100	3000 0	0.2 20	100 0
		HRLT Resistivity 3 (RLA3) (OHMM)	HLDS Bulk Density (RHOM) (G/C3)
		0.2 20	0 4
		HRLT Resistivity 2 (RLA2) (OHMM)	HLDS Long Spaced Photoelectric Effect (PEFL) (----)
		0.2 20	0 10
		HRLT Resistivity 1 (RLA1) (OHMM)	HLDS Bulk Density Correction (DRH) (G/C3)
		0.2 20	-0.25 0.25
		HRLT True Resistivity (RT_HRLT) (OHMM)	
		0.2 20	

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value
HRLT-B: High Resolution Laterolog Array - B		
BHS	Borehole Status	OPEN
BHT	Bottom Hole Temperature (used in calculations)	21 DEGC
CALSTAT	HRLTB Calibration Status	SHALLOW_DONE
CALTEMP	HRLTB Calibration Temperature	18.9924 DEGC
FREQ0	HRLT Frequency Index for Mode 0	32
FREQ1	HRLT Frequency Index for Mode 1	128
FREQ2	HRLT Frequency Index for Mode 2	104
FREQ3	HRLT Frequency Index for Mode 3	86
FREQ4	HRLT Frequency Index for Mode 4	56
FREQ5	HRLT Frequency Index for Mode 5	44
FREQ6	HRLT Frequency Index for Mode 6	116
GCSE	Generalized Caliper Selection	LCAL
GDEV	Average Angular Deviation of Borehole from Normal	0 DEG
GGRD	Geothermal Gradient	0.018227 DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE
ISSBAR	Barite Mud Switch	BARITE
KFAC_HRLT	HRLT K Factor Option	SONDE
LOOPCOEF_S	HRLT Loop Coefficient for Shallow Modes	LOW
LOOPMOD0	HRLT Mode 0 Loop Mode	AUTO
LOOPMOD1	HRLT Mode 1 Loop Mode	AUTO
LOOPMOD2	HRLT Mode 2 Loop Mode	AUTO
LOOPMOD3	HRLT Mode 3 Loop Mode	AUTO

LOOPMOD4	HRLT Mode 4 Loop Mode	AUTO	
LOOPMOD5	HRLT Mode 5 Loop Mode	AUTO	
LOOPMOD6	HRLT Mode 6 Loop Mode	AUTO	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
PROCINV	Inversion Selection	ON	
PROCMFL	Inversion Micro-Resistivity Selection	NO_EXTERNAL_RXO	
PROCMSO	Mechanical Standoff Fin Size	0	IN
PROCRM	Processing Mud Resistivity Select	HRLT_Compute	
PROCSPO	Sonde Position	Centered	
SHT	Surface Hole Temperature	20	DEGC
HLDS: Hostile Litho-Density Sonde			
CLCL	HLDS LS Control Loop Controller Mode	AUTO_DEFAULT	
CLCS	HLDS SS Control Loop Controller Mode	AUTO_DEFAULT	
CLLS	HLDS Mode Loop Long Spacing	AUTO	
CLSS	HLDS Mode Loop Short Spacing	AUTO	
DHC	Density Hole Correction	BS	
DPPM	Density Porosity Processing Mode	HIRS	
FD	Fluid Density	1	G/C3
LATC	HLDS Activation Correction	ON	
LLDL	HLDS LS Low Level Discriminator DAC	14000	
LLDS	HLDS SS Low Level Discriminator DAC	14000	
LLML	HLDS LS Low Level Discriminator Mode	AUTO	
LLMS	HLDS SS Low Level Discriminator Mode	AUTO	
MDEN	Matrix Density	2.6	G/C3
PHVL	HLDS Long Spacing High Voltage Setting	1000	V
PHVS	HLDS Short Spacing High Voltage Setting	1000	V
PSDL	HLDS LS Pulse Shape Compensation DAC	30000	
PSDS	HLDS SS Pulse Shape Compensation DAC	30000	
PSML	HLDS LS Pulse Shape Compensation Mode	AUTO	
PSMS	HLDS SS Pulse Shape Compensation Mode	AUTO	
APS-C: Accelerator-Porosity Tool			
	APS Software Version	0	
AASD	APS Thermal and Array Detectors High Voltage Setting	1939.6	V
ADSO	APS Array Detectors Data Source Switch	Both	
AFSD	APS Far Detector High Voltage Setting	2029.77	V
AHCS	APS Holesize Correction Source	GCSE	
AHSS	APS Holesize Correction Switch	ON	
AMTY	APS Environmental Corrections Mud Type	WaterBaseBarite	
ANSD	APS Near Detector High Voltage Setting	1697.47	V
ASOS	APS Standoff Correction Switch	ON	
ATSS	APS Temperature-Pressure-Salinity Correction Switch	ON	
BHFL_APS	APS TNPH Borehole Fluid Type	WATER	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
BSCO_APS	APS TNPH Borehole Salinity Correction Option	NO	
DPPM	Density Porosity Processing Mode	HIRS	
DSCO_APS	APS TNPH Density Source Correction Option	MEASURED	
FSAL	Formation Salinity	-50000	PPM
FSCO_APS	APS TNPH Formation Salinity Correction Option	NO	
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
HSCO_APS	APS TNPH Hole Size Correction Option	YES	
ISSBAR	Barite Mud Switch	BARITE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
MCCO_APS	APS TNPH Mud Cake Correction Option	NO	
MCOR_APS	APS TNPH Mud Correction	BARI	
MWCO_APS	APS TNPH Mud Weight Correction Option	YES	
NARC	APS Near/Array Calibration Ratio	1.08449	
NFRC	APS Near/Far Calibration Ratio	0.976579	
PTCO_APS	APS TNPH Pressure/Temperature Correction Option	NO	
SHT	Surface Hole Temperature	20	DEGC
TNCO_APS	APS TNPH Computation Option	YES	
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.000822794	
HALE	HNGS Alpha Filter Length	60	IN

HCRB	HNGS Alpha Filter Length	00	IN
HMWM	Mud Weighting Material	NONE	BARI
HNPE	HNGS Processing Enable	YES	YES
ISSBAR	Barite Mud Switch	BARITE	BARITE
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	LIMESTONE
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	YES
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	CENT	CENT
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	-4.27844	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	1.8508	
EDTC-B: Enhanced DTS Cartridge			
BHFL	Borehole Fluid Type	WATER	WATER
BHS	Borehole Status	OPEN	OPEN
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
BSCO	Borehole Salinity Correction Option	NO	NO
CCCO	Casing & Cement Thickness Correction Option	NO	NO
DPPM	Density Porosity Processing Mode	HIRS	HIRS
FSAL	Formation Salinity	-50000	PPM
FSCO	Formation Salinity Correction Option	NO	NO
GCSE	Generalized Caliper Selection	LCAL	LCAL
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	CHART_GEN_9
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	LINEAR_ESTIMATE
HSCO	Hole Size Correction Option	YES	YES
ISSBAR	Barite Mud Switch	BARITE	BARITE
ISSBAR_EDTC	Nuclear Mud Type	BARITE	BARITE
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	LIMESTONE
MCCO	Mud Cake Correction Option	NO	NO
MCOR	Mud Correction	BARI	BARI
MWCO	Mud Weight Correction Option	YES	YES
PTCO	Pressure/Temperature Correction Option	NO	NO
SDAT	Standoff Data Source	SOCN	SOCN
SHT	Surface Hole Temperature	20	DEGC
SOCN	Standoff Distance	0.5	IN
SOCO	Standoff Correction Option	NO	NO
TPOS_EDTC	EDTC Tool Centered/Eccentered	Eccentered	Eccentered
U-ETELM_EDTS	Telemetry Mode for eWAFE	Standard_EDTS	Standard_EDTS
U-TELM_EDTS	Telemetry Mode for WAFE	Standard_EDTS	Standard_EDTS
System and Miscellaneous			
ALTDPCCHAN	Name of alternate depth channel	SpeedCorrectedDepth	SpeedCorrectedDepth
BS	Bit Size	9.875	IN
BSAL	Borehole Salinity	-50000.00	PPM
CSIZ	Current Casing Size	5.500	IN
CWEI	Casing Weight	168.00	LB/F
DFD	Drilling Fluid Density	1.32	G/C3
DO	Depth Offset for Playback	-4717.0	M
FLEV	Fluid Level	-50000.00	M
MST	Mud Sample Temperature	-50000.00	DEGC
PBVSADP	Use alternate depth channel for playback	NO	NO
PP	Playback Processing	NORMAL	NORMAL
RMFS	Resistivity of Mud Filtrate Sample	-50000.0000	OHMM
RW	Resistivity of Connate Water	1.0000	OHMM
TD	Total Depth	4909	M
TDD	Total Depth - Driller	5612.00	M
TDL	Total Depth - Logger	5612.00	M
TWS	Temperature of Connate Water Sample	37.78	DEGC

Format: TripleCombo Vertical Scale: 1:200 Graphics File Created: 20-Jun-2014 18:21

OP System Version: 19C0-187

MSS_LDEO-A	19C0-187	HRLT-B	19C0-187
HLDS	19C0-187	LDSC-B	19C0-187
APS-C	19C0-187	HNGC-B	19C0-187
HNGS-BA	19C0-187	EDTC-B	SKK-5169-EDTCB

Input DLIS Files

DEFAULT	MSS_LDEO_HRLA_LDL_018LUP	FN:26	PRODUCER	19-Jun-2014 00:41	5029.2 M	4689.2 M
---------	--------------------------	-------	----------	-------------------	----------	----------

Output DLIS Files

DEFAULT	MSS_LDEO_HRLA_LDL_033PUP	FN:46	PRODUCER	20-Jun-2014 18:21		
---------	--------------------------	-------	----------	-------------------	--	--

Input DLIS Files

Input DLIS Files

DEFAULT Flip_MSS_LDEO_HRLA_029PUP PRODUCER 20-Jun-2014 18:03 274.2 M -93.7 M

Output DLIS Files

DEFAULT MSS_LDEO_HRLA_LDL_030PUP FN:43 PRODUCER 20-Jun-2014 18:06 274.2 M -93.7 M


OP System Version: 19C0-187


MSS_LDEO-A	19C0-187	HRLT-B	19C0-187
HLDS	19C0-187	LDSC-B	19C0-187
APS-C	19C0-187	HNGC-B	19C0-187
HNGS-BA	19C0-187	EDTC-B	SKK-5169-EDTCB


PIP SUMMARY


Time Mark Every 60 S


<p style="background-color: yellow; padding: 2px;">Caliper Closed on Downlog</p> <p style="background-color: yellow; padding: 2px;">Flipped Downlog</p>		<p>HRLT True Resistivity (RT_HRLT)</p> <p>0.2 (OHMM) 20</p>	
		<p>HRLT Resistivity 1 (RLA1)</p> <p>0.2 (OHMM) 20</p>	
		<p>HRLT Resistivity 2 (RLA2)</p> <p>0.2 (OHMM) 20</p>	<p>HLDS Bulk Density Correction (DRH)</p> <p>-0.25 (G/C3) 0.25</p>
		<p>HRLT Resistivity 3 (RLA3)</p> <p>0.2 (OHMM) 20</p>	<p>HLDS Bulk Density (RHOM)</p> <p>0 (G/C3) 4</p>
	<p>HNGS Spectroscopy Gamma Ray (HSGR)</p> <p>0 (GAPI) 100</p>	<p>Calibrated Downhole Force (CDF) (LBF)</p> <p>3000 0</p>	<p>HRLT Resistivity 5 (RLA5)</p> <p>0.2 (OHMM) 20</p>
<p>HLDS Caliper (LCAL)</p> <p>0 (IN) 20</p>	<p>Tension (TENS) (LBF)</p> <p>10000 0</p>	<p>HRLT Resistivity 4 (RLA4)</p> <p>0.2 (OHMM) 20</p>	<p>APS Corrected Standoff Porosity (STPC)</p> <p>100 (PU) 0</p>

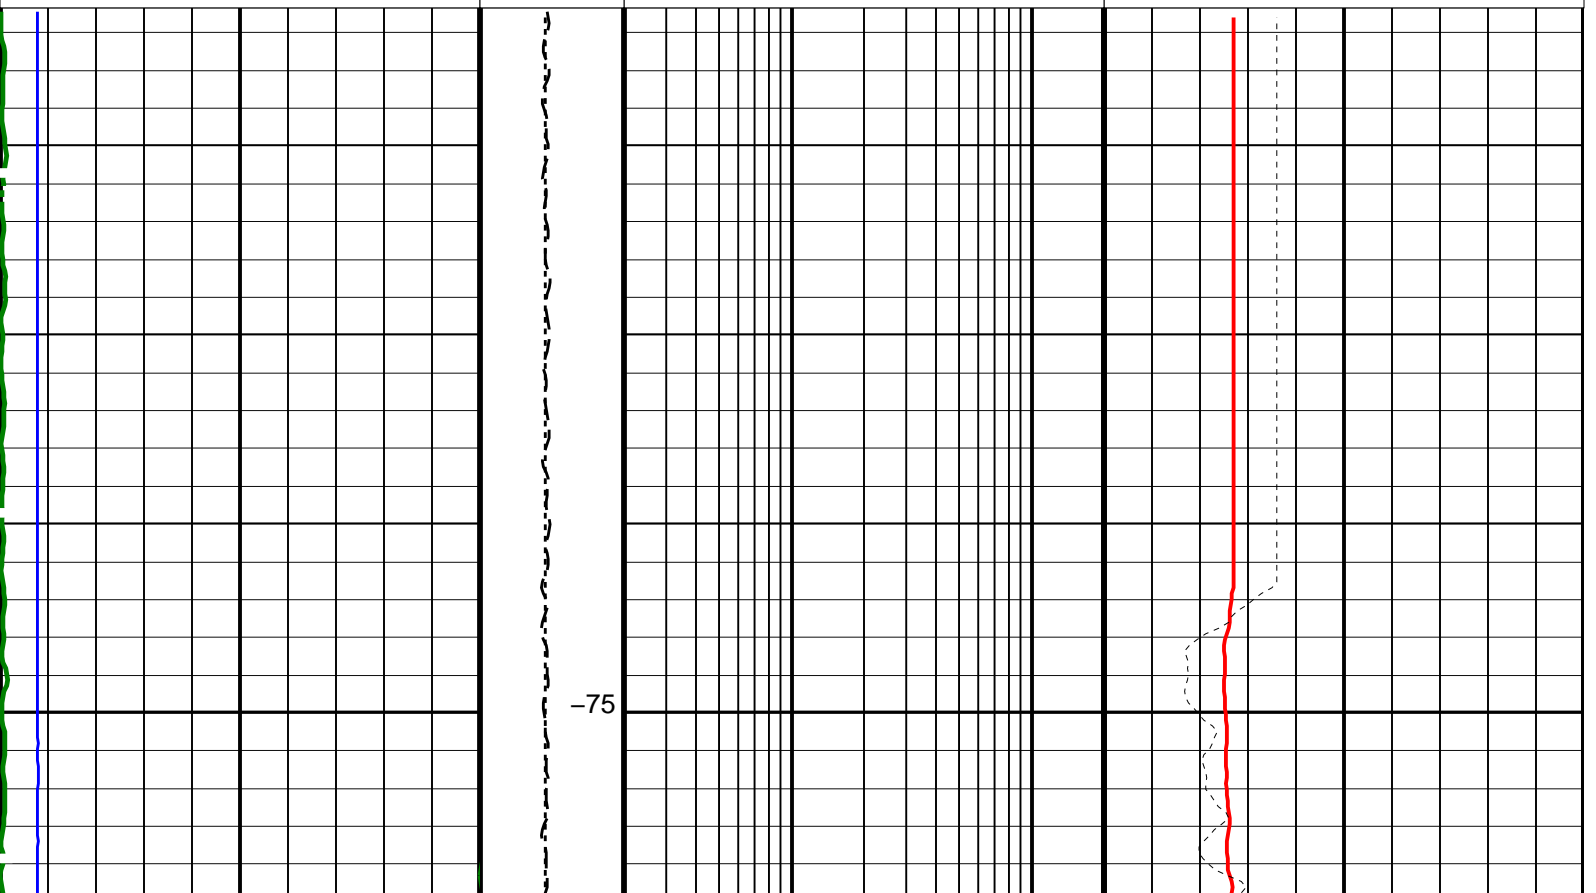


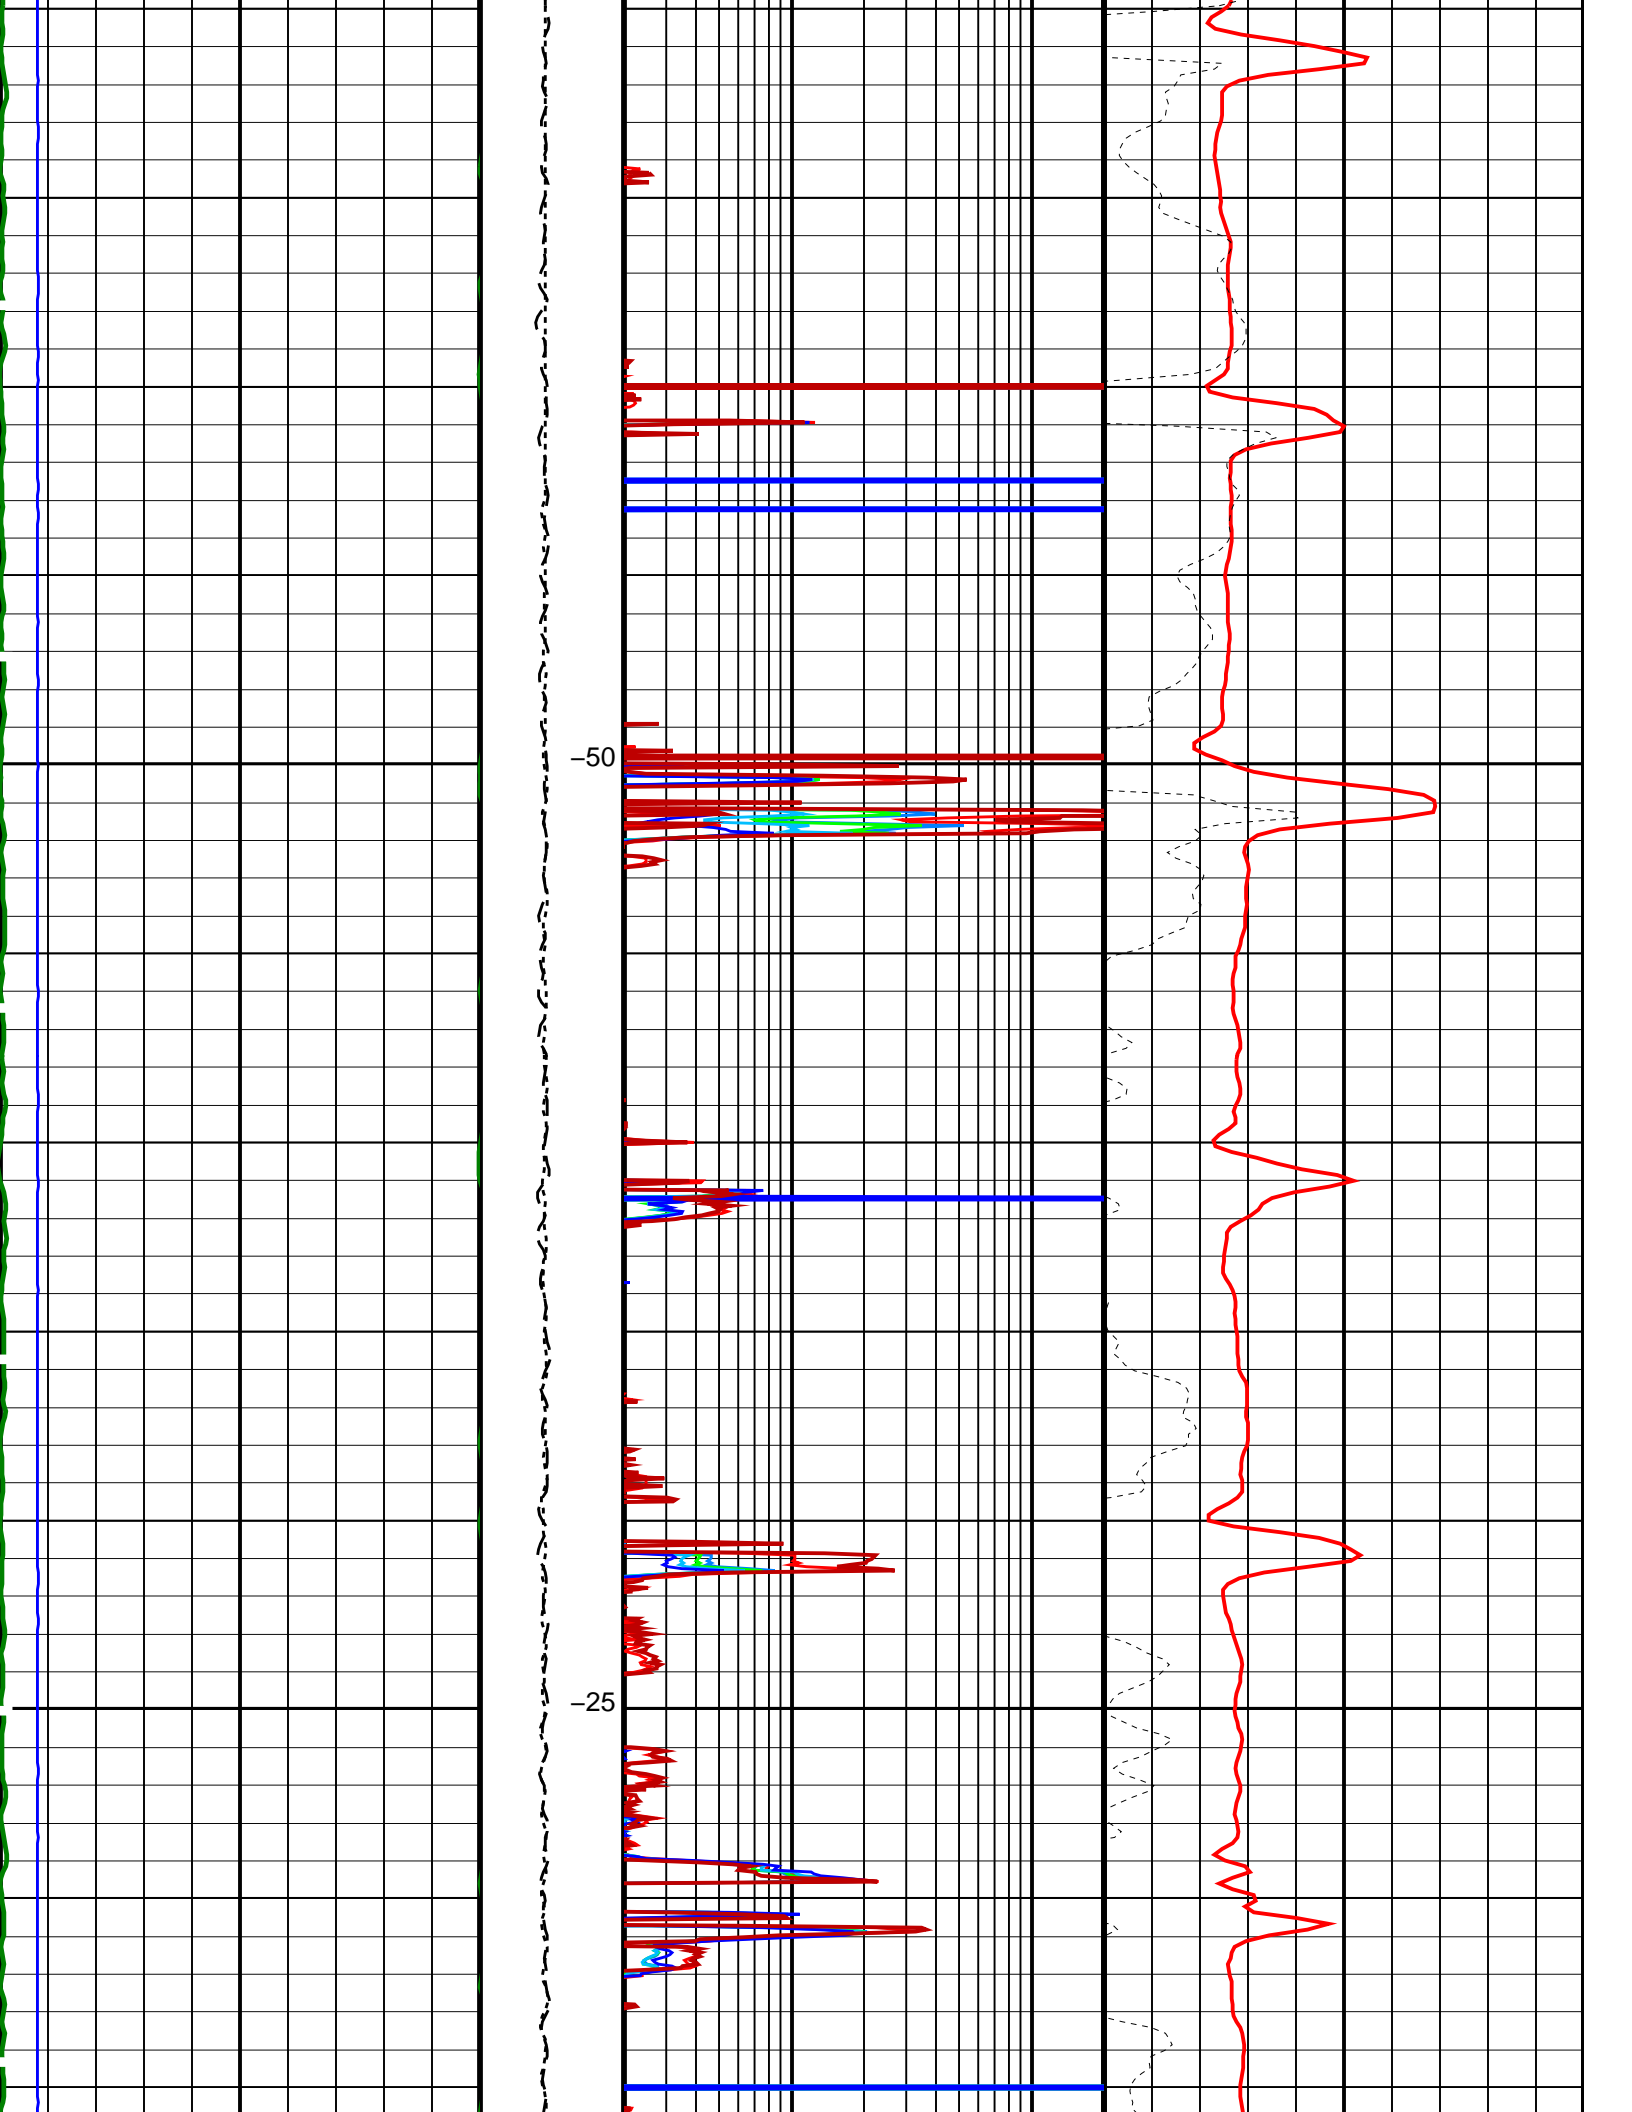


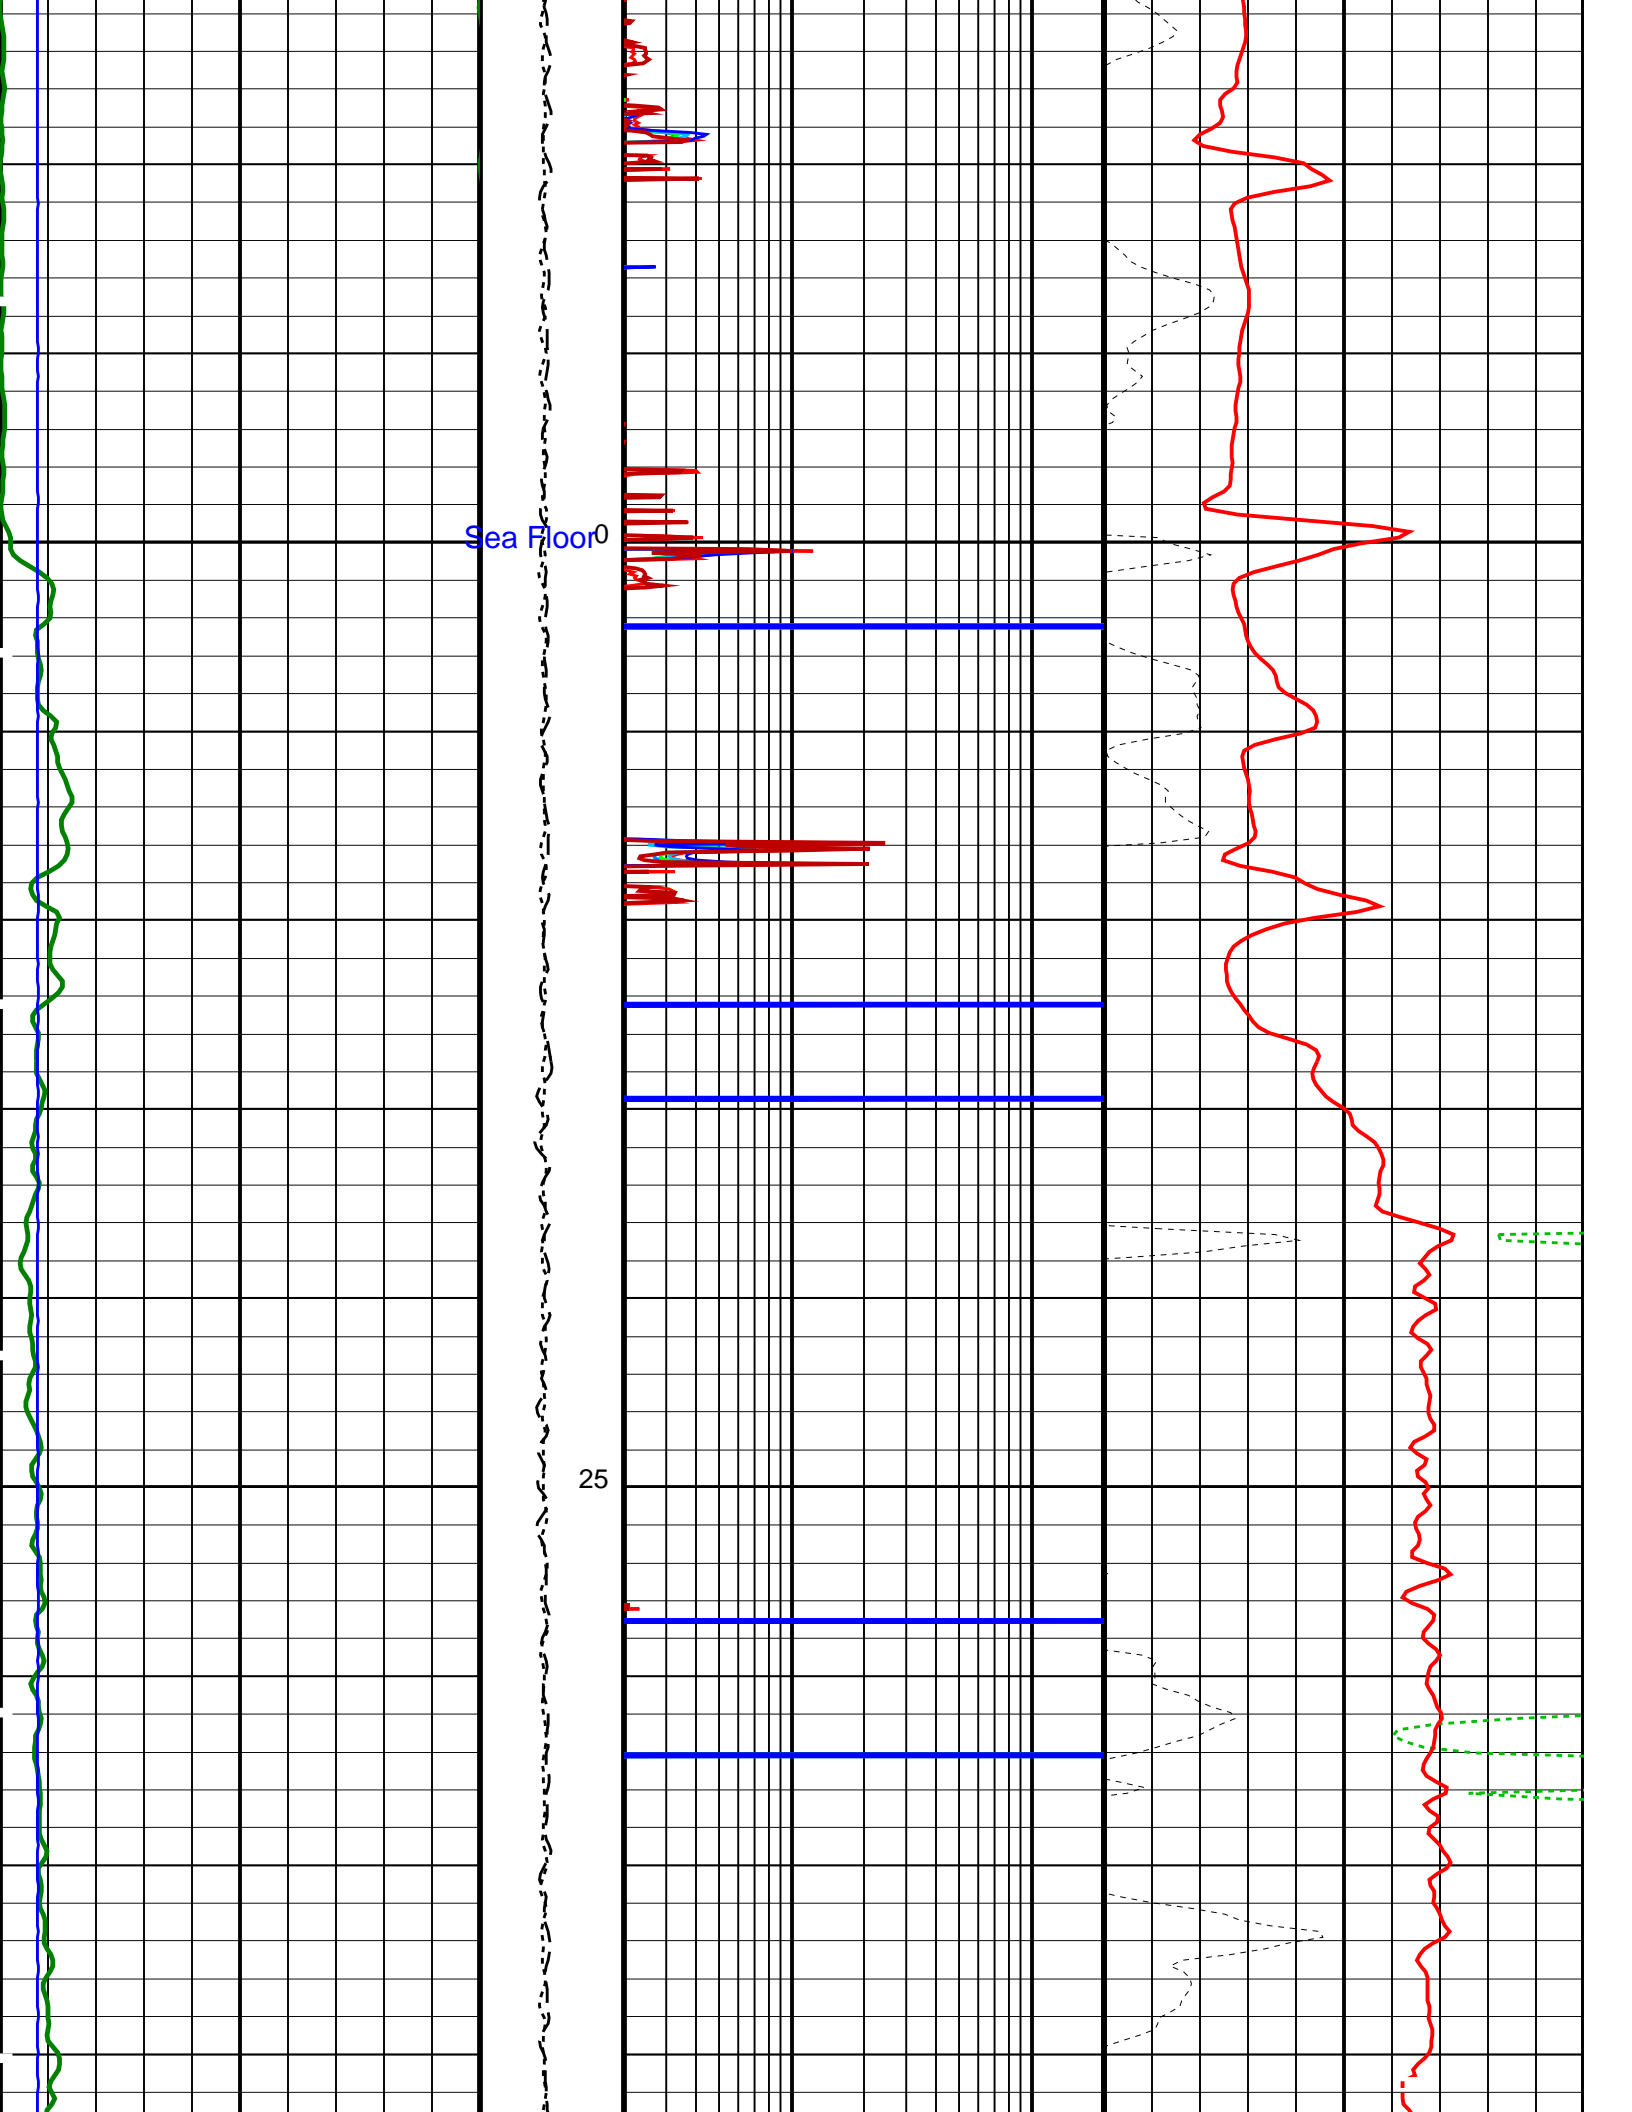


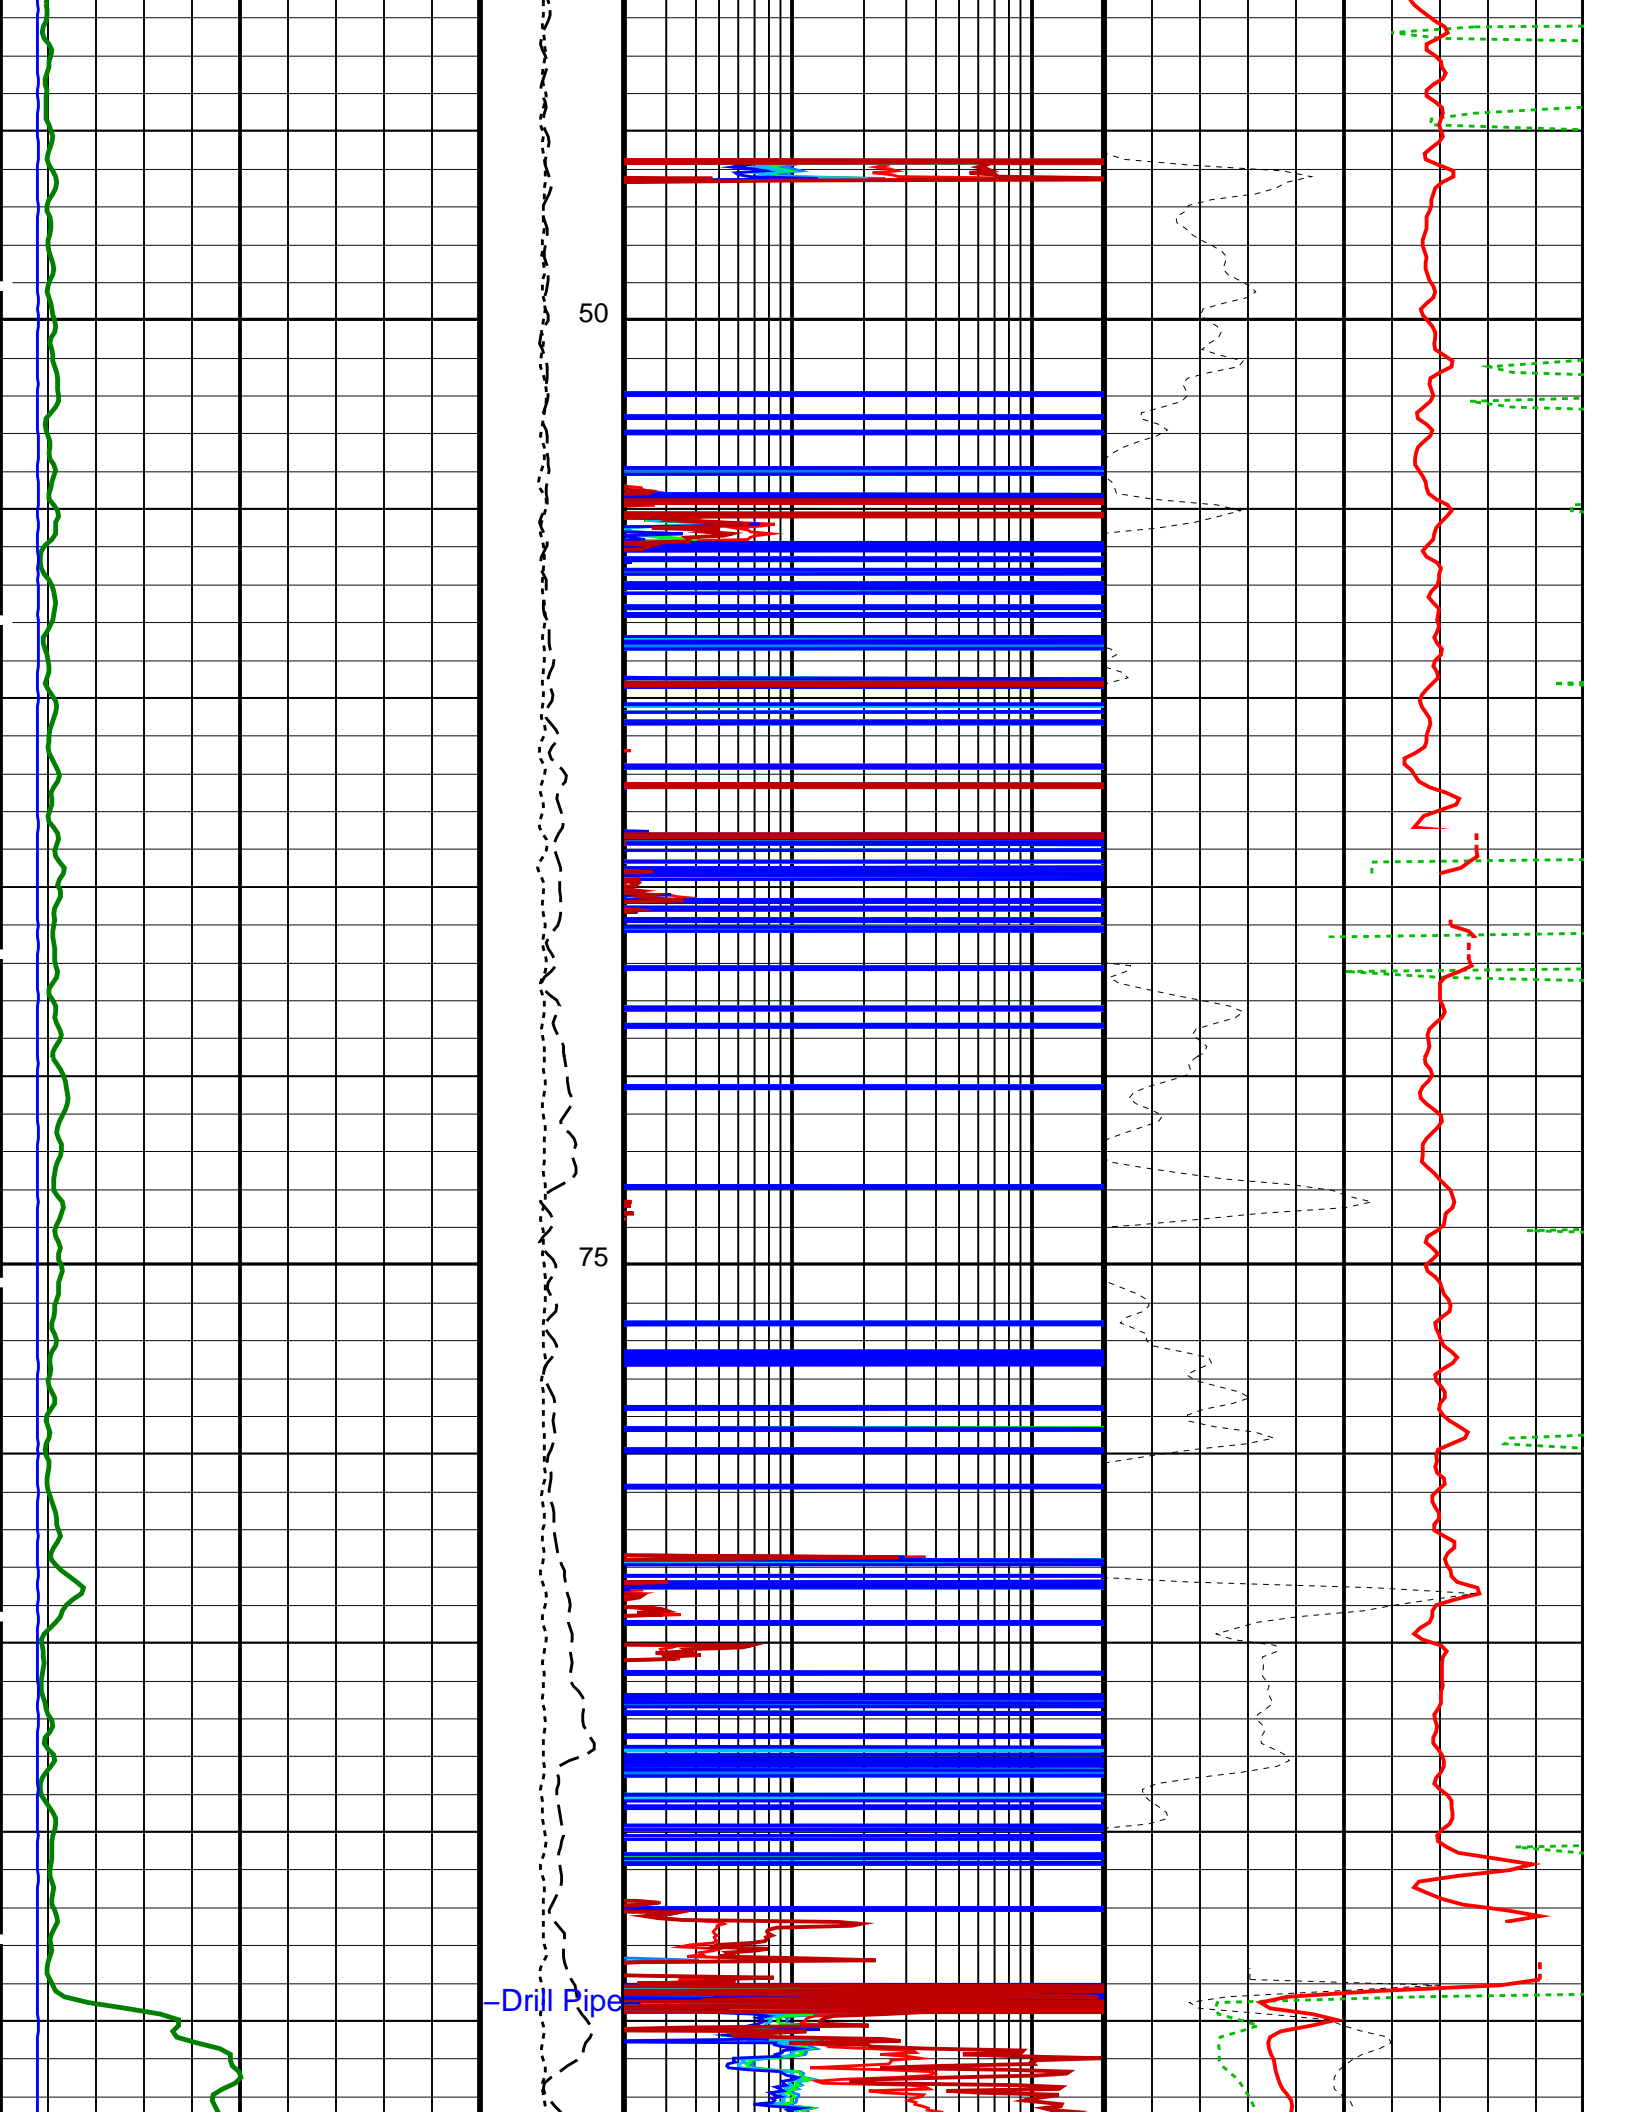

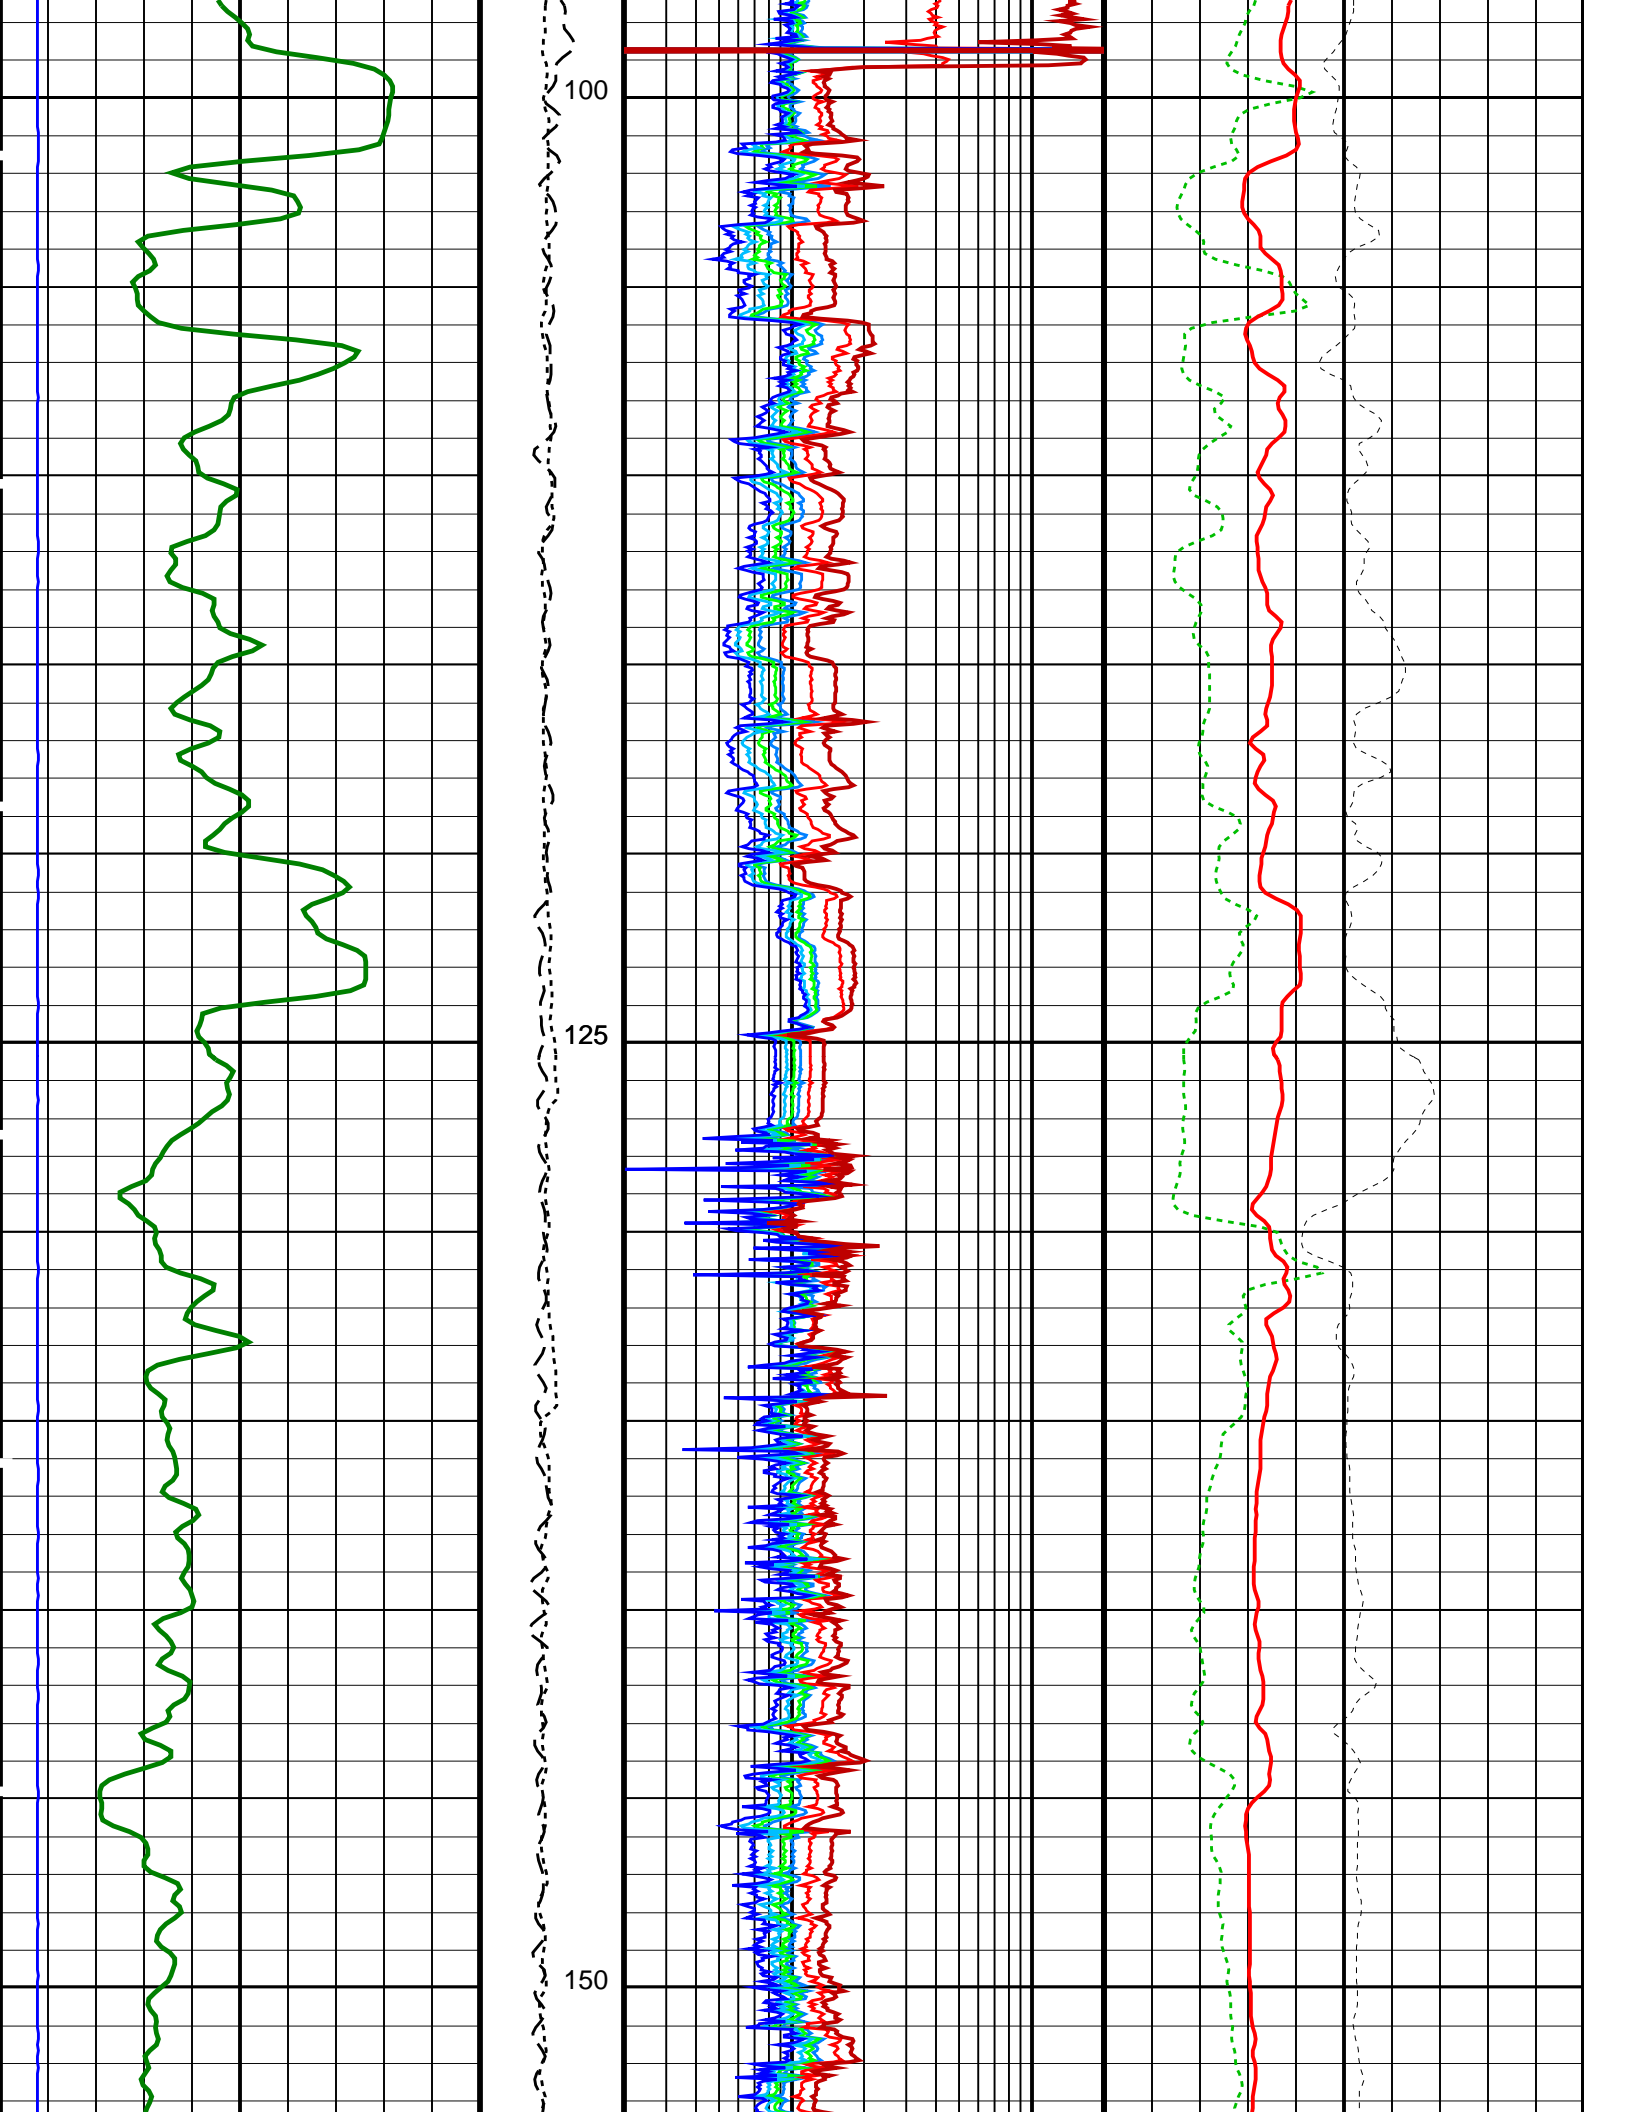

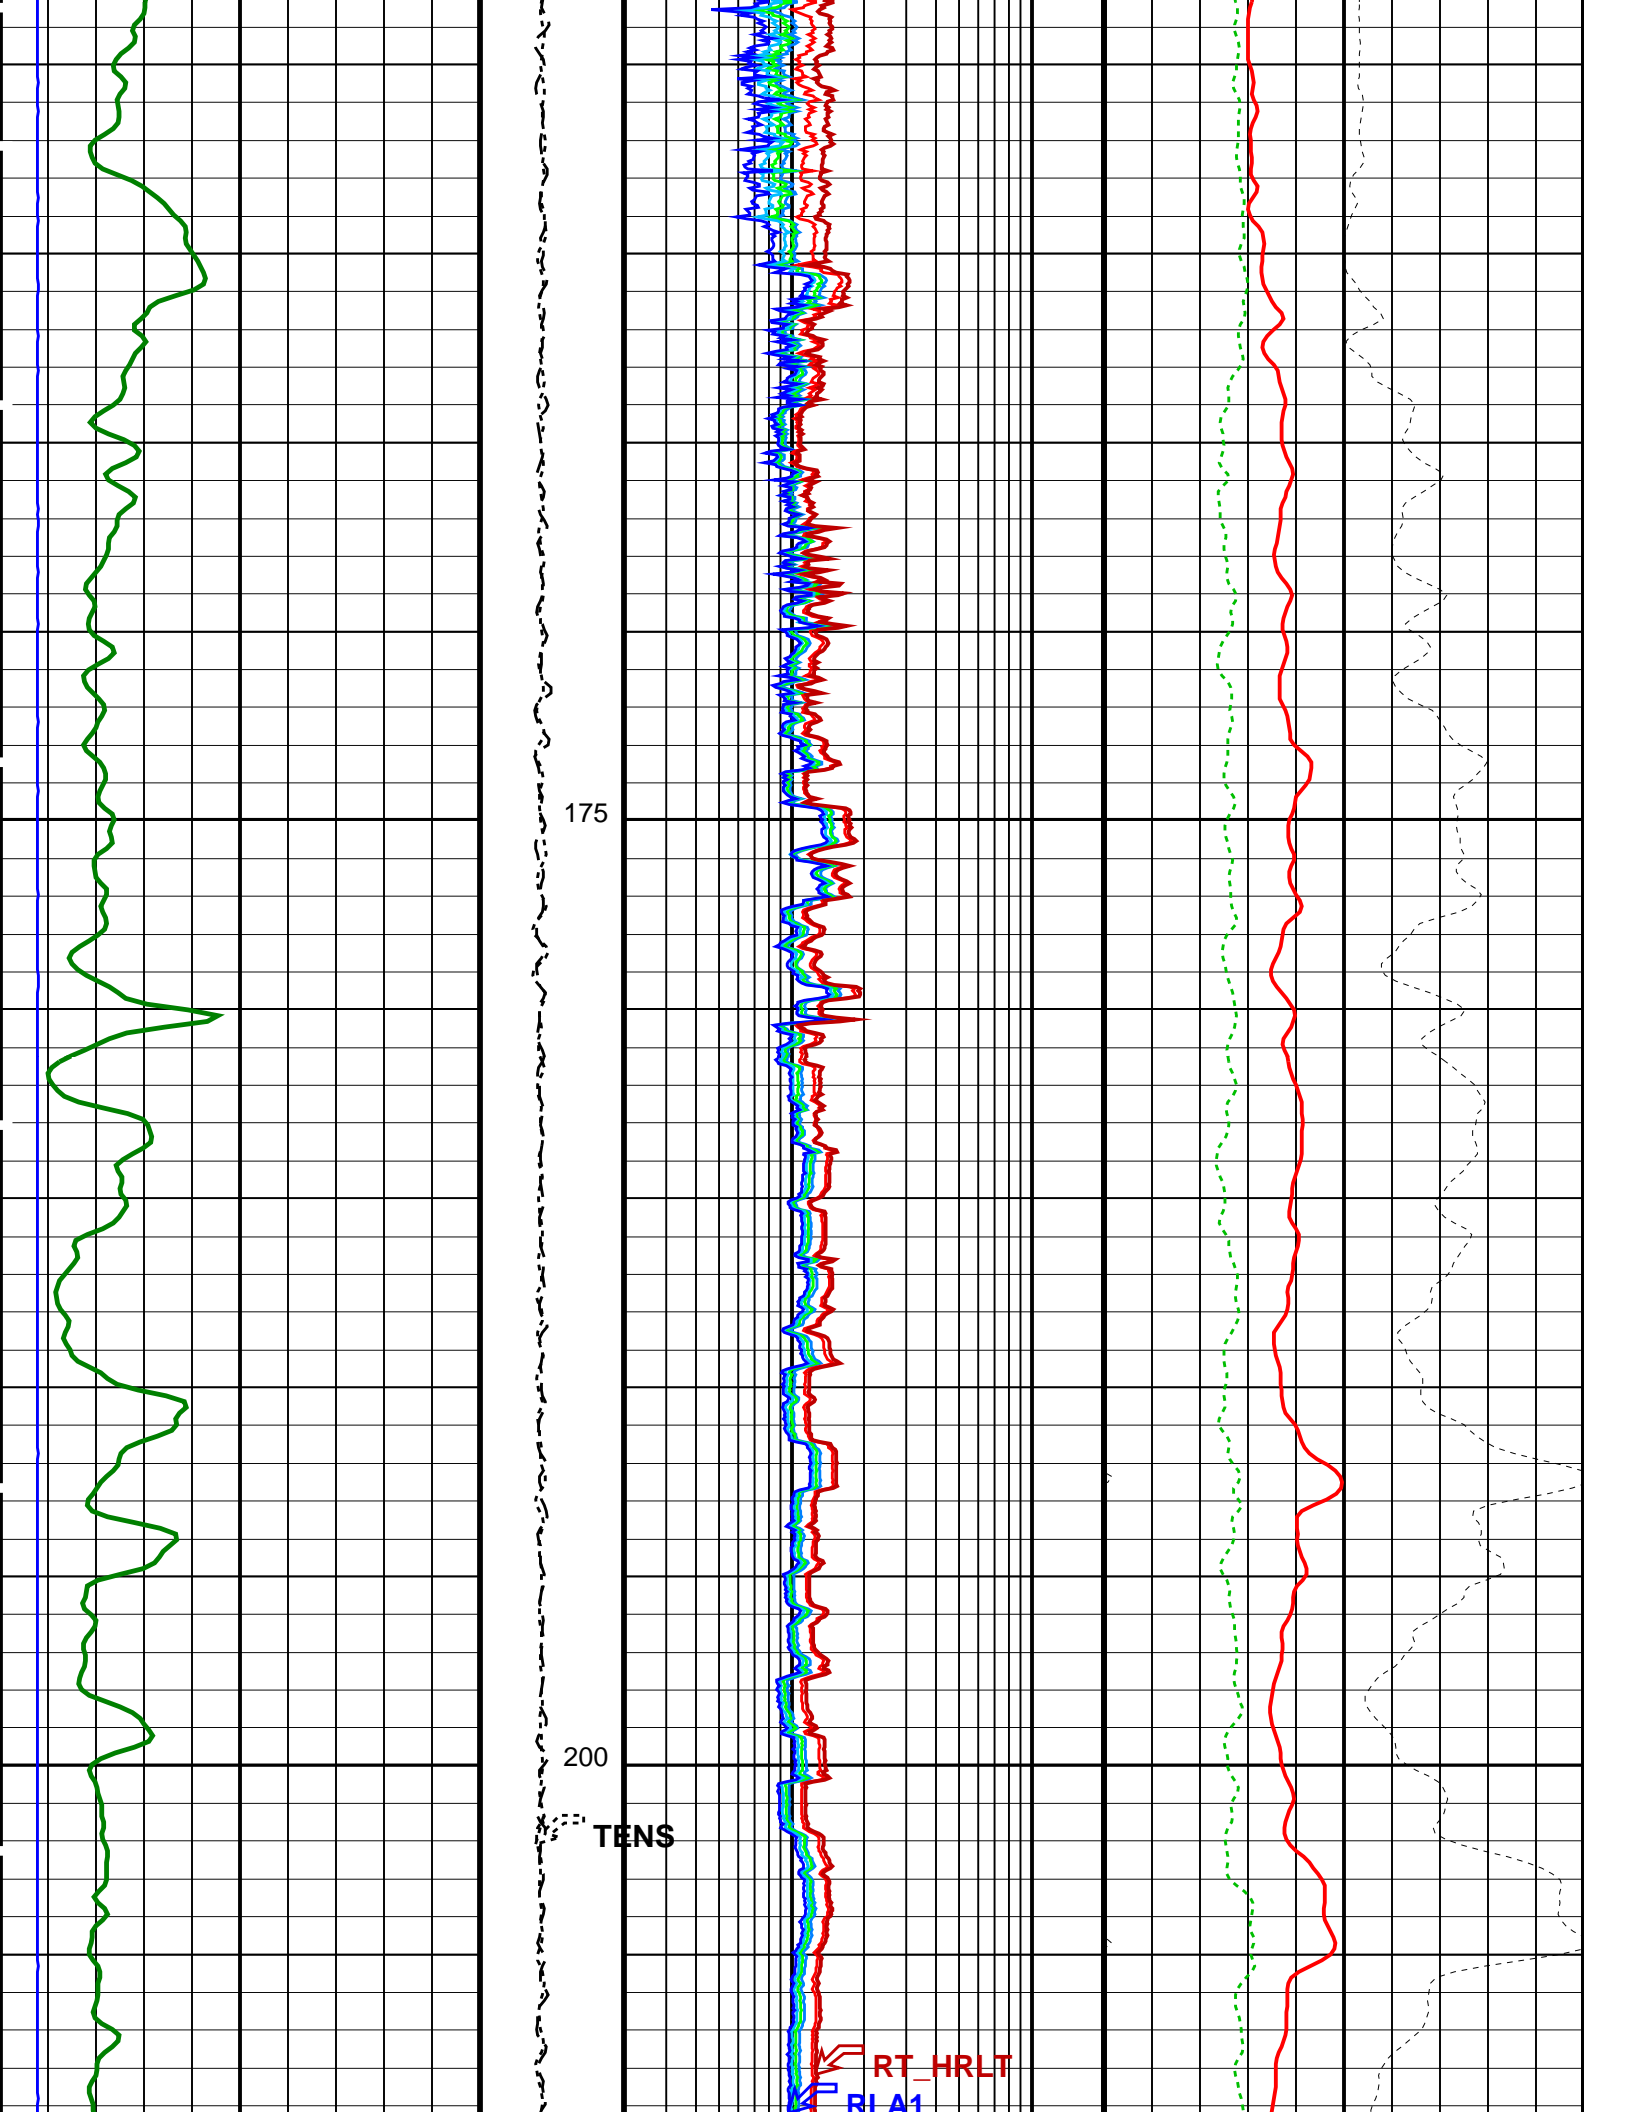

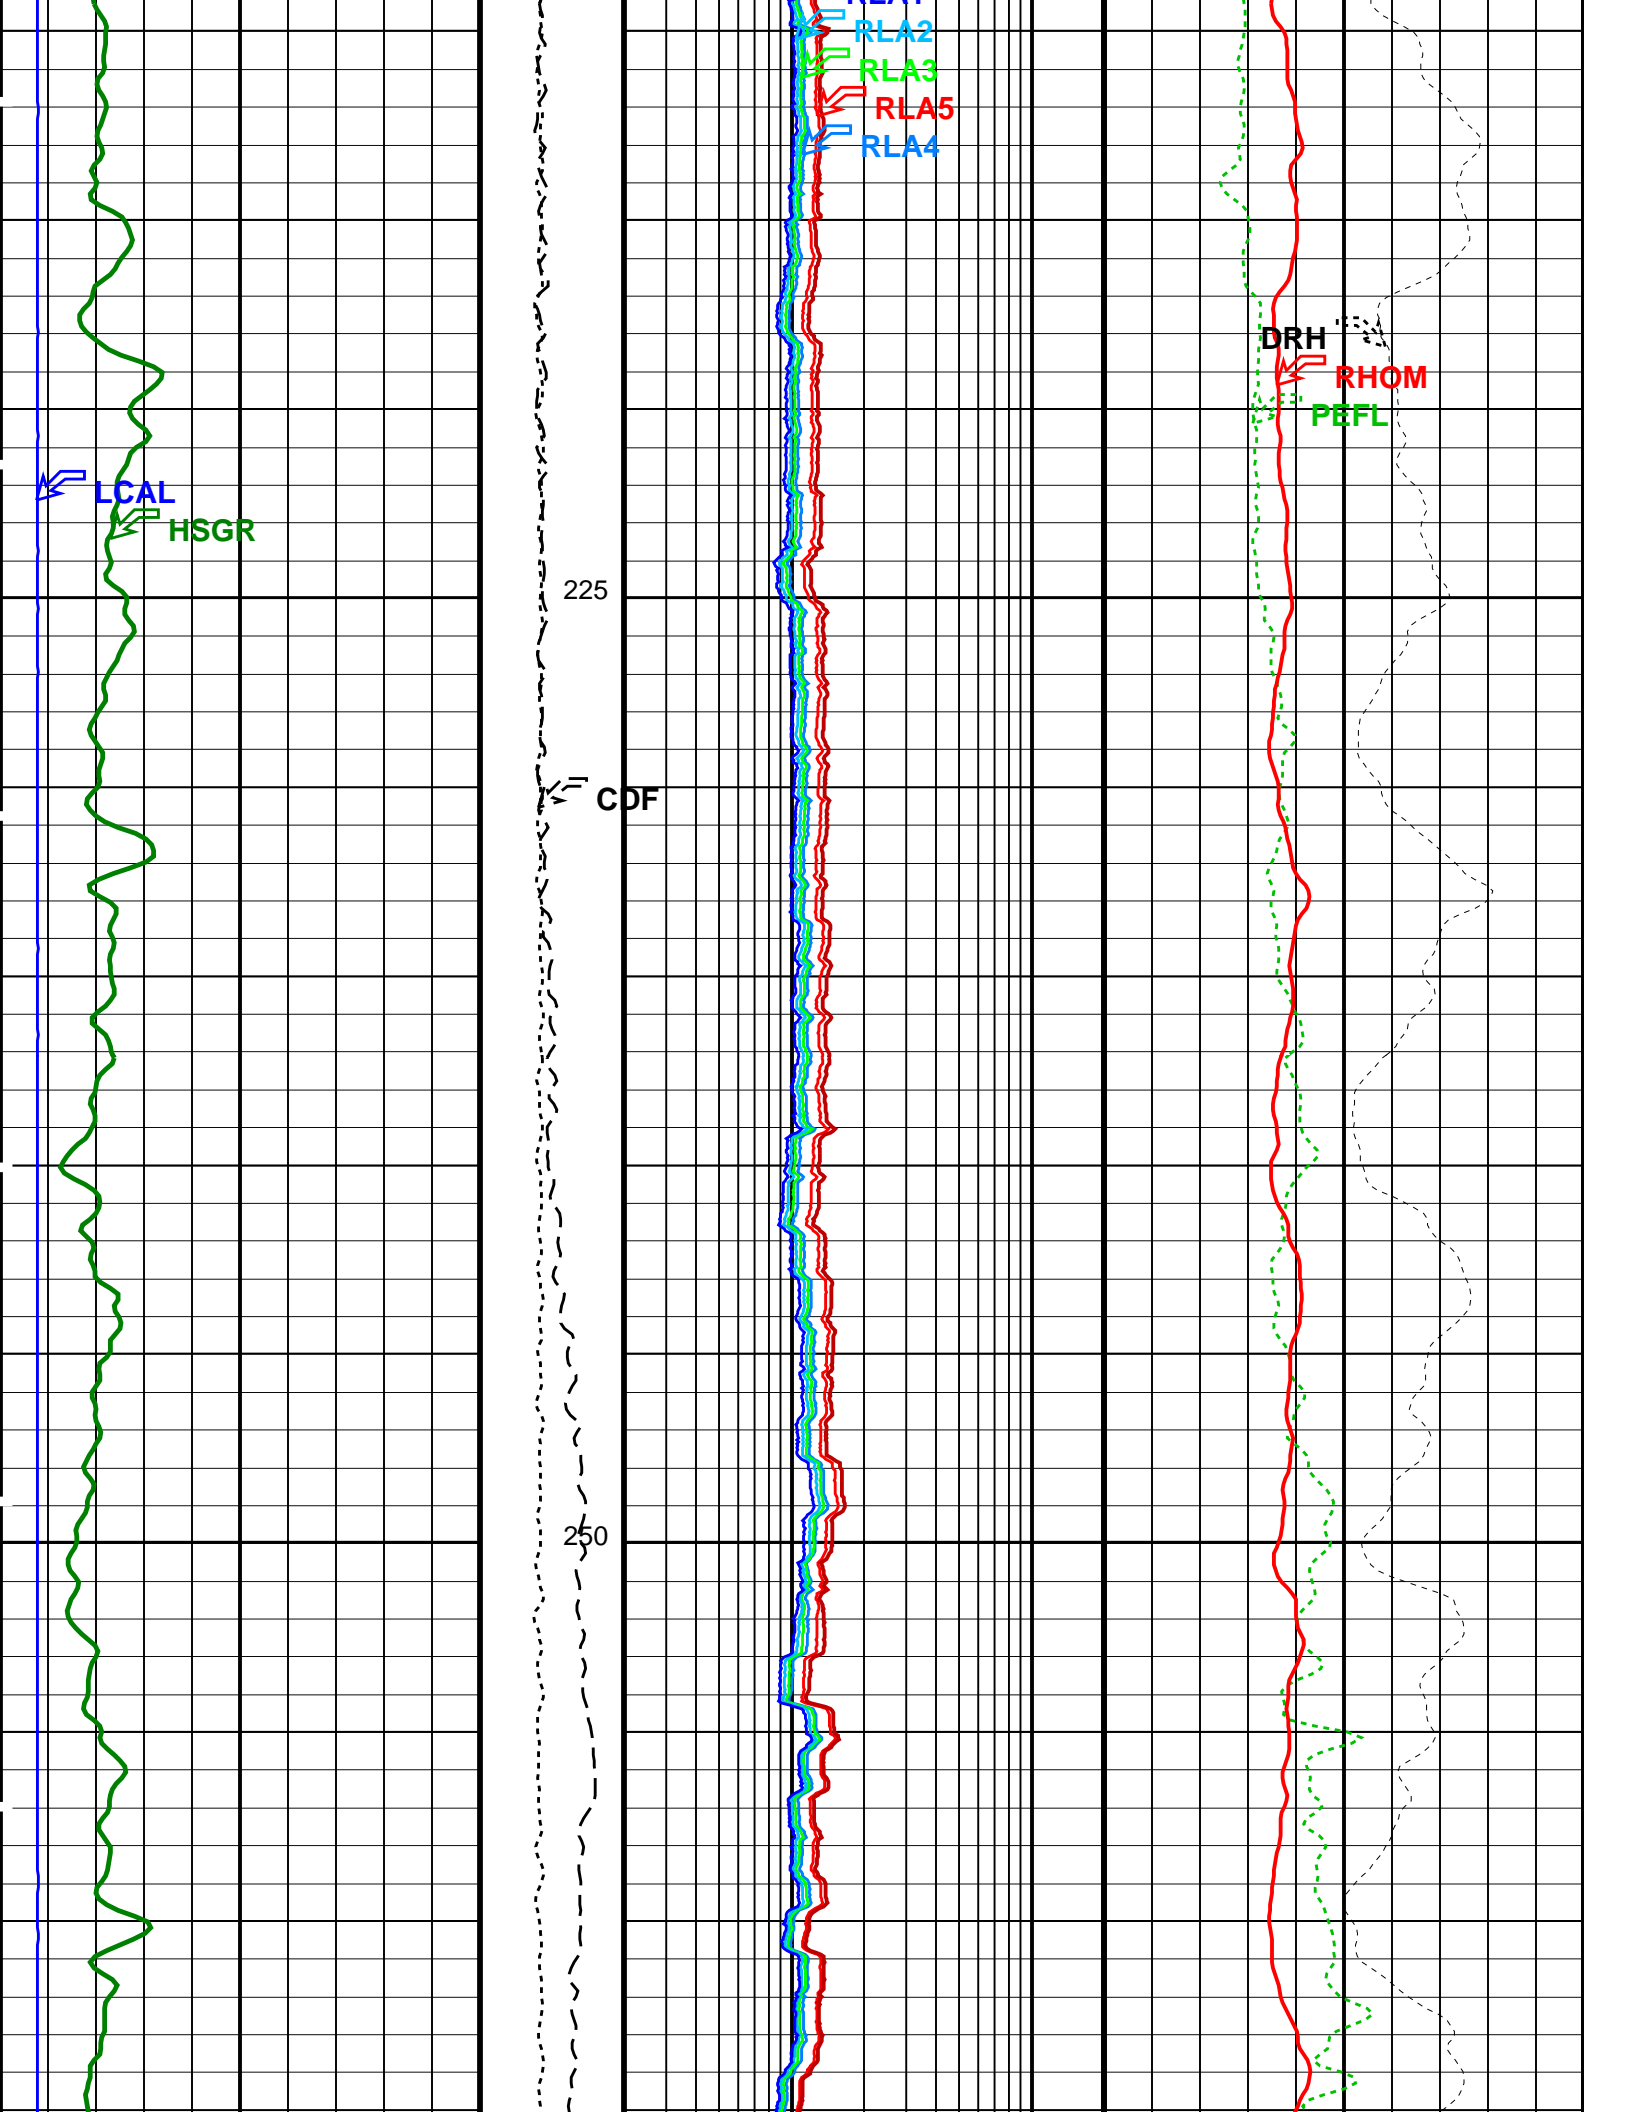

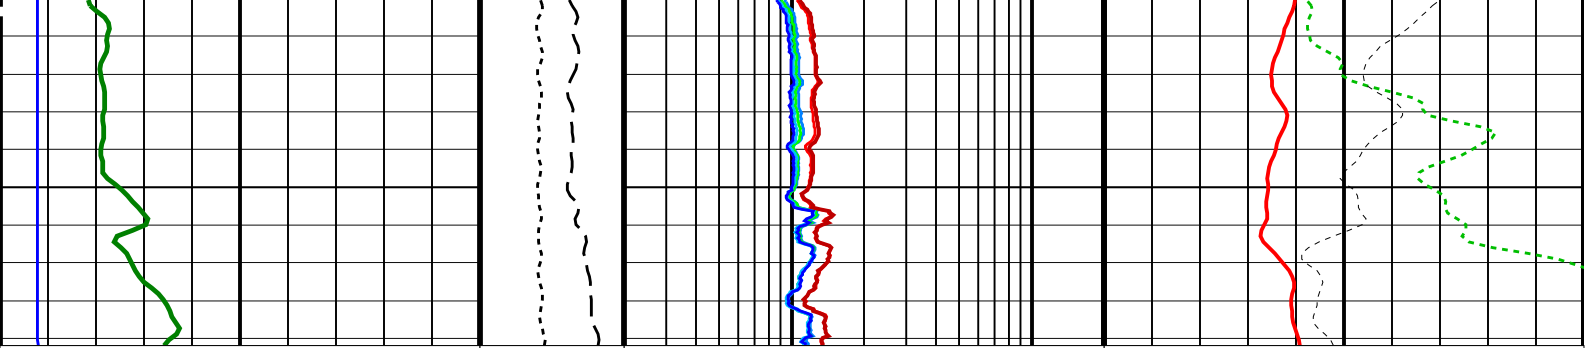

HLDS Caliper (LCAL) 0 (IN) 20	Tension (TENS) (LBF) 10000 0	HRLT Resistivity 4 (RLA4) 0.2 (OHMM) 20	APS Corrected Standoff Porosity (STPC) 100 (PU) 0
HNGS Spectroscopy Gamma Ray (HSGR) 0 (GAPI) 100	Calibrated Downhole Force (CDF) (LBF) 3000 0	HRLT Resistivity 5 (RLA5) 0.2 (OHMM) 20	HLDS Long Spaced Photoelectric Effect (PEFL) 0 (----) 10
Flipped Downlog Caliper Closed on Downlog	HRLT Resistivity 3 (RLA3) 0.2 (OHMM) 20	HLDS Bulk Density (RHOM) 0 (G/C3) 4	
	HRLT Resistivity 2 (RLA2) 0.2 (OHMM) 20	HLDS Bulk Density Correction (DRH) -0.25 (G/C3) 0.25	
	HRLT Resistivity 1 (RLA1) 0.2 (OHMM) 20		
	HRLT True Resistivity (RT_HRLT) 0.2 (OHMM) 20		

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value	
HRLT-B: High Resolution Laterolog Array - B			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
CALSTAT	HRLTB Calibration Status	SHALLOW_DONE	
CALTEMP	HRLTB Calibration Temperature	26.8049	DEGC
FREQ0	HRLT Frequency Index for Mode 0	32	
FREQ1	HRLT Frequency Index for Mode 1	128	
FREQ2	HRLT Frequency Index for Mode 2	104	
FREQ3	HRLT Frequency Index for Mode 3	86	
FREQ4	HRLT Frequency Index for Mode 4	56	
FREQ5	HRLT Frequency Index for Mode 5	44	
FREQ6	HRLT Frequency Index for Mode 6	116	
GCSE	Generalized Caliper Selection	BS	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
ISSBAR	Barite Mud Switch	BARITE	
KFAC_HRLT	HRLT K Factor Option	SONDE	
LOOPCOEF_S	HRLT Loop Coefficient for Shallow Modes	LOW	
LOOPMOD0	HRLT Mode 0 Loop Mode	AUTO	
LOOPMOD1	HRLT Mode 1 Loop Mode	AUTO	
LOOPMOD2	HRLT Mode 2 Loop Mode	AUTO	
LOOPMOD3	HRLT Mode 3 Loop Mode	AUTO	
LOOPMOD4	HRLT Mode 4 Loop Mode	AUTO	
LOOPMOD5	HRLT Mode 5 Loop Mode	AUTO	
LOOPMOD6	HRLT Mode 6 Loop Mode	AUTO	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
PROGINV	Inversion Selection	ON	
PROCMFL	Inversion Micro-Resistivity Selection	NO_EXTERNAL_RXO	
PROCMFO	Mechanical Standoff Fin Size	0	IN
PROCRM	Processing Mud Resistivity Select	HRLT_Compute	
PROCSPO	Sonde Position	Centered	
SHT	Surface Hole Temperature	20	DEGC

Parameter	Description	Value	Units
CLCL	HLDS LS Control Loop Controller Mode	AUTO_DEFAULT	
CLCS	HLDS SS Control Loop Controller Mode	AUTO_DEFAULT	
CLLS	HLDS Mode Loop Long Spacing	AUTO	
CLSS	HLDS Mode Loop Short Spacing	AUTO	
DHC	Density Hole Correction	BS	
DPPM	Density Porosity Processing Mode	HIRS	
FD	Fluid Density	1	G/C3
LATC	HLDS Activation Correction	ON	
LLDL	HLDS LS Low Level Discriminator DAC	14000	
LLDS	HLDS SS Low Level Discriminator DAC	14000	
LLML	HLDS LS Low Level Discriminator Mode	AUTO	
LLMS	HLDS SS Low Level Discriminator Mode	AUTO	
MDEN	Matrix Density	2.6	G/C3
PHVL	HLDS Long Spacing High Voltage Setting	1000	V
PHVS	HLDS Short Spacing High Voltage Setting	1000	V
PSDL	HLDS LS Pulse Shape Compensation DAC	30000	
PSDS	HLDS SS Pulse Shape Compensation DAC	30000	
PSML	HLDS LS Pulse Shape Compensation Mode	AUTO	
PSMS	HLDS SS Pulse Shape Compensation Mode	AUTO	
APS-C: Accelerator-Porosity Tool			
	APS Software Version	0	
AASD	APS Thermal and Array Detectors High Voltage Setting	1939.6	V
ADSO	APS Array Detectors Data Source Switch	Both	
AFSD	APS Far Detector High Voltage Setting	2029.77	V
AHCS	APS Holesize Correction Source	GCSE	
AHSS	APS Holesize Correction Switch	ON	
AMTY	APS Environmental Corrections Mud Type	WaterBaseBarite	
ANSD	APS Near Detector High Voltage Setting	1697.47	V
ASOS	APS Standoff Correction Switch	ON	
ATSS	APS Temperature-Pressure-Salinity Correction Switch	ON	
BHFL_APS	APS TNPH Borehole Fluid Type	WATER	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
BSCO_APS	APS TNPH Borehole Salinity Correction Option	NO	
DPPM	Density Porosity Processing Mode	HIRS	
DSCO_APS	APS TNPH Density Source Correction Option	MEASURED	
FSAL	Formation Salinity	-50000	PPM
FSCO_APS	APS TNPH Formation Salinity Correction Option	NO	
GCSE	Generalized Caliper Selection	BS	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
HSCO_APS	APS TNPH Hole Size Correction Option	YES	
ISSBAR	Barite Mud Switch	BARITE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
MCCO_APS	APS TNPH Mud Cake Correction Option	NO	
MCOR_APS	APS TNPH Mud Correction	BARI	
MWCO_APS	APS TNPH Mud Weight Correction Option	YES	
NARC	APS Near/Array Calibration Ratio	1.08449	
NFRC	APS Near/Far Calibration Ratio	0.976579	
PTCO_APS	APS TNPH Pressure/Temperature Correction Option	NO	
SHT	Surface Hole Temperature	20	DEGC
TNCO_APS	APS TNPH Computation Option	YES	
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	BS	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.000483385	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	BARI	
HNPE	HNGS Processing Enable	YES	
ISSBAR	Barite Mud Switch	BARITE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	CENT	

VBA1	HNGS Detector 1 Variable Barite Factor Running Average	1.11288	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	1.20228	
EDTC-B: Enhanced DTS Cartridge			
BHFL	Borehole Fluid Type	WATER	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	21	DEGC
BSCO	Borehole Salinity Correction Option	NO	
CCCO	Casing & Cement Thickness Correction Option	NO	
DPPM	Density Porosity Processing Mode	HIRS	
FSAL	Formation Salinity	-50000	PPM
FSCO	Formation Salinity Correction Option	NO	
GCSE	Generalized Caliper Selection	BS	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
HSCO	Hole Size Correction Option	YES	
ISSBAR	Barite Mud Switch	BARITE	
ISSBAR_EDTC	Nuclear Mud Type	BARITE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
MCCO	Mud Cake Correction Option	NO	
MCOR	Mud Correction	BARI	
MWCO	Mud Weight Correction Option	YES	
PTCO	Pressure/Temperature Correction Option	NO	
SDAT	Standoff Data Source	SOCN	
SHT	Surface Hole Temperature	20	DEGC
SOCN	Standoff Distance	0.5	IN
SOCO	Standoff Correction Option	NO	
TPOS_EDTC	EDTC Tool Centered/Eccentered	Eccentered	
U-ETELM_EDTS	Telemetry Mode for eWAFE	Standard_EDTS	
U-TELM_EDTS	Telemetry Mode for WAFE	Standard_EDTS	

System and Miscellaneous

ALTDPCCHAN	Name of alternate depth channel	SpeedCorrectedDepth	
BS	Bit Size	9.875	IN
BSAL	Borehole Salinity	-50000.00	PPM
CSIZ	Current Casing Size	5.500	IN
CWEI	Casing Weight	168.00	LB/F
DFD	Drilling Fluid Density	1.32	G/C3
DO	Depth Offset for Playback	0.0	M
FLEV	Fluid Level	-50000.00	M
MST	Mud Sample Temperature	-50000.00	DEGC
PBVSADP	Use alternate depth channel for playback	NO	
PP	Playback Processing	NORMAL	
RMFS	Resistivity of Mud Filtrate Sample	-50000.0000	OHMM
RW	Resistivity of Connate Water	1.0000	OHMM
TD	Total Depth	310	M
TDD	Total Depth - Driller	5612.00	M
TDL	Total Depth - Logger	5612.00	M
TWS	Temperature of Connate Water Sample	37.78	DEGC

Format: TripleCombo Vertical Scale: 1:200 Graphics File Created: 20-Jun-2014 18:06

OP System Version: 19C0-187

MSS_LDEO-A	19C0-187	HRLT-B	19C0-187
HLDS	19C0-187	LDSC-B	19C0-187
APS-C	19C0-187	HNGC-B	19C0-187
HNGS-BA	19C0-187	EDTC-B	SKK-5169-EDTCB

Input DLIS Files

DEFAULT	Flip_MSS_LDEO_HRLA_029PUP	PRODUCER	20-Jun-2014 18:03	274.2 M	-93.7 M
---------	---------------------------	----------	-------------------	---------	---------

Output DLIS Files

DEFAULT	MSS_LDEO_HRLA_LDL_030PUP	FN:43	PRODUCER	20-Jun-2014 18:06
---------	--------------------------	-------	----------	-------------------

Calibration and Check Summary

Measurement	Nominal	Master	Before	After	Change	Limit	Units
High Resolution Laterolog Array - B Wellsite Calibration - HRLT M01							
Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30							
HRLT M0-M1 Voltage Plus - 0	0	N/A	-319.3	-319.0	0.2621	9.681	UV
HRLT M0-M1 Voltage Plus - 1	0	N/A	-333.4	-334.3	-0.8940	9.681	UV

HRLT M0-M1 Voltage Plus - 2	0	N/A	-335.0	-334.9	0.01013	9.681	UV
HRLT M0-M1 Voltage Plus - 3	0	N/A	-338.4	-338.4	-0.05707	9.681	UV
HRLT M0-M1 Voltage Plus - 4	0	N/A	-326.6	-326.4	0.1615	9.681	UV
HRLT M0-M1 Voltage Plus - 5	0	N/A	-322.6	-322.5	0.1267	9.681	UV
HRLT M0-M1 Voltage Plus - 6	0	N/A	323.8	325.1	1.280	9.681	UV
HRLT M0-M1 Voltage Plus - 7	0	N/A	-322.7	-322.7	0	9.681	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT M12

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT M1-M2 Voltage Plus - 0	0	N/A	1755	1754	-1.774	53.42	UV
HRLT M1-M2 Voltage Plus - 1	0	N/A	1834	1839	4.443	53.42	UV
HRLT M1-M2 Voltage Plus - 2	0	N/A	1837	1836	-0.5760	53.42	UV
HRLT M1-M2 Voltage Plus - 3	0	N/A	1855	1855	-0.2561	53.42	UV
HRLT M1-M2 Voltage Plus - 4	0	N/A	1790	1788	-1.754	53.42	UV
HRLT M1-M2 Voltage Plus - 5	0	N/A	1769	1767	-1.449	53.42	UV
HRLT M1-M2 Voltage Plus - 6	0	N/A	-1790	-1797	-6.974	53.42	UV
HRLT M1-M2 Voltage Plus - 7	0	N/A	1781	1781	0	53.42	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT M23

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT M2-M3 Voltage Plus - 0	0	N/A	1741	1739	-1.698	53.42	UV
HRLT M2-M3 Voltage Plus - 1	0	N/A	1832	1836	4.380	53.42	UV
HRLT M2-M3 Voltage Plus - 2	0	N/A	1836	1835	-0.6879	53.42	UV
HRLT M2-M3 Voltage Plus - 3	0	N/A	1857	1857	-0.2483	53.42	UV
HRLT M2-M3 Voltage Plus - 4	0	N/A	1786	1784	-1.740	53.42	UV
HRLT M2-M3 Voltage Plus - 5	0	N/A	1766	1764	-1.340	53.42	UV
HRLT M2-M3 Voltage Plus - 6	0	N/A	-1777	-1783	-6.704	53.42	UV
HRLT M2-M3 Voltage Plus - 7	0	N/A	1781	1781	0	53.42	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT V34

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT A3-A4 Voltage Plus - 0	0	N/A	68450	68400	-53.31	2100	UV
HRLT A3-A4 Voltage Plus - 1	0	N/A	71820	72020	197.5	2100	UV
HRLT A3-A4 Voltage Plus - 2	0	N/A	72280	72270	-12.32	2100	UV
HRLT A3-A4 Voltage Plus - 3	0	N/A	73380	73380	1.516	2100	UV
HRLT A3-A4 Voltage Plus - 4	0	N/A	70540	70490	-55.48	2100	UV
HRLT A3-A4 Voltage Plus - 5	0	N/A	69750	69700	-48.54	2100	UV
HRLT A3-A4 Voltage Plus - 6	0	N/A	-68660	-68960	-293.0	2100	UV
HRLT A3-A4 Voltage Plus - 7	0	N/A	70000	70000	0	2100	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT V45

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT A4-A5 Voltage Plus - 0	0	N/A	68730	68680	-51.44	2100	UV
HRLT A4-A5 Voltage Plus - 1	0	N/A	72220	72390	169.2	2100	UV
HRLT A4-A5 Voltage Plus - 2	0	N/A	72650	72630	-12.33	2100	UV
HRLT A4-A5 Voltage Plus - 3	0	N/A	73720	73720	1.516	2100	UV
HRLT A4-A5 Voltage Plus - 4	0	N/A	70840	70780	-61.51	2100	UV
HRLT A4-A5 Voltage Plus - 5	0	N/A	70030	69990	-34.95	2100	UV
HRLT A4-A5 Voltage Plus - 6	0	N/A	-69040	-69320	-274.8	2100	UV
HRLT A4-A5 Voltage Plus - 7	0	N/A	70000	70000	0	2100	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT V56

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT A5-A6 Voltage Plus - 0	0	N/A	68640	68590	-50.18	2100	UV
HRLT A5-A6 Voltage Plus - 1	0	N/A	71940	72110	172.8	2100	UV
HRLT A5-A6 Voltage Plus - 2	0	N/A	72400	72400	-2.461	2100	UV
HRLT A5-A6 Voltage Plus - 3	0	N/A	73540	73540	6.836	2100	UV
HRLT A5-A6 Voltage Plus - 4	0	N/A	70690	70640	-50.13	2100	UV
HRLT A5-A6 Voltage Plus - 5	0	N/A	69910	69890	-27.83	2100	UV
HRLT A5-A6 Voltage Plus - 6	0	N/A	-68780	-69040	-260.9	2100	UV
HRLT A5-A6 Voltage Plus - 7	0	N/A	70000	70000	0	2100	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT VTP

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT Torpedo-M0 Voltage - 0	0	N/A	-68320	-68250	62.30	2100	UV
HRLT Torpedo-M0 Voltage - 1	0	N/A	-72260	-72460	-202.5	2100	UV
HRLT Torpedo-M0 Voltage - 2	0	N/A	-72700	-72680	21.90	2100	UV
HRLT Torpedo-M0 Voltage - 3	0	N/A	-73820	-73830	-10.85	2100	UV
HRLT Torpedo-M0 Voltage - 4	0	N/A	-70890	-70840	49.79	2100	UV
HRLT Torpedo-M0 Voltage - 5	0	N/A	-70070	-70030	33.38	2100	UV
HRLT Torpedo-M0 Voltage - 6	0	N/A	69040	69330	289.4	2100	UV
HRLT Torpedo-M0 Voltage - 7	0	N/A	-70000	-70000	0	2100	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT VBD

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT Bridle#9-M0 Voltage - 0	0	N/A	-68300	-68250	55.71	2100	UV
HRLT Bridle#9-M0 Voltage - 1	0	N/A	-72250	-72430	-182.6	2100	UV
HRLT Bridle#9-M0 Voltage - 2	0	N/A	-72680	-72670	7.820	2100	UV
HRLT Bridle#9-M0 Voltage - 3	0	N/A	-73800	-73810	-16.64	2100	UV
HRLT Bridle#9-M0 Voltage - 4	0	N/A	-70890	-70830	62.55	2100	UV
HRLT Bridle#9-M0 Voltage - 5	0	N/A	-70070	-70030	42.65	2100	UV

HRLT Bridle#9-M0 Voltage - 6	0	N/A	69020	69310	290.3	2100	UV
HRLT Bridle#9-M0 Voltage - 7	0	N/A	-70000	-70000	0	2100	UV

High Resolution Laterolog Array - B Wellsite Calibration - HRLT ISO

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT Source Current Plus - 0	0	N/A	284.9	284.7	-0.2205	8.520	UA
HRLT Source Current Plus - 1	0	N/A	281.1	281.1	0	8.520	UA
HRLT Source Current Plus - 2	0	N/A	281.1	281.1	0	8.520	UA
HRLT Source Current Plus - 3	0	N/A	281.1	281.1	0	8.520	UA
HRLT Source Current Plus - 4	0	N/A	281.1	281.1	0	8.520	UA
HRLT Source Current Plus - 5	0	N/A	281.1	281.1	0	8.520	UA
HRLT Source Current Plus - 6	0	N/A	281.1	281.1	0	8.520	UA
HRLT Source Current Plus - 7	0	N/A	281.1	281.1	0	8.520	UA

High Resolution Laterolog Array - B Wellsite Calibration - HRLT MV

Before: 19-Jun-2014 0:19 After: 19-Jun-2014 1:30

HRLT Vertical Voltage PI - 0	0	N/A	-321.6	-321.4	0.2695	9.681	UV
HRLT Vertical Voltage PI - 1	0	N/A	-328.0	-328.8	-0.8510	9.681	UV
HRLT Vertical Voltage PI - 2	0	N/A	-328.4	-328.4	-0.008118	9.681	UV
HRLT Vertical Voltage PI - 3	0	N/A	-330.0	-330.1	-0.05759	9.681	UV
HRLT Vertical Voltage PI - 4	0	N/A	-315.6	-315.4	0.2337	9.681	UV
HRLT Vertical Voltage PI - 5	0	N/A	-326.7	-326.6	0.1897	9.681	UV
HRLT Vertical Voltage PI - 6	0	N/A	331.4	332.8	1.429	9.681	UV
HRLT Vertical Voltage PI - 7	0	N/A	-322.7	-322.7	0	9.681	UV

Hostile Litho-Density Sonde Wellsite Calibration - Background Measurement

Master: 18-May-2014 19:49 Before: 10-Jun-2014 22:19 After: 18-May-2014 20:19

SS Cs Resolution Bkg	9.000	7.743	7.746	7.752	0.006506	1.800	%
LS Cs Resolution Bkg	9.000	7.999	7.986	8.037	0.05058	1.800	%
LSW1 Background	100.0	83.92	82.67	83.69	1.024	3.000	CPS
LSW2 Background	100.0	76.32	75.63	74.78	-0.8435	3.000	CPS
LSW3 Background	200.0	172.1	170.5	171.0	0.4849	6.000	CPS
LSW4 Background	250.0	210.7	209.5	210.5	0.9934	7.500	CPS
LSW5 Background	600.0	492.1	491.9	491.6	-0.3414	18.00	CPS
SSW1 Background	100.0	81.53	81.07	81.08	0.007065	3.000	CPS
SSW2 Background	200.0	139.8	139.2	138.5	-0.7151	6.000	CPS
SSW3 Background	500.0	387.8	389.7	387.3	-2.356	15.00	CPS
SSW4 Background	270.0	206.4	210.7	209.5	-1.239	8.100	CPS
SSW5 Background	200.0	147.8	147.6	149.0	1.473	6.000	CPS

Hostile Litho-Density Sonde Wellsite Calibration - Aluminum Measurement

Master: 18-May-2014 19:49

LSW1 Aluminum	600.0	538.3	N/A	N/A	N/A	N/A	CPS
LSW2 Aluminum	900.0	769.4	N/A	N/A	N/A	N/A	CPS
LSW3 Aluminum	1100	928.6	N/A	N/A	N/A	N/A	CPS
LSW4 Aluminum	580.0	465.6	N/A	N/A	N/A	N/A	CPS
LSW5 Aluminum	570.0	422.0	N/A	N/A	N/A	N/A	CPS
SSW1 Aluminum	2800	2327	N/A	N/A	N/A	N/A	CPS
SSW2 Aluminum	8000	6377	N/A	N/A	N/A	N/A	CPS
SSW3 Aluminum	11600	8919	N/A	N/A	N/A	N/A	CPS
SSW4 Aluminum	5000	3682	N/A	N/A	N/A	N/A	CPS
SSW5 Aluminum	660.0	438.9	N/A	N/A	N/A	N/A	CPS

Hostile Litho-Density Sonde Wellsite Calibration - Lithology Measurement

Master: 18-May-2014 19:49

LSW1 Iron	400.0	356.8	N/A	N/A	N/A	N/A	CPS
LSW2 Iron	730.0	604.7	N/A	N/A	N/A	N/A	CPS
LSW3 Iron	1000	798.2	N/A	N/A	N/A	N/A	CPS
LSW4 Iron	520.0	413.6	N/A	N/A	N/A	N/A	CPS
LSW5 Iron	470.0	384.1	N/A	N/A	N/A	N/A	CPS
SSW1 Iron	2100	1682	N/A	N/A	N/A	N/A	CPS
SSW2 Iron	6800	5273	N/A	N/A	N/A	N/A	CPS
SSW3 Iron	10800	8065	N/A	N/A	N/A	N/A	CPS
SSW4 Iron	4600	3345	N/A	N/A	N/A	N/A	CPS
SSW5 Iron	580.0	385.6	N/A	N/A	N/A	N/A	CPS

Hostile Litho-Density Sonde Wellsite Calibration - Caliper Calibration

Before: 11-Jun-2014 0:30

HLDS Caliper Small Ring	12.00	N/A	14.74	N/A	N/A	N/A	IN
HLDS Caliper Large Ring	15.19	N/A	18.18	N/A	N/A	N/A	IN

Accelerator-Porosity Tool Wellsite Calibration - Detector Background

Master: 17-May-2014 21:32 Before: 10-Jun-2014 22:24 After: 19-Jun-2014 2:01

Near Det Bkg Cntrate	30.00	25.77	26.26	26.29	0.02178	N/A	CPS
Far Det Bkg Cntrate	30.00	26.80	27.58	27.98	0.4043	N/A	CPS
Array-1 Det Bkg Cntrate	30.00	25.44	26.75	25.90	-0.8481	N/A	CPS
Array-2 Det Bkg Cntrate	30.00	26.70	27.56	27.66	0.1053	N/A	CPS
Array Therm Det Bkg Cntrate	30.00	27.35	24.63	26.50	1.863	N/A	CPS

Accelerator-Porosity Tool Wellsite Calibration - Calibration Ratios

Master: 17-May-2014 21:51

Near/Far Calibration Ratio	0.9250	0.9766	N/A	N/A	N/A	N/A	
----------------------------	--------	--------	-----	-----	-----	-----	--

Near/Far Calibration Ratio	0.9200	0.9700	N/A	N/A	N/A	N/A	N/A
Near/Array Calibration Ratio	1.030	1.084	N/A	N/A	N/A	N/A	N/A
Near/Array Cal Ratio Up/Down	1.000	1.013	N/A	N/A	N/A	N/A	N/A

Accelerator-Porosity Tool Wellsite Calibration – Tank Check

Master: 17-May-2014 21:51							
Array-1 Standoff Porosity	11.75	10.40	N/A	N/A	N/A	N/A	PU
Array-2 Standoff Porosity	11.75	10.48	N/A	N/A	N/A	N/A	PU
Average Slowing Down Time	6.000	6.060	N/A	N/A	N/A	N/A	US
Array-1 SDT Ratio Up/Down	1.000	0.9751	N/A	N/A	N/A	N/A	
Array-2 SDT Ratio Up/Down	1.000	0.9750	N/A	N/A	N/A	N/A	
Sigma Formation	27.50	34.86	N/A	N/A	N/A	N/A	CU

Accelerator-Porosity Tool Wellsite Calibration – CCR7 signal boxes

Master: 17-May-2014 20:53							
Near Detector Plateau Setting	1650	1697	N/A	N/A	N/A	N/A	V
Far Detector Plateau Setting	2000	2030	N/A	N/A	N/A	N/A	V
Array Detector Plateau Setting	2000	1940	N/A	N/A	N/A	N/A	V

Hostile Natural Gamma Ray Sonde Wellsite Calibration – Detector 1 Check

Master: 17-May-2014 3:32 Before: 10-Jun-2014 22:38 After: 17-May-2014 3:46							
Na 511 Peak Loc	40.00	39.68	39.69	39.70	0.003128	1.000	
Na 511 Peak Res	15.50	14.95	15.43	16.14	0.7069	2.000	%
High Voltage	1150	1174	1175	1174	-0.08655	N/A	V
Na 1785 Peak Loc	142.6	143.3	141.3	142.5	1.252	7.000	
Na 1785 Peak Res	8.500	7.428	7.650	8.638	0.9881	2.000	%
Temperature	15.50	29.15	30.00	29.26	-0.7430	N/A	DEGC
Na Count Rate	45.00	12.49	11.75	11.88	0.1340	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration – Detector 2 Check

Master: 17-May-2014 3:32 Before: 10-Jun-2014 22:38 After: 17-May-2014 3:46							
Na 511 Peak Loc	40.00	39.32	39.63	39.58	-0.04301	1.000	
Na 511 Peak Res	15.50	16.57	16.61	16.31	-0.2982	2.000	%
High Voltage	1150	1107	1110	1108	-1.606	N/A	V
Na 1785 Peak Loc	142.6	140.5	142.7	142.7	-0.004791	7.000	
Na 1785 Peak Res	8.500	9.002	9.484	9.819	0.3349	2.000	%
Temperature	15.50	29.28	30.44	29.38	-1.062	N/A	DEGC
Na Count Rate	45.00	12.67	12.05	12.14	0.09100	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration – Ratio Of Detector 1 To Detector 2

Master: 17-May-2014 3:32 Before: 10-Jun-2014 22:38 After: 17-May-2014 3:46							
Coincidence Count Rate Ratio	1.000	0.9880	0.9769	0.9796	0.002670	0.05000	

Hostile Natural Gamma Ray Sonde Master Calibration – Detector 1 Calibration

Master: 17-May-2014 3:27							
Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	210.1	--	--	--	--	
Th Peak Res	7.000	6.596	--	--	--	--	%
Background Count Rate	142.5	20.48	--	--	--	--	CPS
Gain Ratio	1.000	1.007	--	--	--	--	

Hostile Natural Gamma Ray Sonde Master Calibration – Detector 2 Calibration

Master: 17-May-2014 3:27							
Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	207.6	--	--	--	--	
Th Peak Res	7.000	7.200	--	--	--	--	%
Background Count Rate	142.5	21.26	--	--	--	--	CPS
Gain Ratio	1.000	1.004	--	--	--	--	

Enhanced DTS Cartridge Wellsite Calibration – EDTC Accelerometer Calibration

Before: Calibration out of date 18-Jun-2014 19:30							
EDTC Z-Axis Acceleration	9.810	N/A	9.720	N/A	N/A	N/A	M/S2

Enhanced DTS Cartridge Wellsite Calibration – Detector Calibration

Before: Calibration out of date 17-May-2014 3:36 After: Calibration out of date 17-May-2014 3:43							
Gamma Ray (Jig – Bkg)	157.1	N/A	157.1	153.5	-3.532	14.28	GAPI
Gamma Ray (Calibrated)	165.0	N/A	165.0	161.3	-3.710	15.00	GAPI

Accelerator-Porosity Tool – Detector Plateau Settings :

Near Detector Plateau Setting	1697 V
Far Detector Plateau Setting	2030 V
Array Detector Plateau Setting	1940 V

Primary Equipment:

HRLT Sonde

HRLS - B

768

Auxiliary Equipment:

HRLT lower Housing

HRLH - B

968

HRLT Lower Cartridge

HRLC - B

974

HRLT upper Housing

HRUH - B

978

HRLT Upper Cartridge

HRUC - B

764

High Resolution Laterolog Array - B Wellsite Calibration							
HRLT M01							
Idx	Phase	HRLT M0-M1 Voltage Plus UV	Value	Nominal	Maximum	Minimum	
0	Before		-319.3	-322.7	-280.7	-379.7	
	After		-319.0				
1	Before		-333.4	-322.7	-280.7	-379.7	
	After		-334.3				
2	Before		-335.0	-322.7	-280.7	-379.7	
	After		-334.9				
3	Before		-338.4	-322.7	-280.7	-379.7	
	After		-338.4				
4	Before		-326.6	-322.7	-280.7	-379.7	
	After		-326.4				
5	Before		-322.6	-322.7	-280.7	-379.7	
	After		-322.5				
6	Before		323.8	322.7	379.7	280.7	
	After		325.1				
7	Before		-322.7	-322.7	-280.7	-379.7	
	After		-322.7				
		(Minimum) (Nominal) (Maximum)					
Before: 19-Jun-2014 0:19							
After: 19-Jun-2014 1:30							

High Resolution Laterolog Array - B Wellsite Calibration							
HRLT M12							
Idx	Phase	HRLT M1-M2 Voltage Plus UV	Value	Nominal	Maximum	Minimum	
0	Before		1755	1781	2095	1549	
	After		1754				
1	Before		1834	1781	2095	1549	
	After		1839				
2	Before		1837	1781	2095	1549	
	After		1836				
3	Before		1855	1781	2095	1549	
	After		1855				
4	Before		1790	1781	2095	1549	
	After		1788				
5	Before		1769	1781	2095	1549	
	After		1767				
6	Before		-1790	-1781	-1549	-2095	
	After		-1797				
7	Before		1781	1781	2095	1549	
	After		1781				

(Minimum)	(Nominal)	(Maximum)		
Before: 19-Jun-2014 0:19				
After: 19-Jun-2014 1:30				

High Resolution Laterolog Array – B Wellsite Calibration						
HRLT M23						
Idx	Phase	HRLT M2-M3 Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		1741	1781	2095	1549
	After		1739			
1	Before		1832	1781	2095	1549
	After		1836			
2	Before		1836	1781	2095	1549
	After		1835			
3	Before		1857	1781	2095	1549
	After		1857			
4	Before		1786	1781	2095	1549
	After		1784			
5	Before		1766	1781	2095	1549
	After		1764			
6	Before		-1777	-1781	-1549	-2095
	After		-1783			
7	Before		1781	1781	2095	1549
	After		1781			
		(Minimum) (Nominal) (Maximum)				
Before: 19-Jun-2014 0:19						
After: 19-Jun-2014 1:30						

High Resolution Laterolog Array – B Wellsite Calibration						
HRLT V34						
Idx	Phase	HRLT A3-A4 Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		68450	70000	82360	60900
	After		68400			
1	Before		71820	70000	82360	60900
	After		72020			
2	Before		72280	70000	82360	60900
	After		72270			
3	Before		73380	70000	82360	60900
	After		73380			
4	Before		70540	70000	82360	60900
	After		70490			
5	Before		69750	70000	82360	60900
	After		69700			
6	Before		-68660	-70000	-60900	-82360
	After		-68960			
7	Before		70000	70000	82360	60900
	After		70000			
		(Minimum) (Nominal) (Maximum)				
Before: 19-Jun-2014 0:19						

High Resolution Laterolog Array – B Wellsite Calibration						
HRLT V45						
Idx	Phase	HRLT A4–A5 Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		68730	70000	82360	60900
	After		68680			
1	Before		72220	70000	82360	60900
	After		72390			
2	Before		72650	70000	82360	60900
	After		72630			
3	Before		73720	70000	82360	60900
	After		73720			
4	Before		70840	70000	82360	60900
	After		70780			
5	Before		70030	70000	82360	60900
	After		69990			
6	Before		-69040	-70000	-60900	-82360
	After		-69320			
7	Before		70000	70000	82360	60900
	After		70000			
		(Minimum) (Nominal) (Maximum)				

Before: 19-Jun-2014 0:19

After: 19-Jun-2014 1:30

High Resolution Laterolog Array – B Wellsite Calibration						
HRLT V56						
Idx	Phase	HRLT A5–A6 Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		68640	70000	82360	60900
	After		68590			
1	Before		71940	70000	82360	60900
	After		72110			
2	Before		72400	70000	82360	60900
	After		72400			
3	Before		73540	70000	82360	60900
	After		73540			
4	Before		70690	70000	82360	60900
	After		70640			
5	Before		69910	70000	82360	60900
	After		69890			
6	Before		-68780	-70000	-60900	-82360
	After		-69040			
7	Before		70000	70000	82360	60900
	After		70000			
		(Minimum) (Nominal) (Maximum)				

Before: 19-Jun-2014 0:19

After: 19-Jun-2014 1:30

High Resolution Laterolog Array – B Wellsite Calibration						
--	--	--	--	--	--	--

HRLT VTP

Idx	Phase	HRLT Torpedo-M0 Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		-68320	-70000	-60900	-82360
	After		-68250			
1	Before		-72260	-70000	-60900	-82360
	After		-72460			
2	Before		-72700	-70000	-60900	-82360
	After		-72680			
3	Before		-73820	-70000	-60900	-82360
	After		-73830			
4	Before		-70890	-70000	-60900	-82360
	After		-70840			
5	Before		-70070	-70000	-60900	-82360
	After		-70030			
6	Before		69040	70000	82360	60900
	After		69330			
7	Before		-70000	-70000	-60900	-82360
	After		-70000			
			(Minimum)	(Nominal)	(Maximum)	

Before: 19-Jun-2014 0:19

After: 19-Jun-2014 1:30

High Resolution Laterolog Array - B Wellsite Calibration

HRLT VBD

Idx	Phase	HRLT Bridle#9-M0 Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		-68300	-70000	-60900	-82360
	After		-68250			
1	Before		-72250	-70000	-60900	-82360
	After		-72430			
2	Before		-72680	-70000	-60900	-82360
	After		-72670			
3	Before		-73800	-70000	-60900	-82360
	After		-73810			
4	Before		-70890	-70000	-60900	-82360
	After		-70830			
5	Before		-70070	-70000	-60900	-82360
	After		-70030			
6	Before		69020	70000	82360	60900
	After		69310			
7	Before		-70000	-70000	-60900	-82360
	After		-70000			
			(Minimum)	(Nominal)	(Maximum)	

Before: 19-Jun-2014 0:19

After: 19-Jun-2014 1:30

High Resolution Laterolog Array - B Wellsite Calibration

HRLT ISO

Idx	Phase	HRLT Source Current Plus UA	Value	Nominal	Maximum	Minimum
	Before		284.9			

0	Before		284.7	284.0	334.1	247.0
1	Before		281.1	281.1	330.7	244.4
	After		281.1			
2	Before		281.1	281.1	330.7	244.4
	After		281.1			
3	Before		281.1	281.1	330.7	244.4
	After		281.1			
4	Before		281.1	281.1	330.7	244.4
	After		281.1			
5	Before		281.1	281.1	330.7	244.4
	After		281.1			
6	Before		281.1	281.1	330.7	244.4
	After		281.1			
7	Before		281.1	281.1	330.7	244.4
	After		281.1			
			(Minimum)	(Nominal)	(Maximum)	

Before: 19-Jun-2014 0:19
After: 19-Jun-2014 1:30

High Resolution Laterolog Array – B Wellsite Calibration						
HRLT MV						
Idx	Phase	HRLT Vertical Voltage Plus UV	Value	Nominal	Maximum	Minimum
0	Before		-321.6	-322.7	-280.7	-379.7
	After		-321.4			
1	Before		-328.0	-322.7	-280.7	-379.7
	After		-328.8			
2	Before		-328.4	-322.7	-280.7	-379.7
	After		-328.4			
3	Before		-330.0	-322.7	-280.7	-379.7
	After		-330.1			
4	Before		-315.6	-322.7	-280.7	-379.7
	After		-315.4			
5	Before		-326.7	-322.7	-280.7	-379.7
	After		-326.6			
6	Before		331.4	322.7	379.7	280.7
	After		332.8			
7	Before		-322.7	-322.7	-280.7	-379.7
	After		-322.7			
			(Minimum)	(Nominal)	(Maximum)	

Before: 19-Jun-2014 0:19
After: 19-Jun-2014 1:30

Hostile Litho-Density Sonde / Equipment Identification

Primary Equipment:		
Hostile Litho Density Sonde	HLDS – D	35
Hostile Litho Density High Voltage	HLDV – D	35
Gamma Source Radioactive	GSR – Z	8113

Hostile Litho–Density Sonde Wellsite Calibration								
Background Measurement								
Phase	SS Cs Resolution Bkg %	Value	Phase	LS Cs Resolution Bkg %	Value	Phase	LSW1 Background CPS	Value
Master		7.743	Master		7.999	Master		83.92
Before		7.746	Before		7.986	Before		82.67
After		7.752	After		8.037	After		83.69
		7.000 (Minimum)			9.000 (Nominal)			11.00 (Maximum)
		7.000 (Minimum)			9.000 (Nominal)			11.00 (Maximum)
		55.00 (Minimum)			100.0 (Nominal)			150.0 (Maximum)
Phase	LSW2 Background CPS	Value	Phase	LSW3 Background CPS	Value	Phase	LSW4 Background CPS	Value
Master		76.32	Master		172.1	Master		210.7
Before		75.63	Before		170.5	Before		209.5
After		74.78	After		171.0	After		210.5
		50.00 (Minimum)			100.0 (Nominal)			140.0 (Maximum)
		110.0 (Minimum)			200.0 (Nominal)			290.0 (Maximum)
		140.0 (Minimum)			250.0 (Nominal)			360.0 (Maximum)
Phase	LSW5 Background CPS	Value	Phase	SSW1 Background CPS	Value	Phase	SSW2 Background CPS	Value
Master		492.1	Master		81.53	Master		139.8
Before		491.9	Before		81.07	Before		139.2
After		491.6	After		81.08	After		138.5
		330.0 (Minimum)			600.0 (Nominal)			830.0 (Maximum)
		55.00 (Minimum)			100.0 (Nominal)			150.0 (Maximum)
		100.0 (Minimum)			200.0 (Nominal)			260.0 (Maximum)
Phase	SSW3 Background CPS	Value	Phase	SSW4 Background CPS	Value	Phase	SSW5 Background CPS	Value
Master		387.8	Master		206.4	Master		147.8
Before		389.7	Before		210.7	Before		147.6
After		387.3	After		209.5	After		149.0
		280.0 (Minimum)			500.0 (Nominal)			700.0 (Maximum)
		150.0 (Minimum)			270.0 (Nominal)			380.0 (Maximum)
		110.0 (Minimum)			200.0 (Nominal)			270.0 (Maximum)
Master: 18–May–2014 19:49			Before: 10–Jun–2014 22:19			After: 18–May–2014 20:19		

Hostile Litho–Density Sonde Master Calibration								
Detector Background Measurement								
Phase	LSW1 Background CPS	Value	Phase	LSW2 Background CPS	Value	Phase	LSW3 Background CPS	Value
Master		83.92	Master		76.32	Master		172.1
		55.00 (Minimum)			100.0 (Nominal)			150.0 (Maximum)
		50.00 (Minimum)			100.0 (Nominal)			140.0 (Maximum)
		110.0 (Minimum)			200.0 (Nominal)			290.0 (Maximum)
Phase	LSW4 Background CPS	Value	Phase	LSW5 Background CPS	Value	Phase	LS Cs Resolution Bkg %	Value
Master		210.7	Master		492.1	Master		7.999
		140.0 (Minimum)			250.0 (Nominal)			360.0 (Maximum)
		330.0 (Minimum)			600.0 (Nominal)			830.0 (Maximum)
		7.000 (Minimum)			9.000 (Nominal)			11.00 (Maximum)
Phase	SSW1 Background CPS	Value	Phase	SSW2 Background CPS	Value	Phase	SSW3 Background CPS	Value
Master		81.53	Master		139.8	Master		387.8
		55.00 (Minimum)			100.0 (Nominal)			150.0 (Maximum)
		100.0 (Minimum)			200.0 (Nominal)			260.0 (Maximum)
		280.0 (Minimum)			500.0 (Nominal)			700.0 (Maximum)
Phase	SSW4 Background CPS	Value	Phase	SSW5 Background CPS	Value	Phase	SS Cs Resolution Bkg %	Value
Master		206.4	Master		147.8	Master		7.743
		150.0 (Minimum)			270.0 (Nominal)			380.0 (Maximum)
		110.0 (Minimum)			200.0 (Nominal)			270.0 (Maximum)
		7.000 (Minimum)			9.000 (Nominal)			11.00 (Maximum)
Master: 18–May–2014 19:49								

Hostile Litho–Density Sonde Master Calibration								
Detector Aluminum Measurement (bkgd-subtracted)								
Phase	LSW1 Aluminum CPS	Value	Phase	LSW2 Aluminum CPS	Value	Phase	LSW3 Aluminum CPS	Value
Master		538.3	Master		769.4	Master		928.6
		420.0 (Minimum)			600.0 (Nominal)			770.0 (Maximum)
		650.0 (Minimum)			900.0 (Nominal)			1150 (Maximum)
		800.0 (Minimum)			1100 (Nominal)			1450 (Maximum)
Phase	LSW4 Aluminum CPS	Value	Phase	LSW5 Aluminum CPS	Value	Phase	SSW1 Aluminum CPS	Value
Master		465.6	Master		422.0	Master		2327

410.0 (Minimum)	580.0 (Nominal)	740.0 (Maximum)	Phase	SSW2 Aluminum CPS	Value	410.0 (Minimum)	570.0 (Nominal)	740.0 (Maximum)	Phase	SSW3 Aluminum CPS	Value	2000 (Minimum)	2800 (Nominal)	3200 (Maximum)	Phase	SSW4 Aluminum CPS	Value
			Master		6377				Master		8919				Master		3682
5800 (Minimum)	8000 (Nominal)	9300 (Maximum)				8300 (Minimum)	11600 (Nominal)	13500 (Maximum)				3500 (Minimum)	5000 (Nominal)	5800 (Maximum)			
			Phase	SSW5 Aluminum CPS	Value												
			Master		438.9												
430.0 (Minimum)	660.0 (Nominal)	770.0 (Maximum)															

Master: 18-May-2014 19:49

Hostile Litho-Density Sonde Master Calibration																	
Detector Litholog Measurement (bkgd-subtracted)																	
Phase	LSW1 Iron CPS			Value	Phase	LSW2 Iron CPS			Value	Phase	LSW3 Iron CPS			Value			
Master				356.8	Master				604.7	Master				798.2			
	290.0 (Minimum)	400.0 (Nominal)	560.0 (Maximum)			520.0 (Minimum)	730.0 (Nominal)	950.0 (Maximum)			720.0 (Minimum)	1000 (Nominal)	1350 (Maximum)				
Phase	LSW4 Iron CPS			Value	Phase	LSW5 Iron CPS			Value	Phase	SSW1 Iron CPS			Value			
Master				413.6	Master				384.1	Master				1682			
	370.0 (Minimum)	520.0 (Nominal)	700.0 (Maximum)			340.0 (Minimum)	470.0 (Nominal)	750.0 (Maximum)			1500 (Minimum)	2100 (Nominal)	2400 (Maximum)				
Phase	SSW2 Iron CPS			Value	Phase	SSW3 Iron CPS			Value	Phase	SSW4 Iron CPS			Value			
Master				5273	Master				8065	Master				3345			
	4900 (Minimum)	6800 (Nominal)	7900 (Maximum)			7800 (Minimum)	10800 (Nominal)	12600 (Maximum)			3300 (Minimum)	4600 (Nominal)	5400 (Maximum)				
Phase	SSW5 Iron CPS			Value													
Master				385.6													
	420.0 (Minimum)	580.0 (Nominal)	680.0 (Maximum)														

Master: 18-May-2014 19:49

Hostile Litho-Density Sonde Master Calibration																	
Quality Ratios																	
Phase	AL CALIBRATION RATIO 1			Value	Phase	AL CALIBRATION RATIO 2			Value	Phase	AL CALIBRATION RATIO 3			Value			
Master				1.046	Master				2.165	Master				0.6065			
	0.9000 (Minimum)	1.000 (Nominal)	1.100 (Maximum)			1.900 (Minimum)	2.100 (Nominal)	2.300 (Maximum)			0.4500 (Minimum)	0.5500 (Nominal)	0.6500 (Maximum)				
Phase	AL CALIBRATION RATIO 4			Value	Phase	Pad-Wear SS Ratio			Value	Phase	Pad-Wear LS Ratio			Value			
Master				0.5648	Master				0.9921	Master				0.9878			
	0.4000 (Minimum)	0.5500 (Nominal)	0.6500 (Maximum)			0.9800 (Minimum)	0.9880 (Nominal)	0.9960 (Maximum)			0.9800 (Minimum)	0.9880 (Nominal)	0.9960 (Maximum)				
Phase	Pad-Position SS Ratio			Value	Phase	Pad-Position LS Ratio			Value								
Master				0.9668	Master				0.9008								
	0.9900 (Minimum)	0.9940 (Nominal)	1.015 (Maximum)			0.9850 (Minimum)	0.9940 (Nominal)	1.010 (Maximum)									

Master: 18-May-2014 19:49

Litho-Density Spectroscopy Cartridge - B / Equipment Identification

Primary Equipment:
 LDSC Cartridge LDSC - B 326

Auxiliary Equipment:
 LDSC Housing LDSH - A 303

Accelerator-Porosity Tool / Equipment Identification

Primary Equipment:
 Accelerator-Porosity Sonde APS - C 212
 APS Minitron MNTR - F 6504

Auxiliary Equipment:
 Accelerator-Porosity Housing APH - AC 121
 APS Calibration Water Tank SFT - 178 1

Accelerator-Porosity Tool Wellsite Calibration									
Detector Background									
Phase	Near Det Bkg Cntrate CPS	Value	Phase	Far Det Bkg Cntrate CPS	Value	Phase	Array-1 Det Bkg Cntrate CPS	Value	
Master		25.77	Master		26.80	Master		25.44	
Before		26.26	Before		27.58	Before		26.75	
After		26.29	After		27.98	After		25.90	
	1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)			1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)			1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)		
Phase	Array-2 Det Bkg Cntrate CPS	Value	Phase	Array Therm Det Bkg Cntrate CPS	Value				
Master		26.70	Master		27.35				
Before		27.56	Before		24.63				
After		27.66	After		26.50				
	1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)			1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)					
Master: 17-May-2014 21:32			Before: 10-Jun-2014 22:24			After: 19-Jun-2014 2:01			

Accelerator-Porosity Tool Wellsite Calibration									
Calibration Ratios									
Phase	Near/Far Calibration Ratio	Value	Phase	Near/Array Calibration Ratio	Value	Phase	Near/Array Cal Ratio Up/Down	Value	
Master		0.9766	Master		1.084	Master		1.013	
	0.8000 (Minimum) 0.9250 (Nominal) 1.050 (Maximum)			0.9000 (Minimum) 1.030 (Nominal) 1.170 (Maximum)			0.9700 (Minimum) 1.000 (Nominal) 1.030 (Maximum)		
Master: 17-May-2014 21:51									

Accelerator-Porosity Tool Wellsite Calibration									
Tank Check									
Phase	Array-1 Standoff Porosity PU	Value	Phase	Array-2 Standoff Porosity PU	Value	Phase	Average Slowing Down Time US	Value	
Master		10.40	Master		10.48	Master		6.060	
	9.900 (Minimum) 11.75 (Nominal) 13.60 (Maximum)			9.900 (Minimum) 11.75 (Nominal) 13.60 (Maximum)			5.500 (Minimum) 6.000 (Nominal) 6.250 (Maximum)		
Phase	Array-1 SDT Ratio Up/Down	Value	Phase	Array-2 SDT Ratio Up/Down	Value	Phase	Sigma Formation CU	Value	
Master		0.9751	Master		0.9750	Master		34.86	
	0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)			0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)			20.00 (Minimum) 27.50 (Nominal) 35.00 (Maximum)		
Master: 17-May-2014 21:51									

Accelerator-Porosity Tool Master Calibration									
Detector Calibration									
Phase	Near/Far Calibration Ratio	Value	Phase	Near/Array Calibration Ratio	Value	Phase	Near/Array Cal Ratio Up/Down	Value	
Master		0.9766	Master		1.084	Master		1.013	
	0.8000 (Minimum) 0.9250 (Nominal) 1.050 (Maximum)			0.9000 (Minimum) 1.030 (Nominal) 1.170 (Maximum)			0.9700 (Minimum) 1.000 (Nominal) 1.030 (Maximum)		
Master: 17-May-2014 21:51									

Accelerator-Porosity Tool Master Calibration									
Tank Check									
Phase	Array-1 Standoff Porosity PU	Value	Phase	Array-2 Standoff Porosity PU	Value	Phase	Average Slowing Down Time US	Value	
Master		10.40	Master		10.48	Master		6.060	
	9.900 (Minimum) 11.75 (Nominal) 13.60 (Maximum)			9.900 (Minimum) 11.75 (Nominal) 13.60 (Maximum)			5.500 (Minimum) 6.000 (Nominal) 6.250 (Maximum)		
Phase	Array-1 SDT Ratio Up/Down	Value	Phase	Array-2 SDT Ratio Up/Down	Value	Phase	Sigma Formation CU	Value	
Master		0.9751	Master		0.9750	Master		34.86	
	0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)			0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)			20.00 (Minimum) 27.50 (Nominal) 35.00 (Maximum)		
Master: 17-May-2014 21:51									

Hostile Natural Gamma Ray Cartridge - B / Equipment Identification

Primary Equipment:

UNGC Cartridge

UNGC - B

200

Auxiliary Equipment:
HNGC Housing

HNGH - A

115

Hostile Natural Gamma Ray Sonde / Equipment Identification

Primary Equipment:
HNGS Sonde

HNGS - BA

194

Auxiliary Equipment:
HNGS Sonde Housing
Gamma Source Radioactive

HNSH - BA

205

GSR - U 616008

Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 1 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		39.68	Master		14.95	Master		1174
Before		39.69	Before		15.43	Before		1175
After		39.70	After		16.14	After		1174
	37.50 (Minimum) 40.00 (Nominal) 43.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		143.3	Master		7.428	Master		29.15
Before		141.3	Before		7.650	Before		30.00
After		142.5	After		8.638	After		29.26
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		12.49						
Before		11.75						
After		11.88						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 17-May-2014 3:32			Before: 10-Jun-2014 22:38			After: 17-May-2014 3:46		

Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 2 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		39.32	Master		16.57	Master		1107
Before		39.63	Before		16.61	Before		1110
After		39.58	After		16.31	After		1108
	37.50 (Minimum) 40.00 (Nominal) 43.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		140.5	Master		9.002	Master		29.28
Before		142.7	Before		9.484	Before		30.44
After		142.7	After		9.819	After		29.38
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		12.67						
Before		12.05						
After		12.14						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 17-May-2014 3:32			Before: 10-Jun-2014 22:38			After: 17-May-2014 3:46		

Ratio Of Detector 1 To Detector 2

Phase	Coincidence Count Rate Ratio	Value
Master		0.9880
Before		0.9769
After		0.9796
	0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)	
Master: 17-May-2014 3:32		
Before: 10-Jun-2014 22:38		
After: 17-May-2014 3:46		

Hostile Natural Gamma Ray Sonde Master Calibration

Detector 1 Calibration

Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value
Master		41.00	Master		210.1	Master		6.596
	38.00 (Minimum) 40.00 (Nominal) 43.00 (Maximum)			201.0 (Minimum) 209.6 (Nominal) 218.3 (Maximum)			5.000 (Minimum) 7.000 (Nominal) 9.000 (Maximum)	
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value			
Master		20.48	Master		1.007			
	10.00 (Minimum) 142.5 (Nominal) 265.0 (Maximum)			0.9400 (Minimum) 1.000 (Nominal) 1.060 (Maximum)				
Master: 17-May-2014 3:27								

Hostile Natural Gamma Ray Sonde Master Calibration

Detector 2 Calibration

Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value
Master		41.00	Master		207.6	Master		7.200
	38.00 (Minimum) 40.00 (Nominal) 43.00 (Maximum)			201.0 (Minimum) 209.6 (Nominal) 218.3 (Maximum)			5.000 (Minimum) 7.000 (Nominal) 9.000 (Maximum)	
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value			
Master		21.26	Master		1.004			
	10.00 (Minimum) 142.5 (Nominal) 265.0 (Maximum)			0.9400 (Minimum) 1.000 (Nominal) 1.060 (Maximum)				
Master: 17-May-2014 3:27								

Enhanced DTS Cartridge / Equipment Identification

Primary Equipment:

EDTC Gamma Ray Detector EDTG - A/B 8305
 Enhanced DTS Cartridge EDTC - B 8317

Auxiliary Equipment:

EDTC Housing EDTH - B 8303

Enhanced DTS Cartridge Wellsite Calibration

EDTC Accelerometer Calibration

Phase	EDTC Z-Axis Acceleration M/S2	Value
Before		9.720
	9.610 (Minimum) 9.810 (Nominal) 10.01 (Maximum)	
Before: 18-Jun-2014 19:30		

Enhanced DTS Cartridge Wellsite Calibration

Detector Calibration

Phase	Gamma Ray Background GAPI	Value	Phase	Gamma Ray (Jig - Bkg) GAPI	Value	Phase	Gamma Ray (Calibrated) GAPI	Value
Before		6.621	Before		157.1	Before		165.0
After		6.812	After		153.5	After		161.3
	0 (Minimum) 30.00 (Nominal) 120.0 (Maximum)			142.8 (Minimum) 157.1 (Nominal) 171.3 (Maximum)			150.0 (Minimum) 165.0 (Nominal) 180.0 (Maximum)	
Before: 17-May-2014 3:36			After: 17-May-2014 3:43					

Company: **Lamont Doherty Earth Observatory**

Schlumberger

Well: **Expedition 351, Site U1438D**

Field: **IBM Arc Origins**

Rig: **JOIDES Resolution**

Ocean: **Pacific**

High Resolution Laterolog Array (HRLA)

HLDS/APS Density/Porosity

Natural Gamma Ray