

Company: Lamont Doherty

Well: ODP Leg 204, Site 1247B

Field: Hydrate Ridge

Ocean: Pacific **State:** Oregon


Natural Gamma Ray Spectroscopy

Ocean: Pacific
 Field: Hydrate Ridge
 Location: W 125.2 *
 Well: ODP Leg 204, Site 1247B
 Company: Lamont Doherty

LOCATION					
W 125.2 *		Elev.:	K.B.	11.3 m	
N 44.6 *			G.L.	-846 m	
			D.F.	11 m	
Permanent Datum:	MSL	Elev.:	0 m		
Log Measured From:	RKB		11.3 m	above Perm. Datum	
Drilling Measured From:	RKB				
API Serial No.		Max. Hole Devi.		Longitude	Latitude

Logging Date	23-Aug-2002				
Run Number	1				
Depth Driller	1066 m				
Schlumberger Depth	1066 m				
Bottom Log Interval	1034 m				
Top Log Interval	920 m				
Casing Driller Size @ Depth	0.000 in @ 920 m				
Casing Schlumberger	920 m				
Bit Size	11.438 in				
Type Fluid In Hole	Sepiolite Salt Water Base				
Density	Viscosity				
Fluid Loss	PH				
Source Of Sample	Mud Pit				
RM @ Measured Temperature	0.322 ohm.m	@	27 degC	@	
RMF @ Measured Temperature	@	@		@	
RMC @ Measured Temperature	@	@		@	
Source RMF	RMC				
RM @ MRT	RMF @ MRT	0.392 @ 18	@ 18	@	@
Maximum Recorded Temperatures	18 degC				
Circulation Stopped	23-Aug-2002	Time	16:00		
Logger On Bottom	23-Aug-2002	Time	19:00		
Unit Number	99	Location	Houston-ODP		
Recorded By	K. Swain				
Witnessed By	G. Guerin, S. Barr, T. Collett				

Logging Date				
Run Number				
Depth Driller				
Schlumberger Depth				
Bottom Log Interval				
Top Log Interval				
Casing Driller Size @ Depth				
Casing Schlumberger				
Bit Size				
Type Fluid In Hole				
Density	Viscosity			
Fluid Loss	PH			
Source Of Sample				
RM @ Measured Temperature		@		
RMF @ Measured Temperature		@		
RMC @ Measured Temperature		@		
Source RMF	RMC			
RM @ MRT	RMF @ MRT	@	@	@
Maximum Recorded Temperatures				
Circulation Stopped				
Logger On Bottom				
Unit Number				
Recorded By				
Witnessed By				

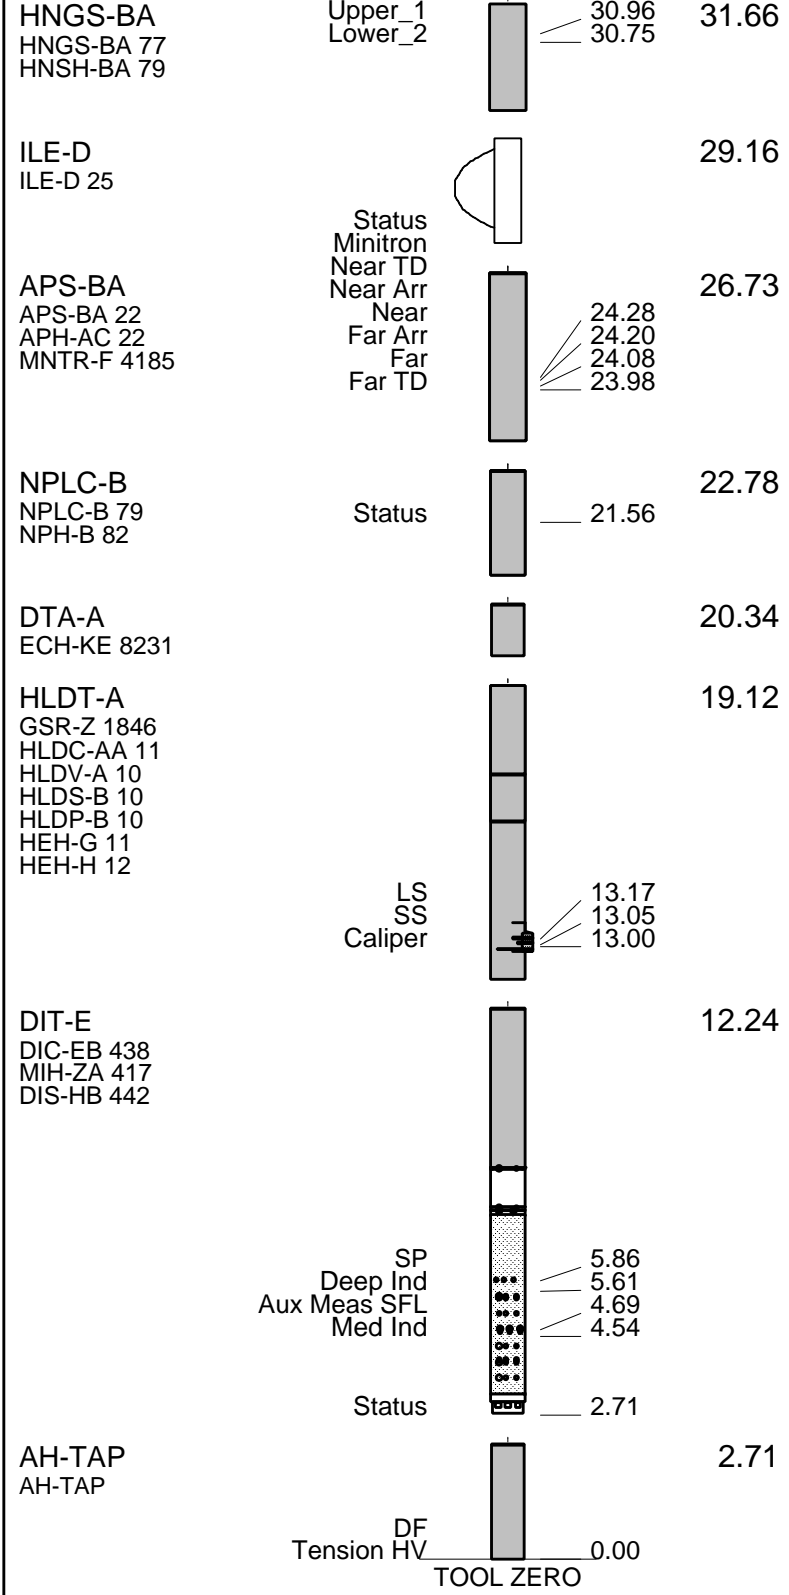

TOOL ZERO

MAXIMUM STRING DIAMETER 3.88 IN
 MEASUREMENTS RELATIVE TO TOOL ZERO
 ALL LENGTHS IN METERS

Output DLIS Files


DEFAULT	PI_LDL_APS_NGS_004LUP	FN:4	PRODUCER	23-Aug-2002 18:58	1067.6 M	834.4 M
REDUCE	PI_LDL_APS_NGS_004LUP	FN:5	PRODUCER	23-Aug-2002 18:58	1067.6 M	833.2 M


OP System Version: 10C0-306 MCM


DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		


PIP SUMMARY


Time Mark Every 60 S

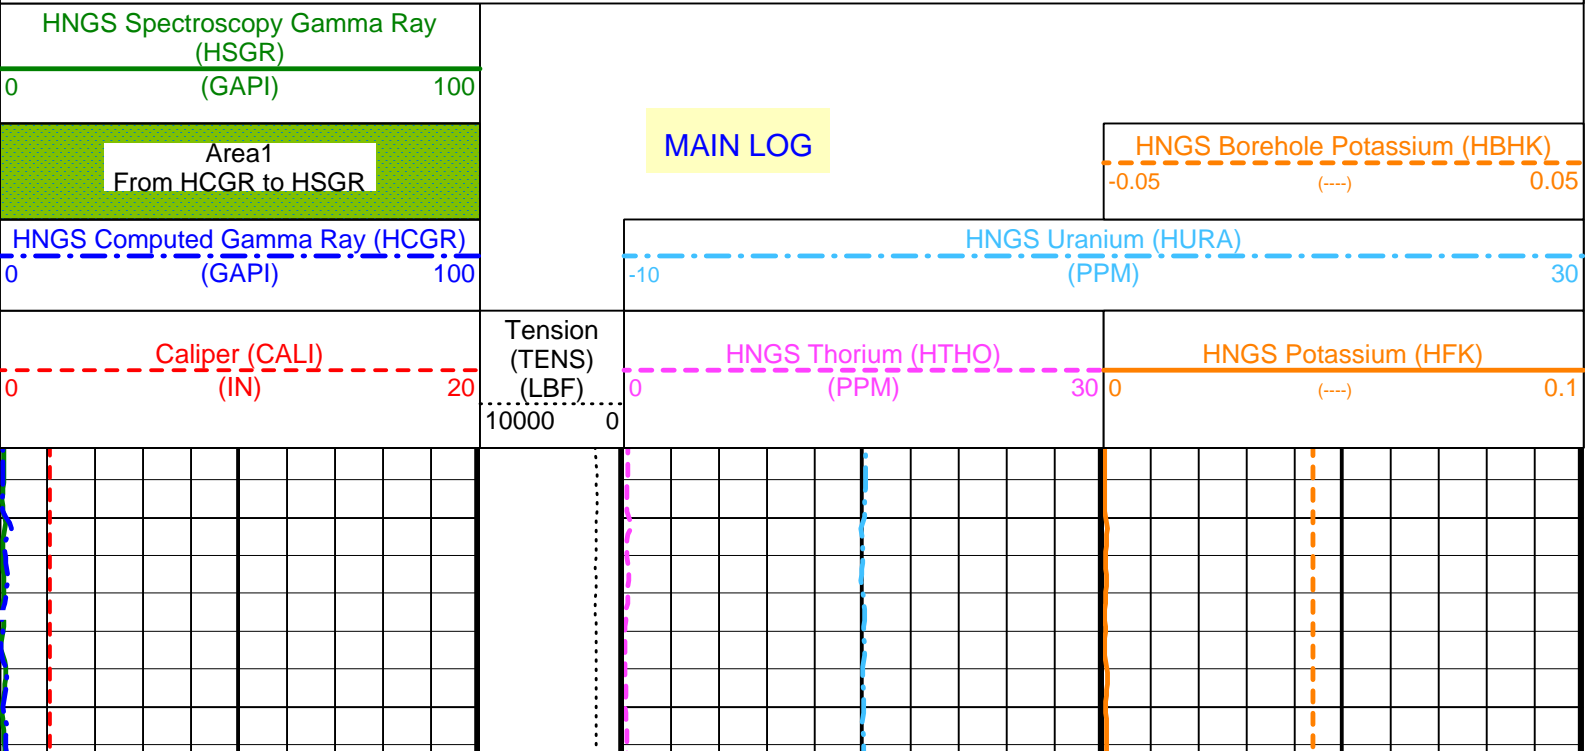


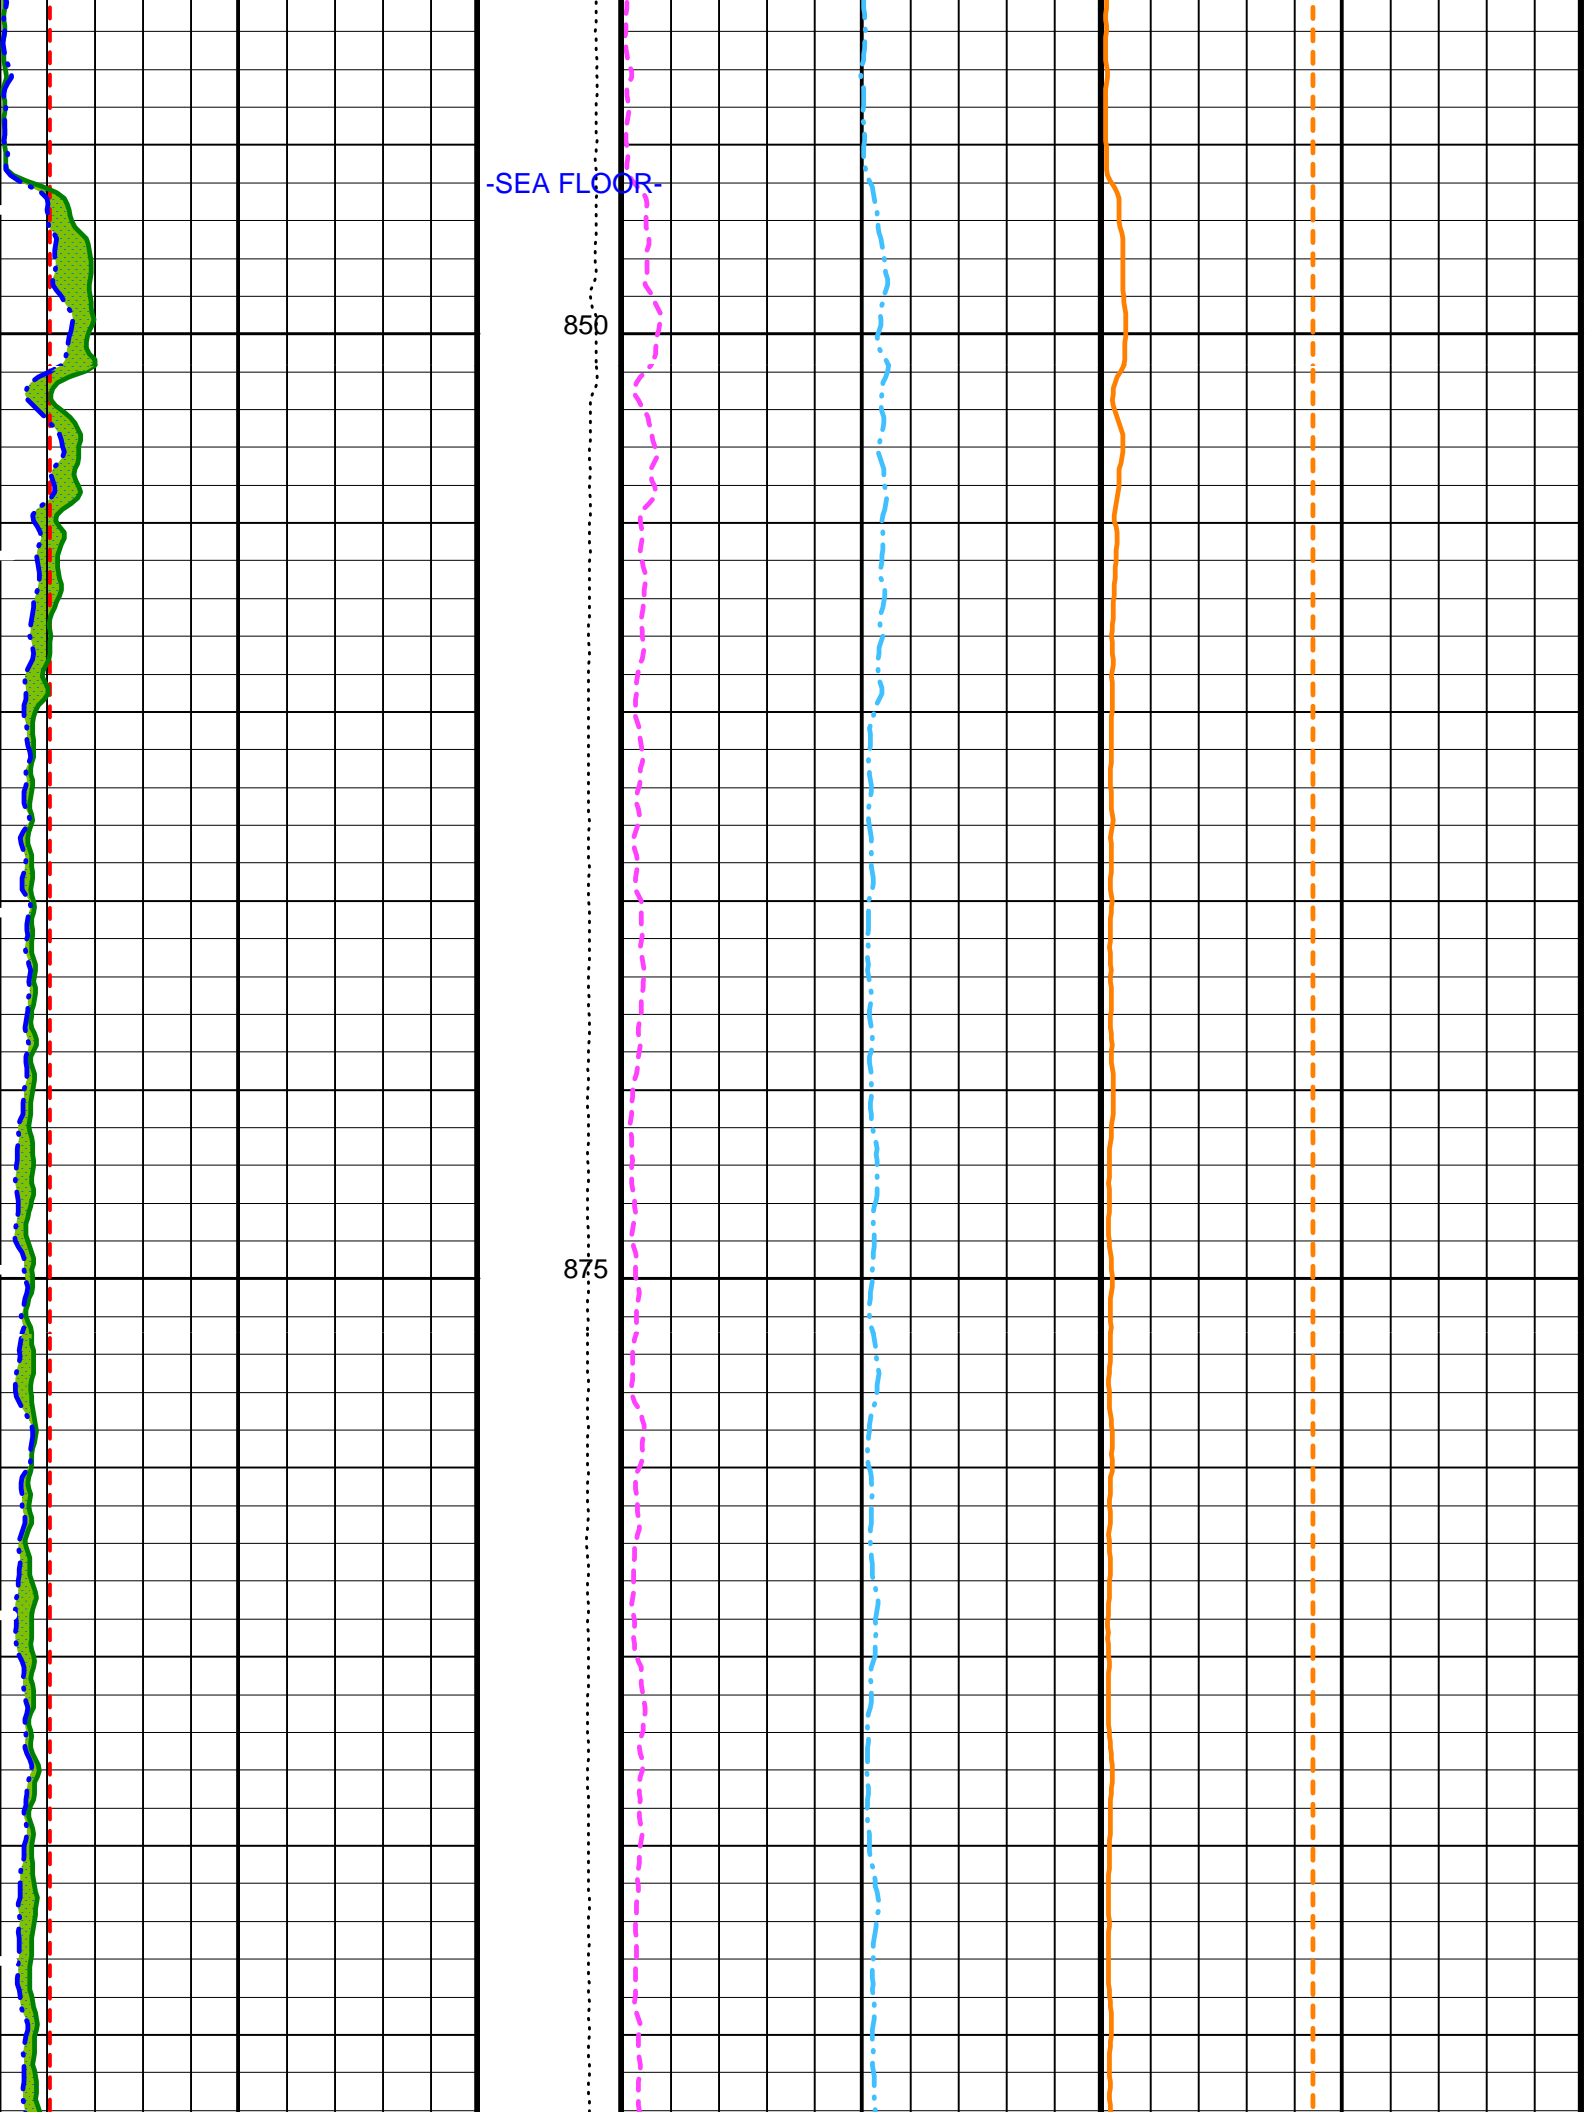

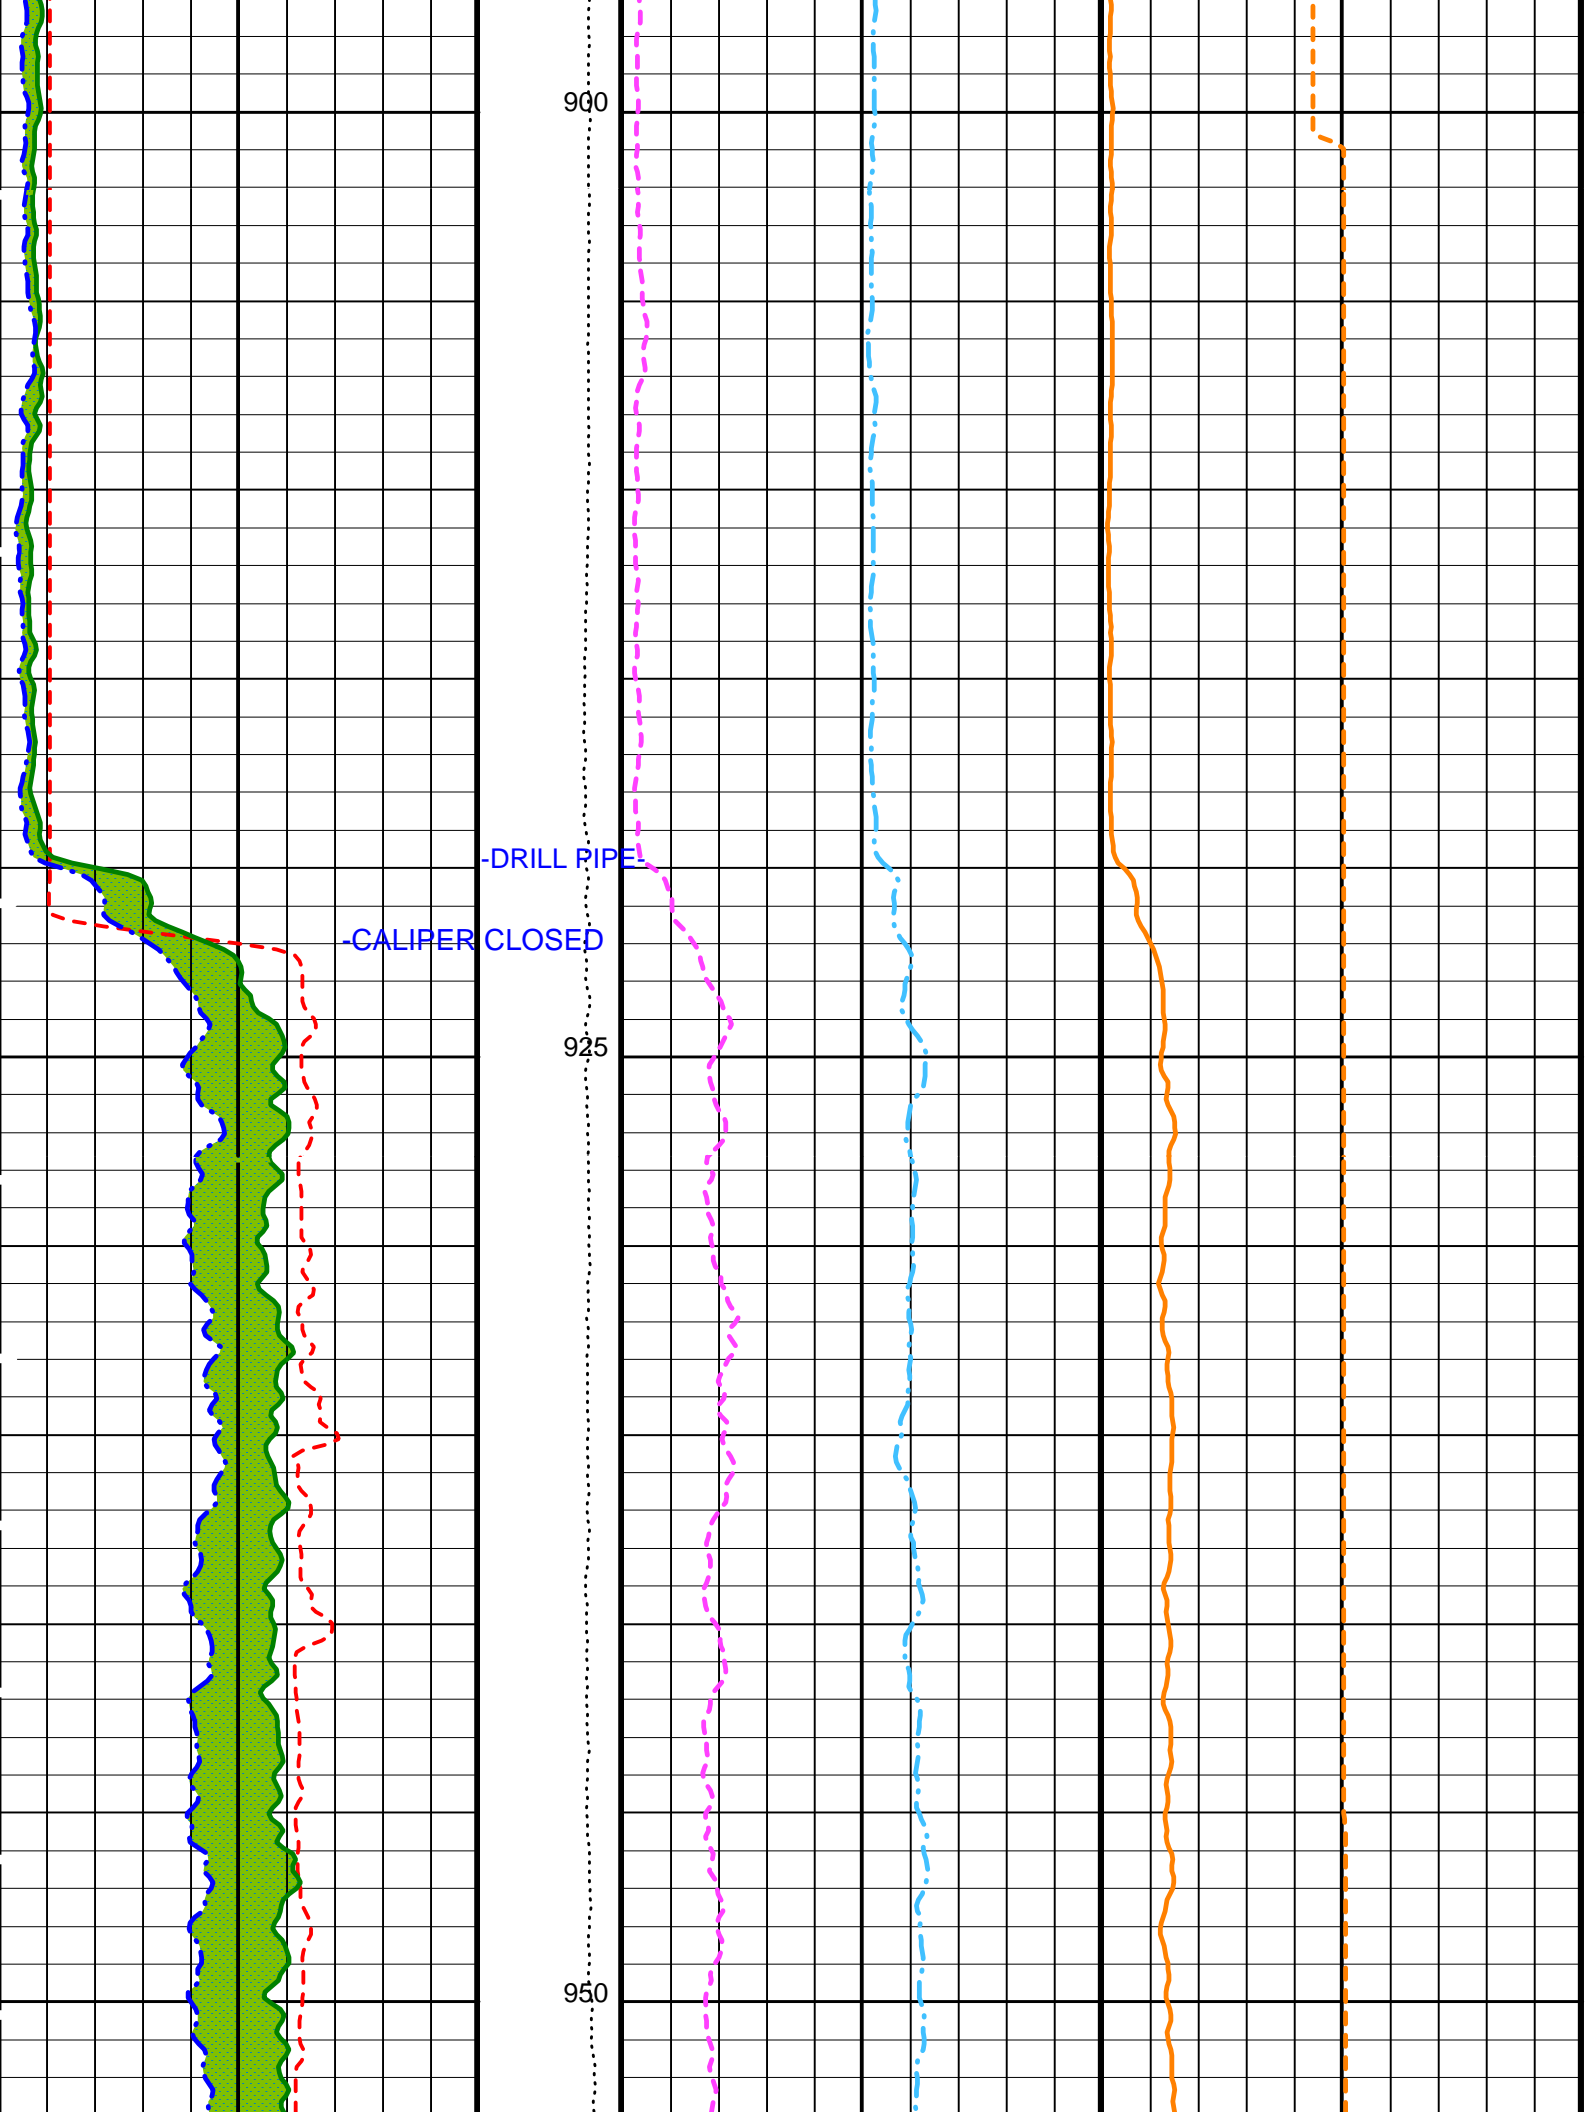

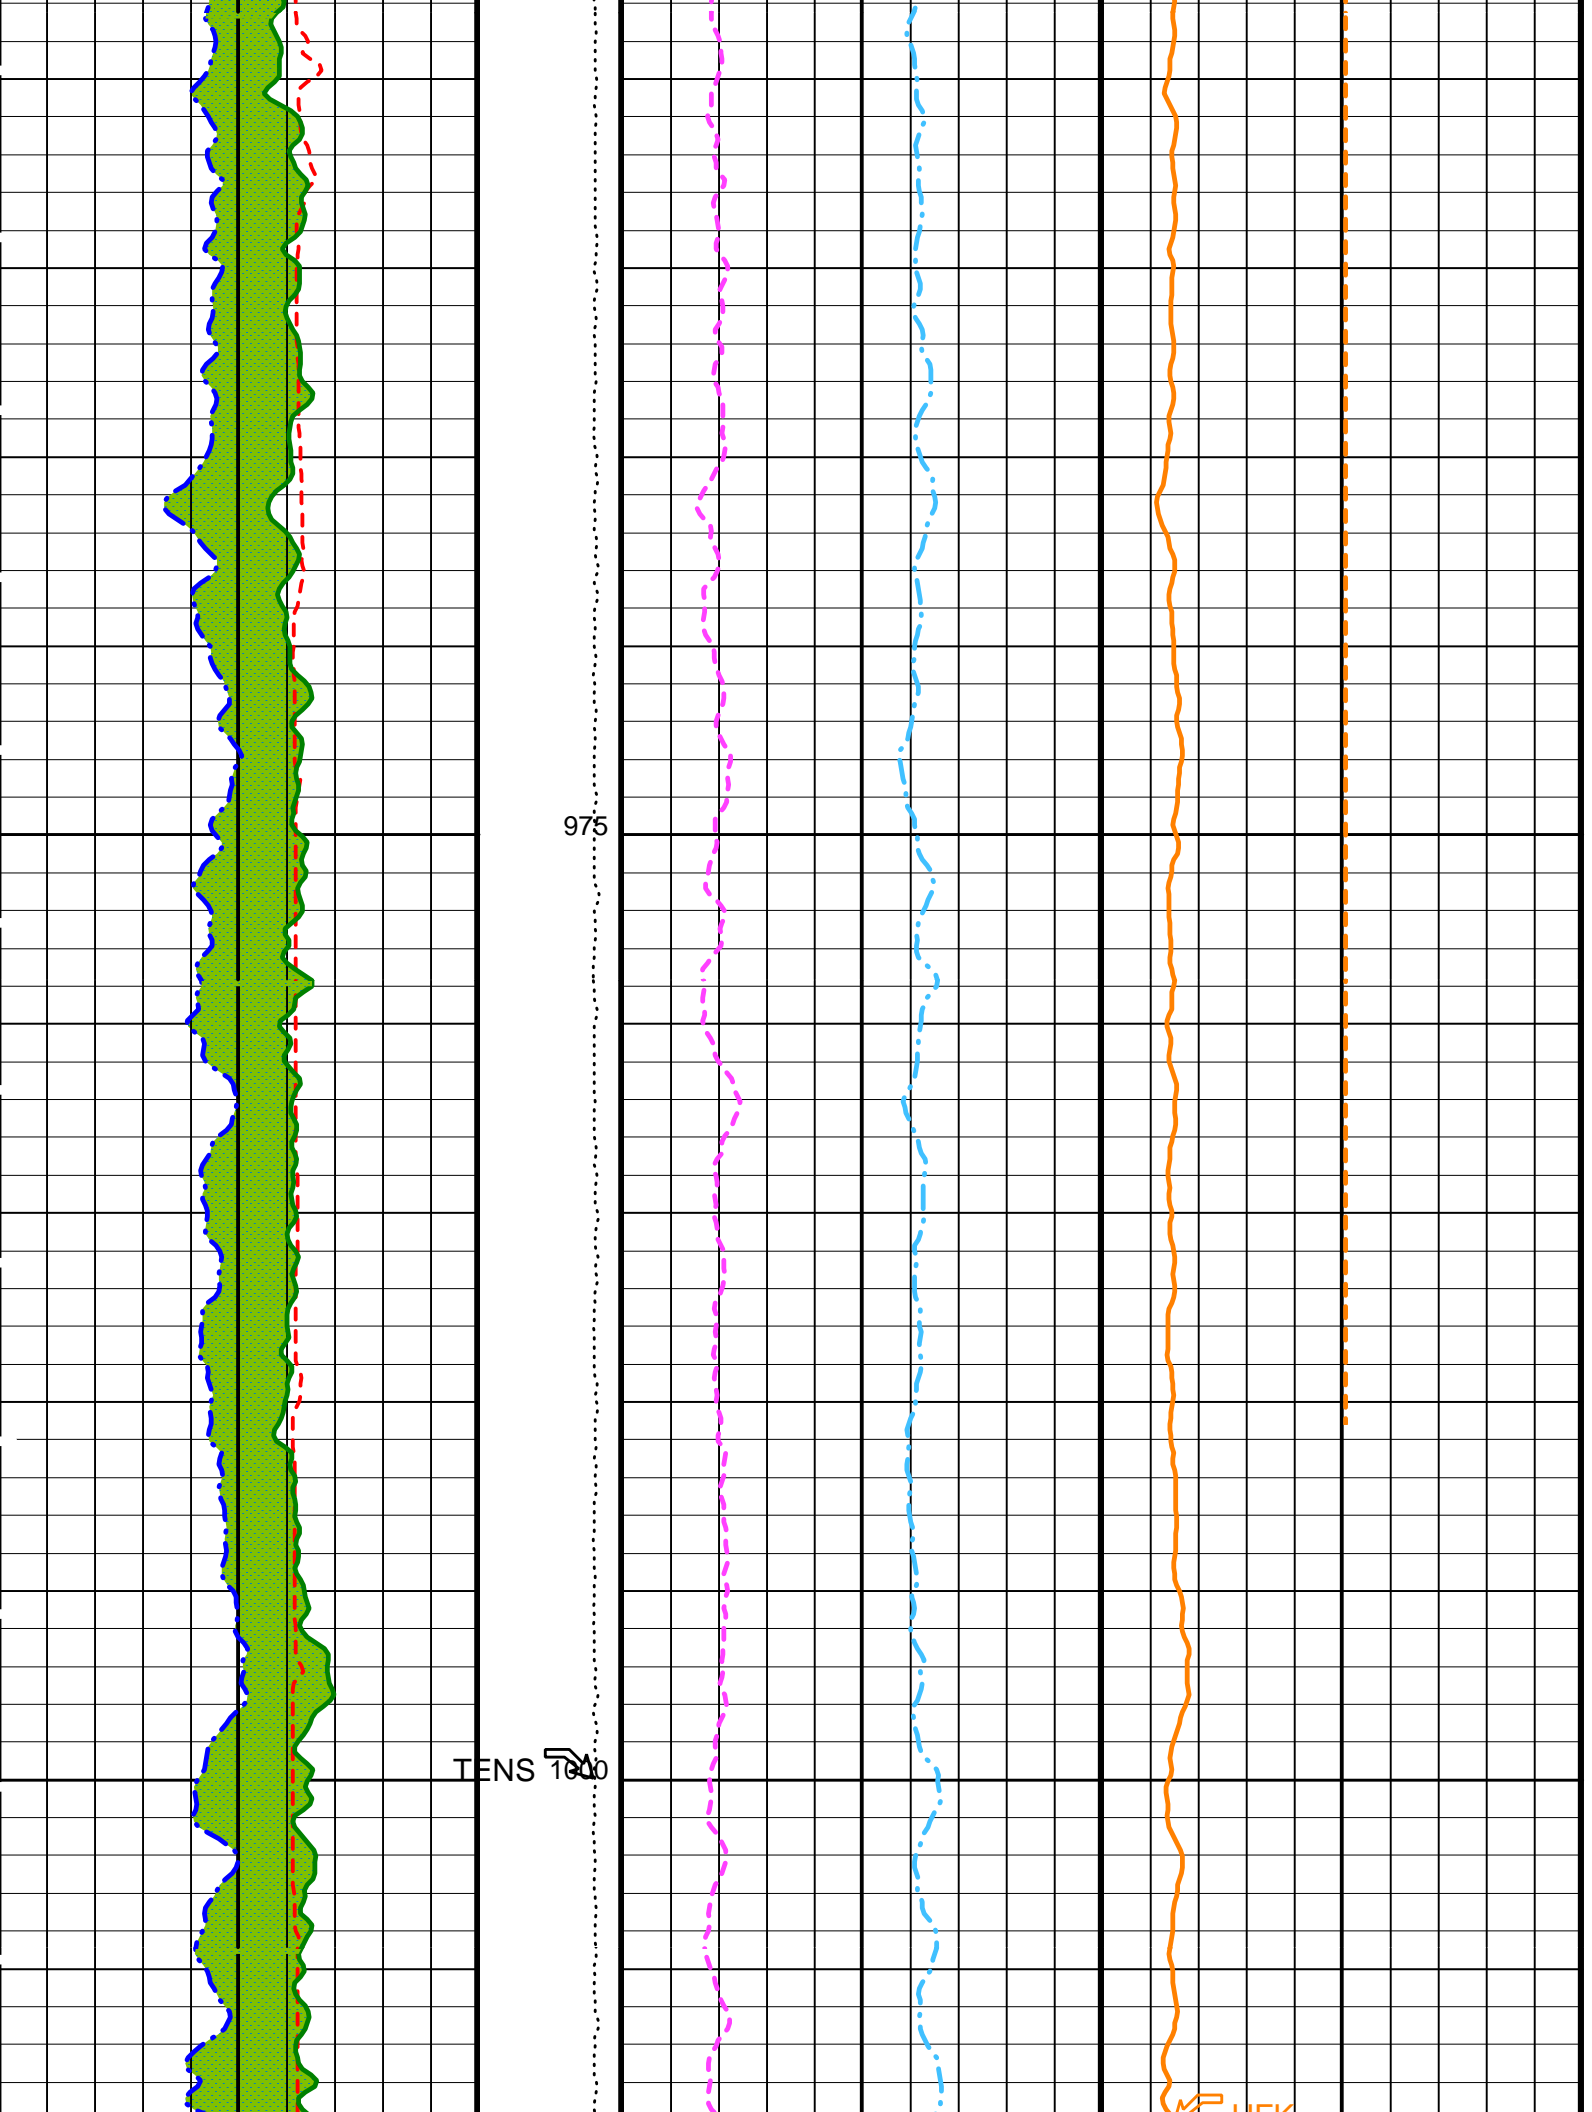

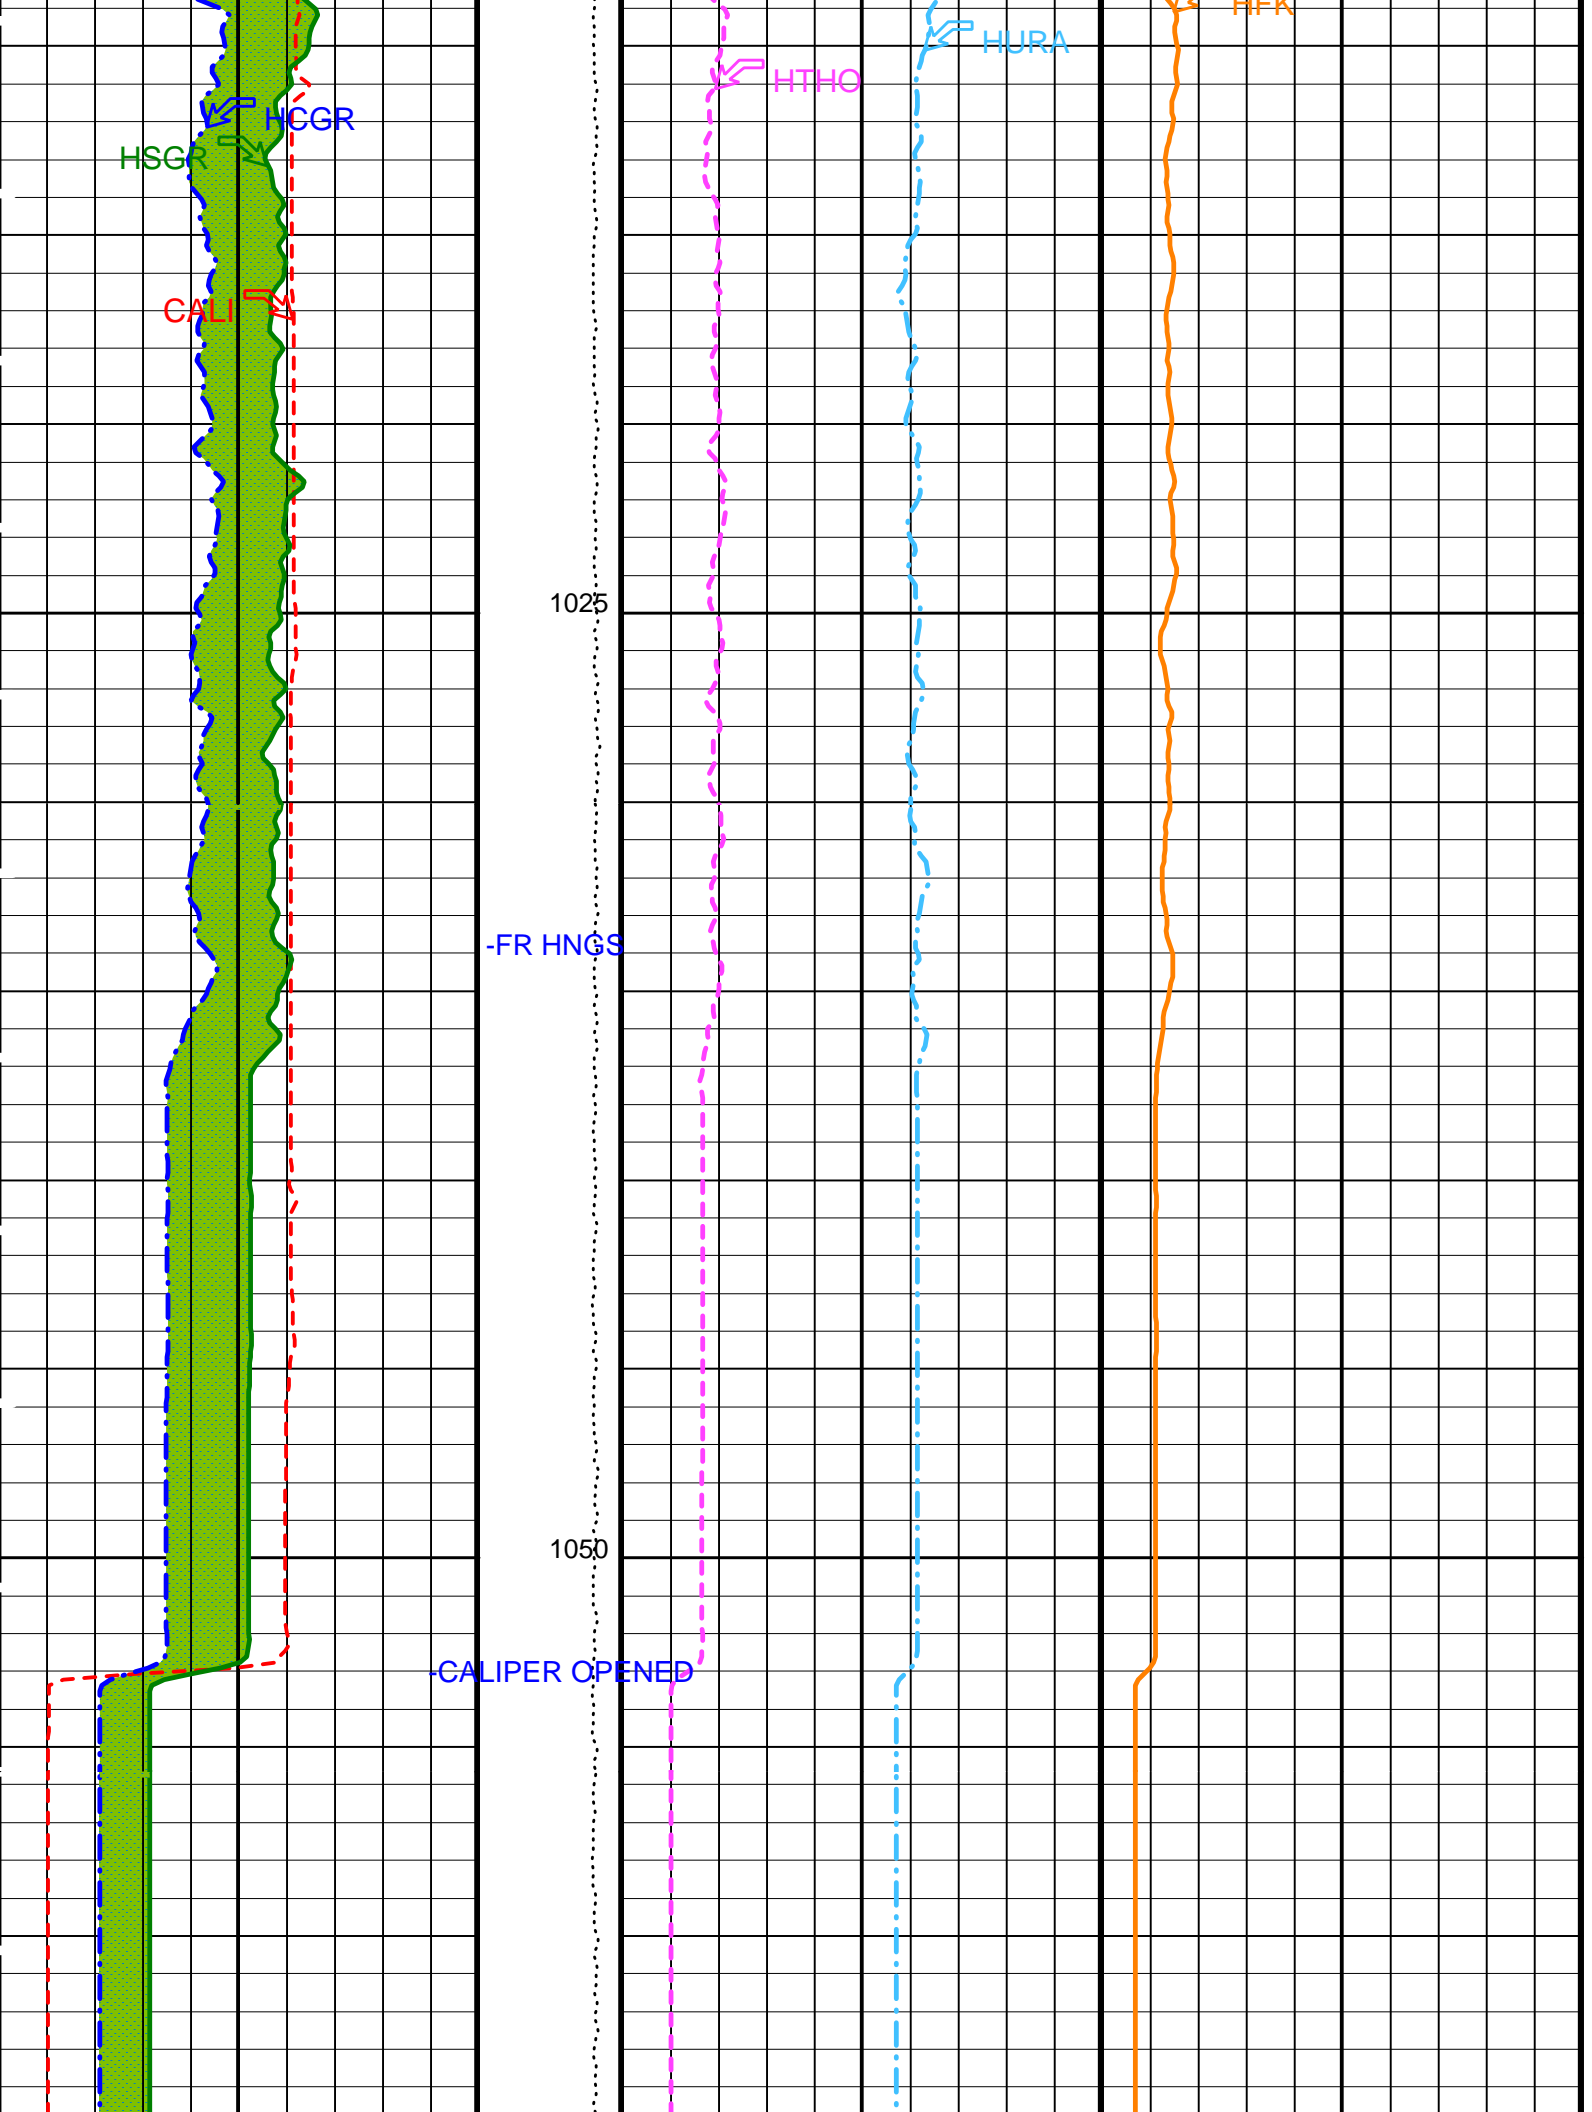

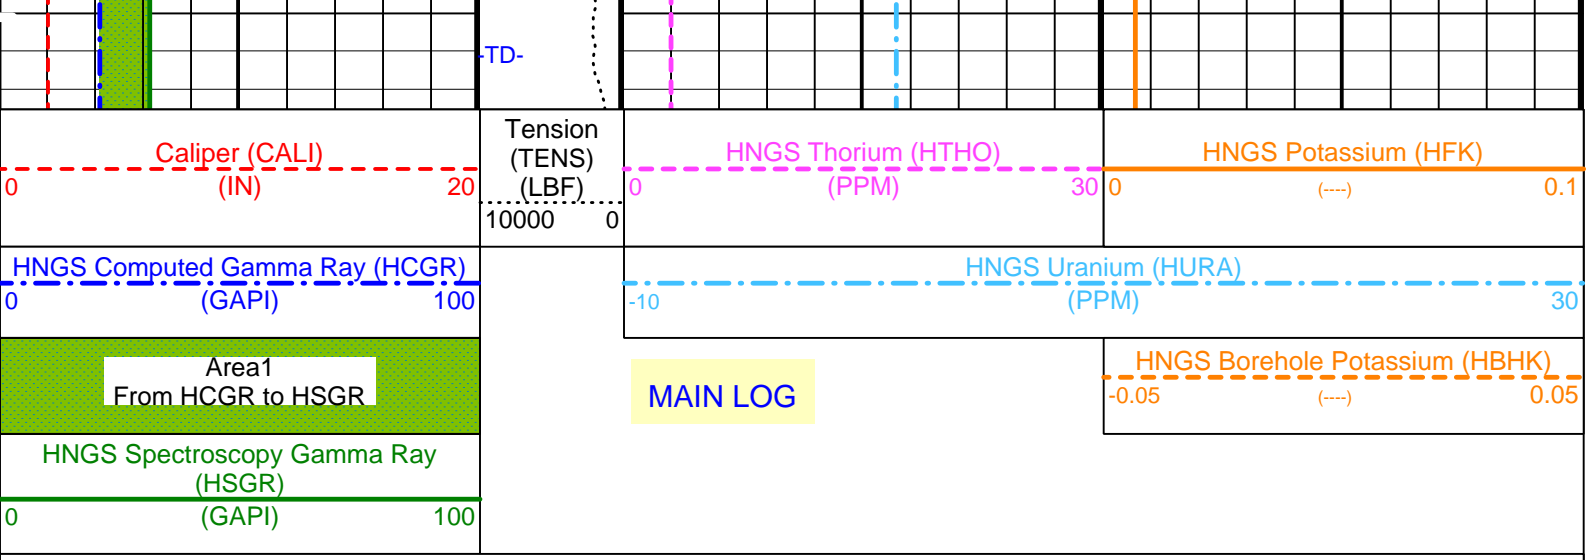

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value
DIT-E: Dual Induction - E		
BHS	Borehole Status	OPEN
GCSE	Generalized Caliper Selection	CALI
APS-BA: Accelerator-Porosity Tool		
BHS	Borehole Status	OPEN
GCSE	Generalized Caliper Selection	CALI
HNGS-BA: Hostile Natural Gamma Ray Sonde		
BAR1	HNGS Detector 1 Barite Constant	1
BAR2	HNGS Detector 2 Barite Constant	1
BHK	HNGS Borehole Potassium Correction Concentration	0
BHS	Borehole Status	OPEN
CSD1	Inner Casing Outer Diameter	0 IN
CSD2	Outer Casing Outer Diameter	0 IN
CSW1	Inner Casing Weight	0 LB/F
CSW2	Outer Casing Weight	0 LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE
GCSE	Generalized Caliper Selection	CALI
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW
HABK	HNGS Borehole Potassium Running Average	-0.00756454
HALF	HNGS Alpha Filter Length	60 IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE
HMWM	Mud Weighting Material	NATU
HNPE	HNGS Processing Enable	YES
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3 CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3 CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES
TPOS	Tool Position	ECCE
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.961934
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.981195
System and Miscellaneous		
BS	Bit Size	11.438 IN
DFD	Drilling Fluid Density	1.10 G/C3

Format: HNGSYields Vertical Scale: 1:200 Graphics File Created: 23-Aug-2002 18:58

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_004LUP	FN:4	PRODUCER	23-Aug-2002 18:58
REDUCE	PI_LDL_APS_NGS_004LUP	FN:5	PRODUCER	23-Aug-2002 18:58

Output DLIS Files


DEFAULT	PI_LDL_APS_NGS_005LUP	FN:6	PRODUCER	23-Aug-2002 19:51	1049.3 M	916.7 M
REDUCE	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	23-Aug-2002 19:51	1049.3 M	916.4 M


OP System Version: 10C0-306 MCM


DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

PIP SUMMARY

Time Mark Every 60 S

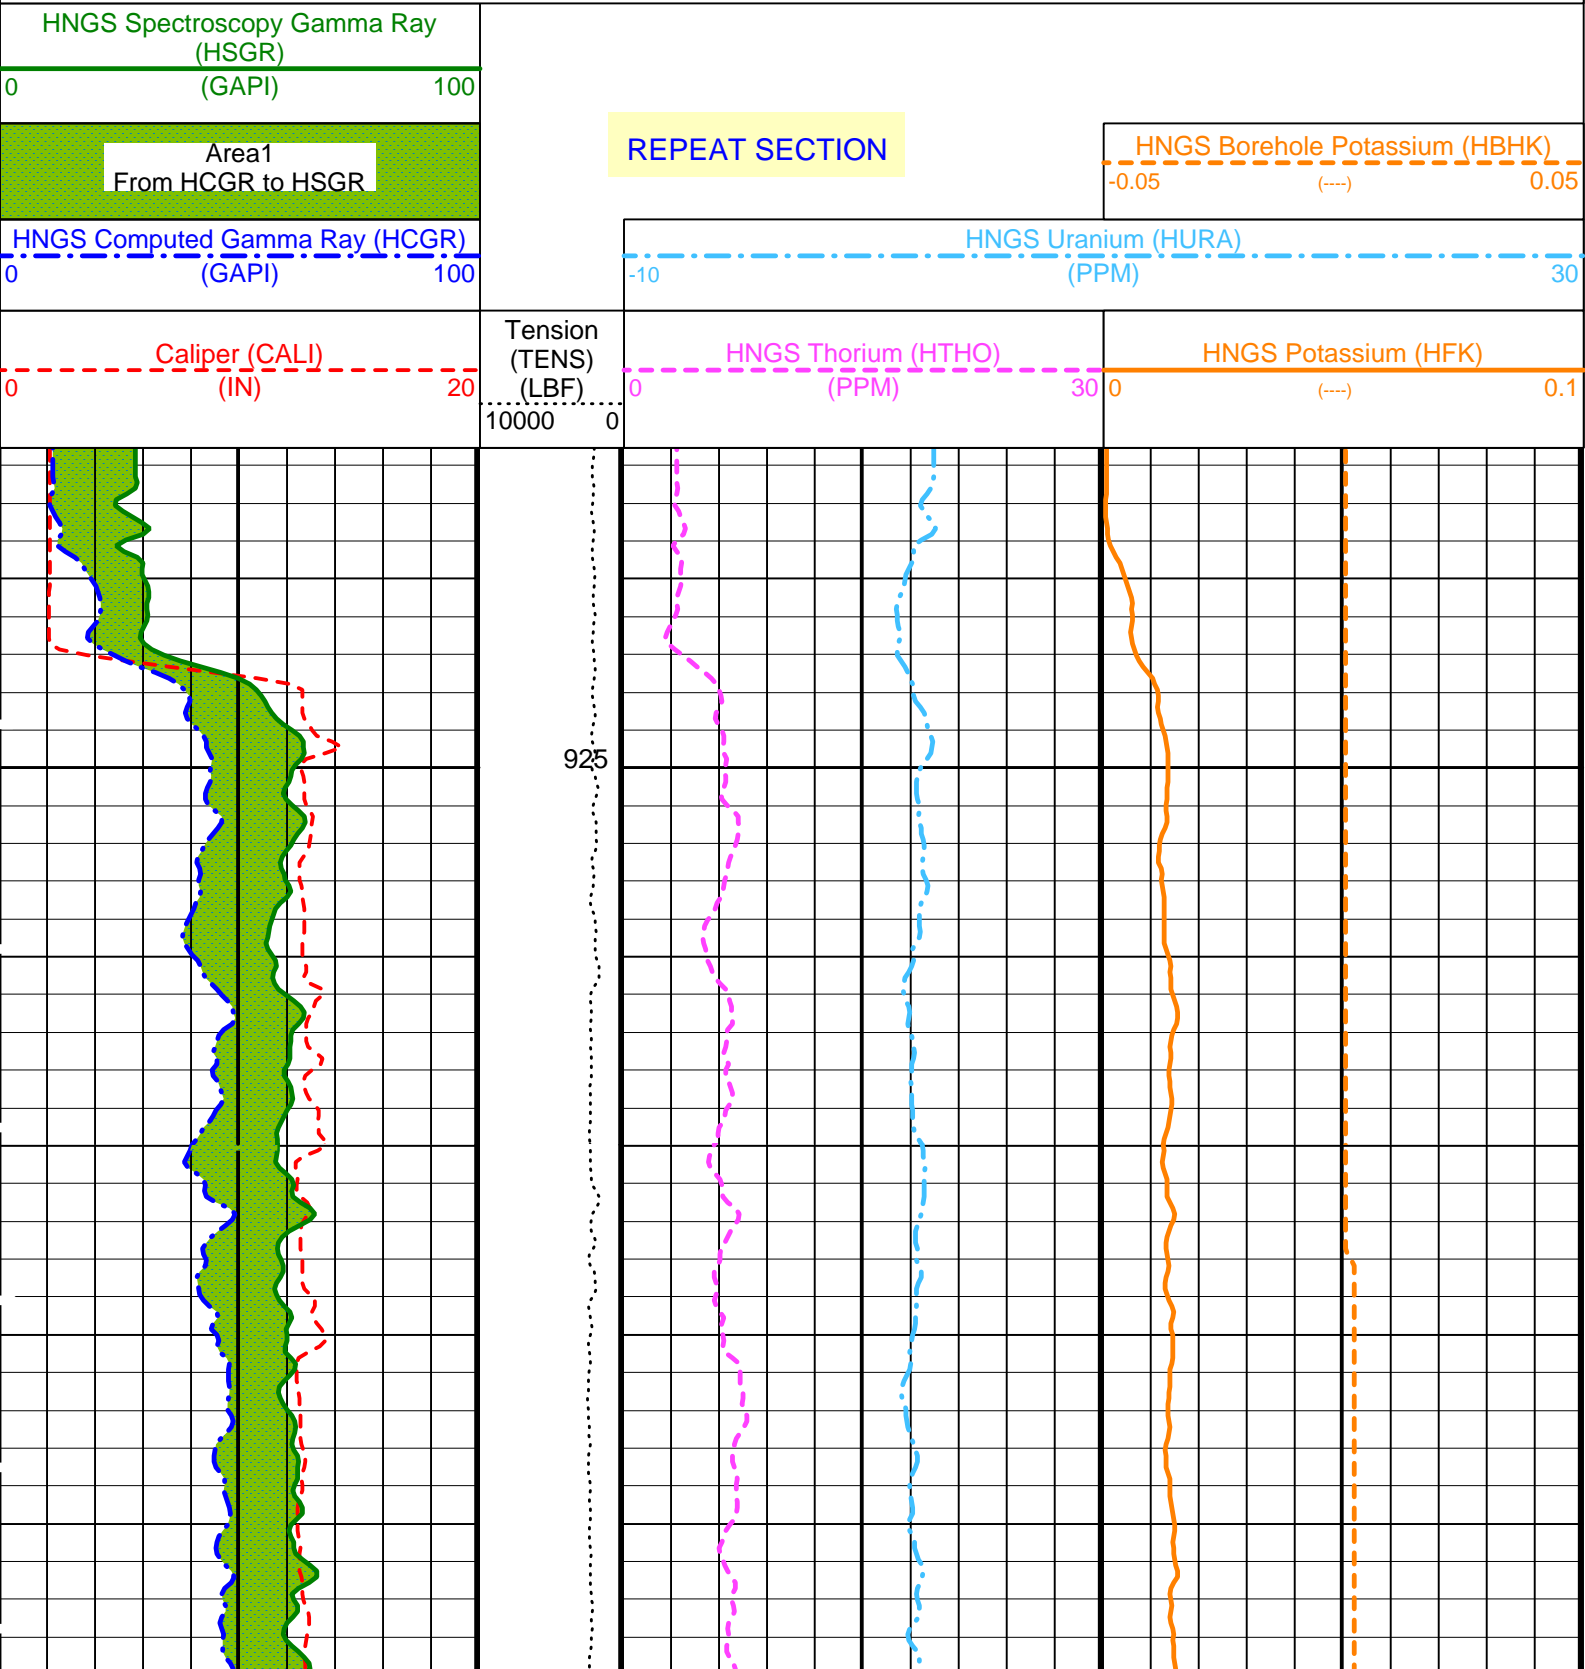

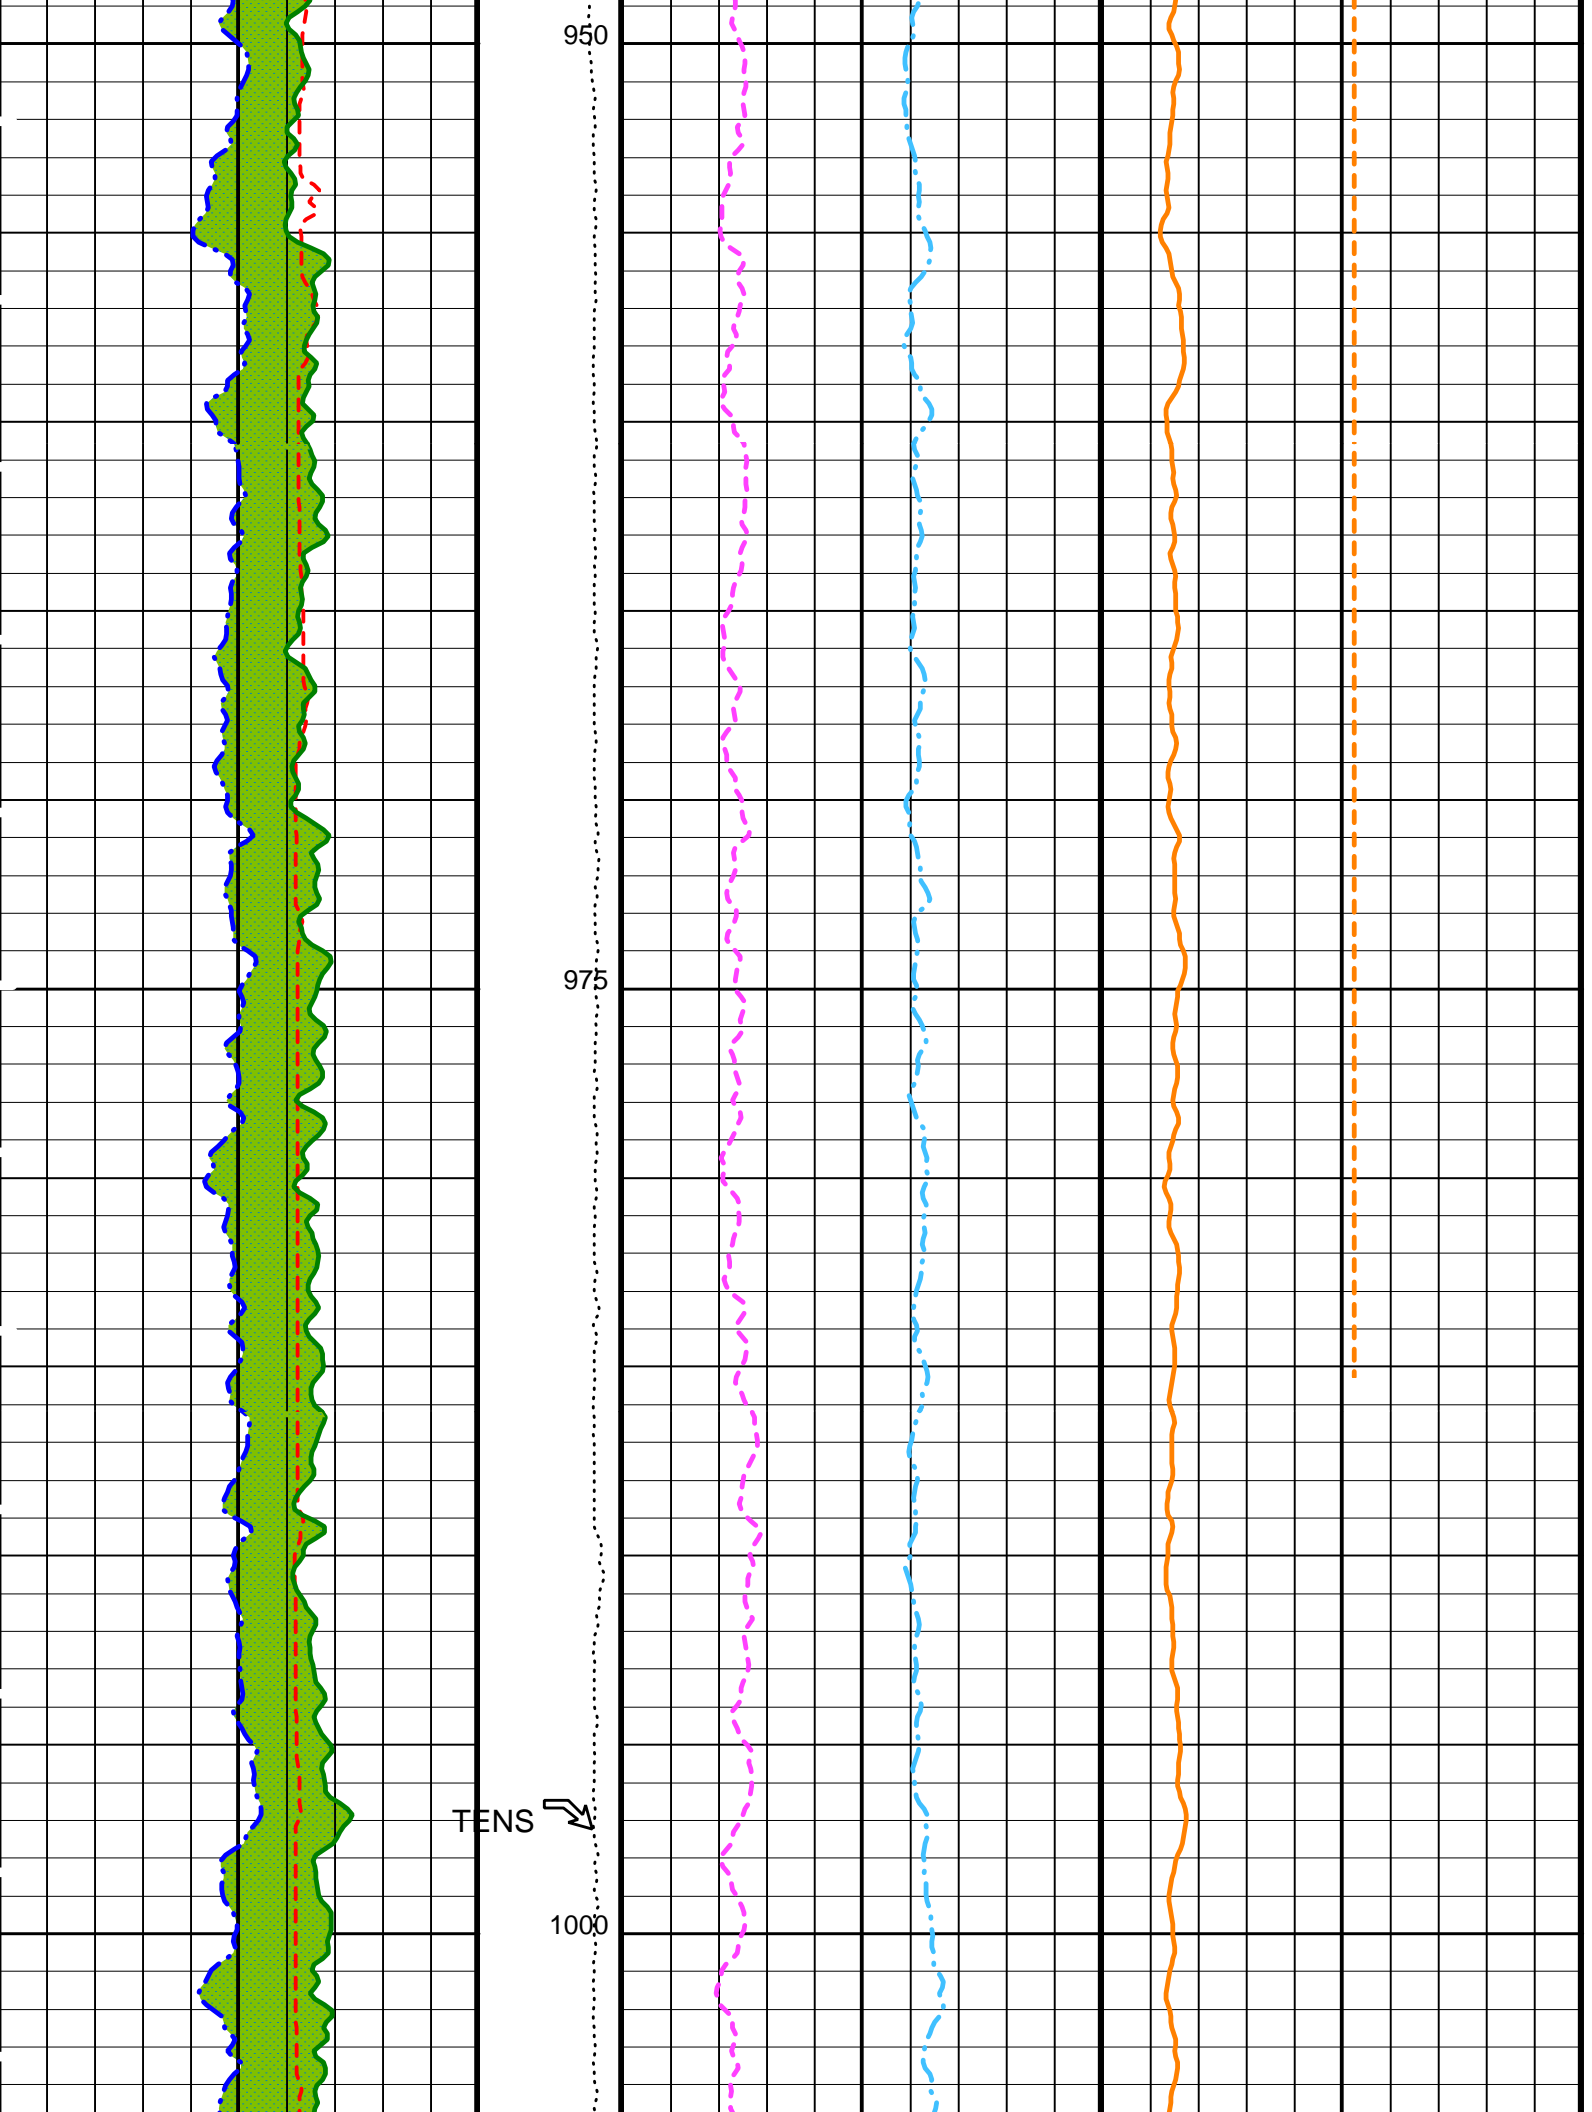

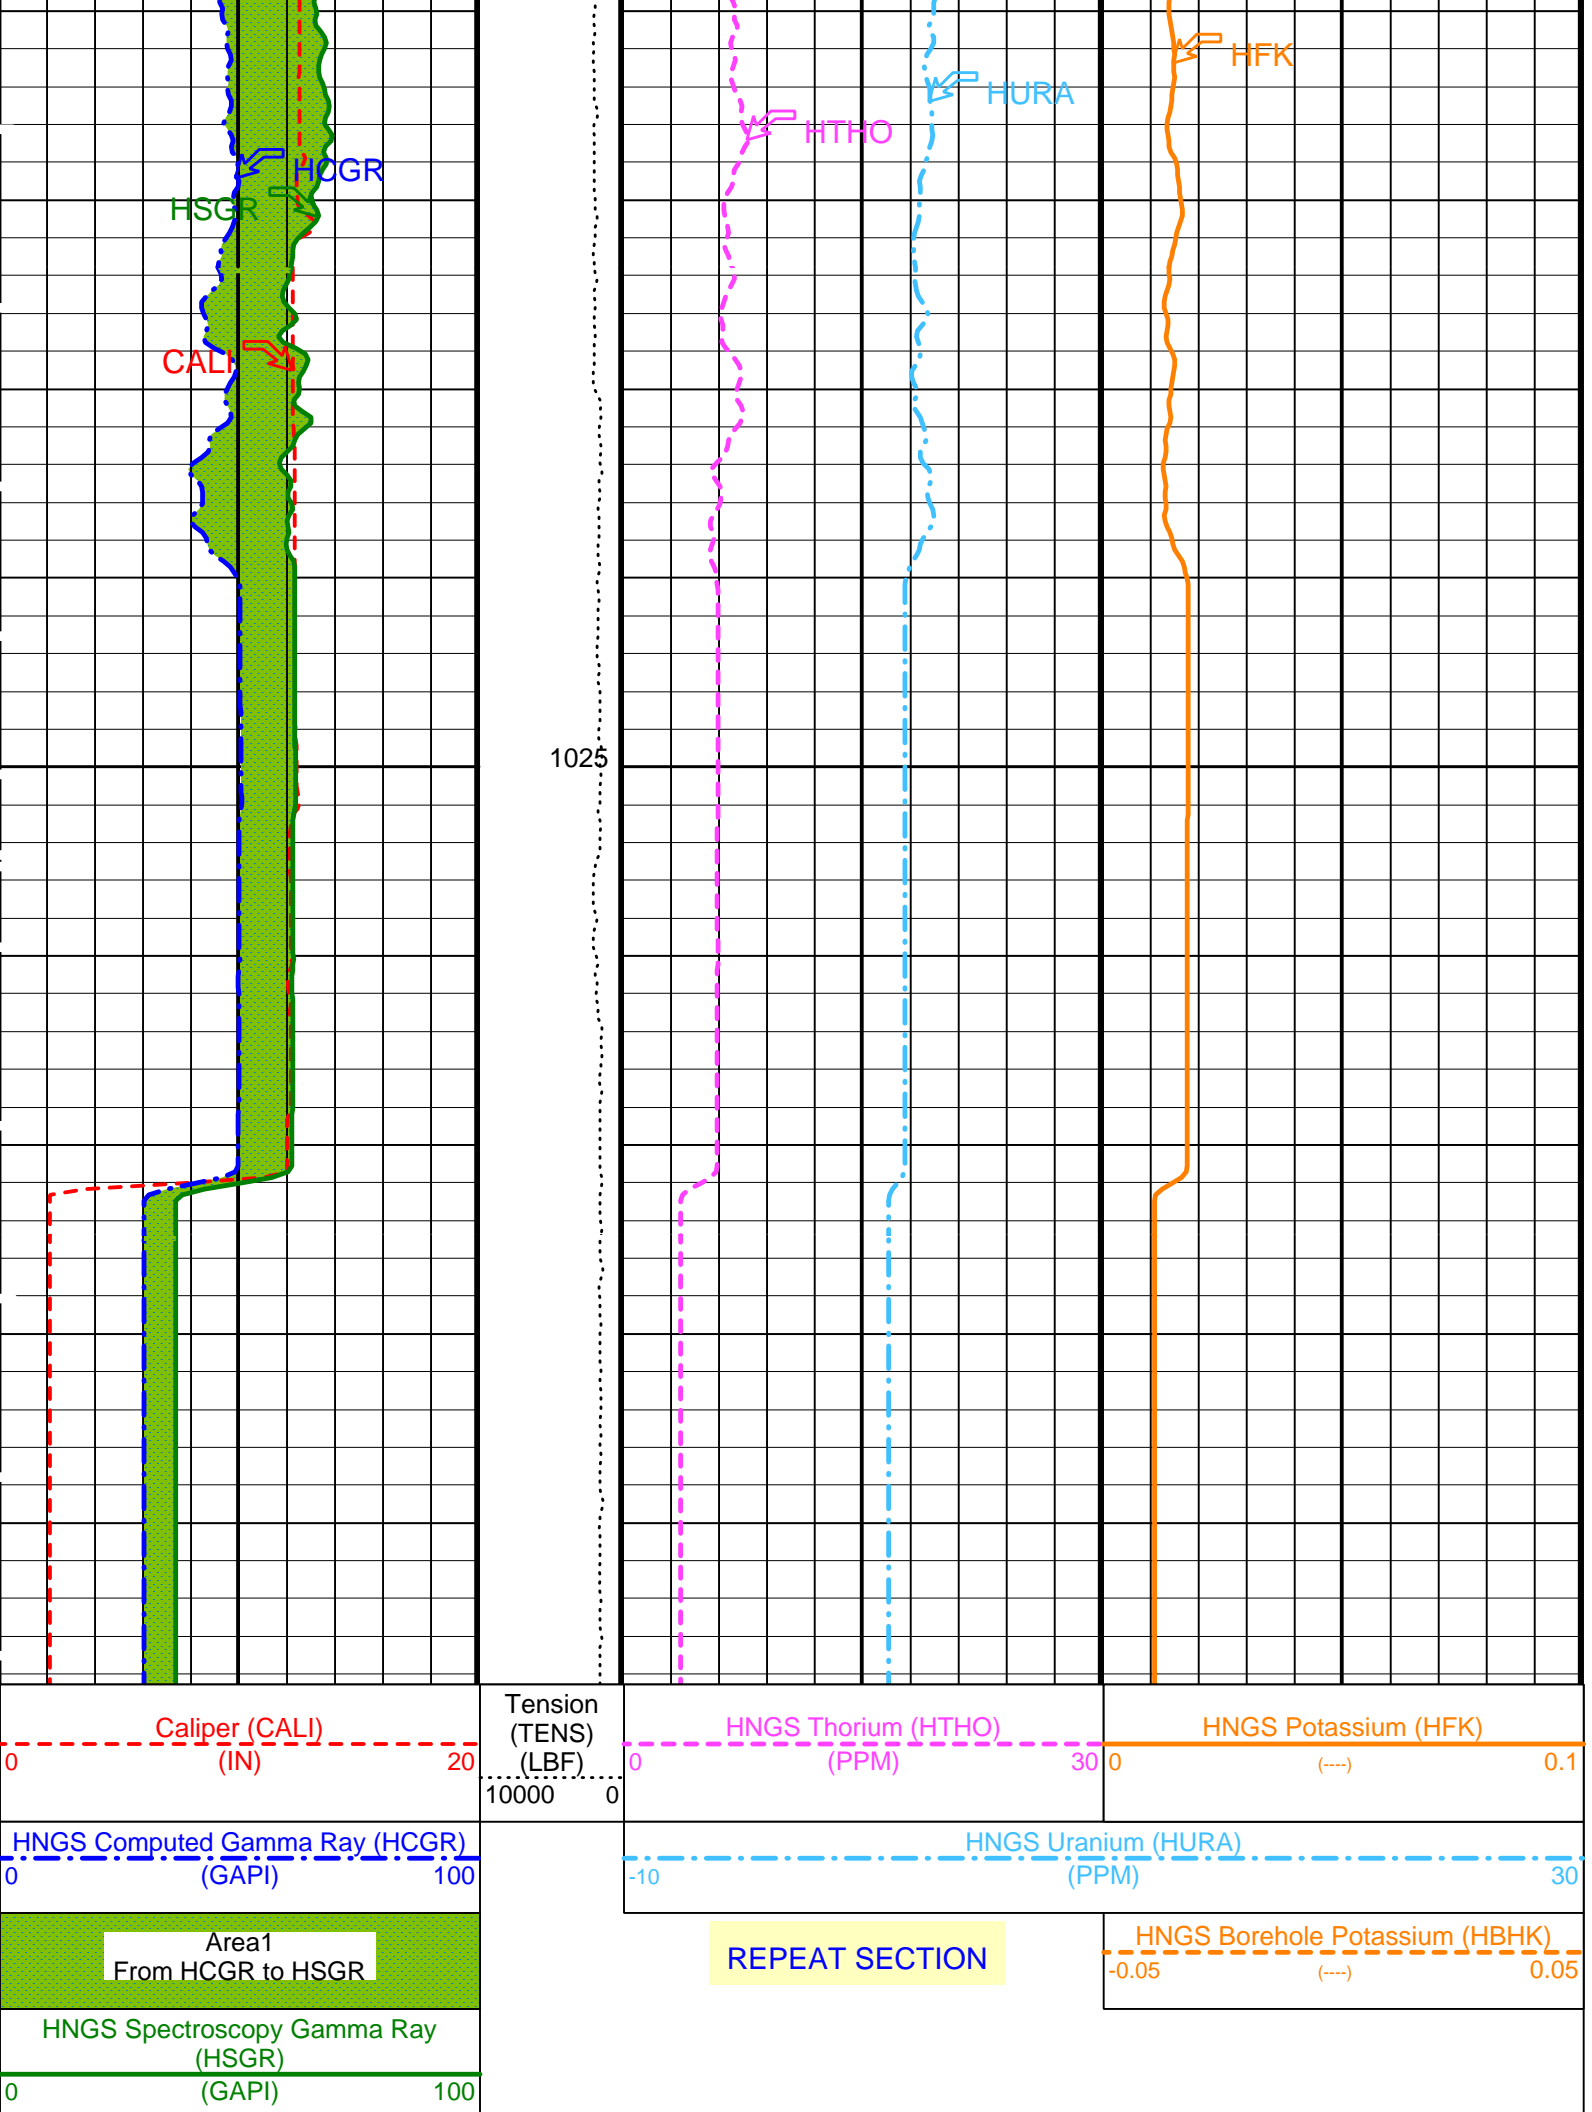

Parameters

DLIS Name	Description	Value	
DIT-E: Dual Induction - E			
BHS	Borehole Status	OPEN	
GCSE	Generalized Caliper Selection	CALI	
APS-BA: Accelerator-Porosity Tool			
BHS	Borehole Status	OPEN	
GCSE	Generalized Caliper Selection	CALI	
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	CALI	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.00221159	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	NATU	
HNPE	HNGS Processing Enable	YES	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
TPOS	Tool Position	ECCE	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.96978	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.972291	
System and Miscellaneous			
BS	Bit Size	11.438	IN
DFD	Drilling Fluid Density	1.10	G/C3

Format: HNGSYields Vertical Scale: 1:200 Graphics File Created: 23-Aug-2002 19:51

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_005LUP	FN:6	PRODUCER	23-Aug-2002 19:51
REDUCE	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	23-Aug-2002 19:51

Calibration and Check Summary

Measurement	Nominal	Master	Before	After	Change	Limit	Units
Hostile Environment Litho Density - A Wellsite Calibration - Background Measurement							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 23-Aug-2002 23:03							
LSW1 Background	100.0	88.67	86.74	85.83	-0.9071	0.03000	CPS
LSW2 Background	105.0	93.18	91.70	90.78	-0.9218	0.03000	CPS
LSW3 Background	210.0	177.4	176.2	176.7	0.5443	0.03000	CPS
LSW4 Background	290.0	236.8	236.6	234.4	-2.197	0.03000	CPS
LSW5 Background	610.0	518.0	517.3	519.9	2.595	0.03000	CPS
SSW1 Background	100.0	83.02	84.95	84.35	-0.5992	0.03000	CPS
SSW2 Background	200.0	165.1	166.3	165.2	-1.114	0.03000	CPS
SSW3 Background	530.0	440.7	439.6	438.1	-1.522	0.03000	CPS
SSW4 Background	280.0	232.4	232.4	233.4	0.9281	0.03000	CPS
SSW5 Background	205.0	174.0	173.3	174.7	1.441	0.03000	CPS

Hostile Environment Litho Density - A Wellsite Calibration - Tool Quality Control Information High Voltage

Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 23-Aug-2002 23:03								
LS Bkg. High Voltage	1133	1133	1130	1130	0.2719	N/A	V	
SS Bkg. High Voltage	1177	1177	1171	1170	-1.102	N/A	V	
Hostile Environment Litho Density - A Wellsite Calibration - Detectors Resolution From BKG Measurements								
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 23-Aug-2002 23:03								
LS Background Resolution	1.000	1.032	1.032	1.025	-0.007081	N/A		
SS Background Resolution	1.000	0.9430	0.9416	0.9411	-0.0004674	N/A		
Hostile Environment Litho Density - A Wellsite Calibration - Caliper Calibration								
Before: 24-Jul-2002 17:38								
Caliper Small Ring	12.00	N/A	17.14	N/A	N/A	N/A	IN	
Caliper Large Ring	15.25	N/A	21.07	N/A	N/A	N/A	IN	
Accelerator-Porosity Tool Wellsite Calibration - Detector Background								
Master: 24-Jul-2002 9:08 Before: 23-Aug-2002 19:57 After: 23-Aug-2002 22:14								
Near Det Bkg Cntrate	30.00	32.30	32.20	31.59	-0.6166	N/A	CPS	
Far Det Bkg Cntrate	30.00	33.62	32.72	35.16	2.440	N/A	CPS	
Array-1 Det Bkg Cntrate	30.00	28.88	29.71	28.05	-1.661	N/A	CPS	
Array-2 Det Bkg Cntrate	30.00	29.64	29.69	30.36	0.6743	N/A	CPS	
Array Therm Det Bkg Cntrate	30.00	32.75	32.67	32.93	0.2644	N/A	CPS	
Accelerator-Porosity Tool Wellsite Calibration - Calibration Ratios								
Master: 24-Jul-2002 9:08								
Near/Far Calibration Ratio	0.9250	0.9076	N/A	N/A	N/A	N/A		
Near/Array Calibration Ratio	1.030	1.066	N/A	N/A	N/A	N/A		
Near/Array Cal Ratio Up/Down	1.000	1.006	N/A	N/A	N/A	N/A		
Accelerator-Porosity Tool Wellsite Calibration - Tank Check								
Master: 24-Jul-2002 9:09								
Array-1 Standoff Porosity	11.75	11.51	N/A	N/A	N/A	N/A	PU	
Array-2 Standoff Porosity	11.75	11.19	N/A	N/A	N/A	N/A	PU	
Average Slowing Down Time	6.000	5.884	N/A	N/A	N/A	N/A	US	
Array-1 SDT Ratio Up/Down	1.000	0.9901	N/A	N/A	N/A	N/A		
Array-2 SDT Ratio Up/Down	1.000	0.9732	N/A	N/A	N/A	N/A		
Sigma Formation	27.50	27.88	N/A	N/A	N/A	N/A	CU	
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 1 Check								
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 23-Aug-2002 23:04								
Na 511 Peak Loc	40.00	40.59	40.60	40.55	-0.05260	1.000		
Na 511 Peak Res	15.50	16.79	16.89	15.90	-0.9905	2.000	%	
High Voltage	1150	1224	1220	1219	-1.110	30.00	V	
Na 1785 Peak Loc	142.6	145.1	146.3	145.5	-0.7973	7.000		
Na 1785 Peak Res	8.500	10.40	8.694	9.747	1.053	2.000	%	
Temperature	15.50	24.98	22.43	20.41	-2.013	N/A	DEGC	
Na Count Rate	45.00	50.31	49.89	48.96	-0.9234	8.000	CPS	
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 2 Check								
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 23-Aug-2002 23:04								
Na 511 Peak Loc	40.00	40.58	40.59	40.59	0.001343	1.000		
Na 511 Peak Res	15.50	16.72	16.53	16.53	-0.003351	2.000	%	
High Voltage	1150	1253	1250	1246	-3.410	30.00	V	
Na 1785 Peak Loc	142.6	144.7	144.3	144.8	0.4459	7.000		
Na 1785 Peak Res	8.500	9.766	9.897	9.612	-0.2849	2.000	%	
Temperature	15.50	24.15	21.87	20.67	-1.203	N/A	DEGC	
Na Count Rate	45.00	50.19	49.39	48.77	-0.6201	8.000	CPS	
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Ratio Of Detector 1 To Detector 2								
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 23-Aug-2002 23:04								
Coincidence Count Rate Ratio	1.000	1.004	1.010	1.003	-0.006575	0.05000		
Hostile Natural Gamma Ray Sonde Master Calibration - Detector 1 Calibration								
Master: 13-Jul-2002 3:01								
Na 511 Peak Set Point	40.00	41.00	--	--	--	--		
Th Peak Loc	209.6	208.9	--	--	--	--		
Th Peak Res	7.000	8.227	--	--	--	--	%	
Background Count Rate	142.5	24.67	--	--	--	--	CPS	
Gain Ratio	1.000	0.9793	--	--	--	--		
Hostile Natural Gamma Ray Sonde Master Calibration - Detector 2 Calibration								
Master: 13-Jul-2002 3:01								
Na 511 Peak Set Point	40.00	41.00	--	--	--	--		
Th Peak Loc	209.6	208.8	--	--	--	--		
Th Peak Res	7.000	8.191	--	--	--	--	%	
Background Count Rate	142.5	22.68	--	--	--	--	CPS	
Gain Ratio	1.000	0.9792	--	--	--	--		

Accelerator-Porosity Tool - Detector Plateau Settings :

Near Detector Plateau Setting 1748 V

Far Detector Plateau Setting 2052 V
 Array Detector Plateau Setting 1969 V

Dual Induction - E / Equipment Identification

Primary Equipment:		
Dual Induction Sonde	DIS - HB	442
Dual Induction Cartridge	DIC - EB	438
Auxiliary Equipment:		
Mass Isolated Housing	MIH - ZA	417

Hostile Environment Litho Density - A / Equipment Identification

Primary Equipment:		
HOSTILE ENVIRONMENT LITHO DENSITY HIGH V	HLDV - A	10
HOSTILE ENVIRONMENT LITHO DENSITY CARTRI	HLDC - AA	11
Gamma Source Radioactive	GSR - Z	1846
Auxiliary Equipment:		
HOSTILE ENVIRONMENT LITHO DENSITY SONDE	HLDS - B	10
HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG	HEH - H	12
HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG	HEH - G	11
HOSTILE ENVIRONMENT LITHO DENSITY PAD	HLDP - B	10

Nuclear Porosity Lithology Cartridge - B / Equipment Identification

Primary Equipment:		
NPLC Cartridge	NPLC - B	79
Auxiliary Equipment:		
NPLC Housing	NPH - B	82

Accelerator-Porosity Tool / Equipment Identification

Primary Equipment:		
Accelerator-Porosity Sonde	APS - BA	22
APS Minitron	MNTR - F	4185
Auxiliary Equipment:		
Accelerator-Porosity Housing	APH - AC	22
APS Calibration Water Tank	SFT - 178	4722
APS Aluminium Calibrator Sleeve	SFT - 281	24

Hostile Natural Gamma Ray Sonde / Equipment Identification

Primary Equipment:		
HNGS Sonde	HNGS - BA	77
Auxiliary Equipment:		
HNGS Sonde Housing	HNSH - BA	79
Gamma Source Radioactive	GSR - U	135

Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 1 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.59	Master		16.79	Master		1224
Before		40.60	Before		16.89	Before		1220
After		40.55	After		15.90	After		1219
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	

Na 1785 Peak Loc			Na 1785 Peak Res %			Temperature DEGC		
Phase	Value	Value	Phase	Value	Phase	Value	Value	Value
Master	145.1	145.1	Master	10.40	Master	24.98	24.98	24.98
Before	146.3	146.3	Before	8.694	Before	22.43	22.43	22.43
After	145.5	145.5	After	9.747	After	20.41	20.41	20.41
	135.0 (Minimum)	150.3 (Maximum)		7.000 (Minimum)	11.00 (Maximum)		-28.89 (Minimum)	60.00 (Maximum)
Na Count Rate CPS								
Phase	Value	Value						
Master	50.31	50.31						
Before	49.89	49.89						
After	48.96	48.96						
	10.00 (Minimum)	100.0 (Maximum)						
Master: 13-Jul-2002 3:08			Before: 24-Jul-2002 12:59			After: 23-Aug-2002 23:04		






Hostile Natural Gamma Ray Sonde Wellsite Calibration								
Detector 2 Check								
Na 511 Peak Loc			Na 511 Peak Res %			High Voltage V		
Phase	Value	Value	Phase	Value	Phase	Value	Value	Value
Master	40.58	40.58	Master	16.72	Master	1253	1253	1253
Before	40.59	40.59	Before	16.53	Before	1250	1250	1250
After	40.59	40.59	After	16.53	After	1246	1246	1246
	37.50 (Minimum)	42.50 (Maximum)		12.00 (Minimum)	19.00 (Maximum)		900.0 (Minimum)	1600 (Maximum)
Na 1785 Peak Loc			Na 1785 Peak Res %			Temperature DEGC		
Phase	Value	Value	Phase	Value	Phase	Value	Value	Value
Master	144.7	144.7	Master	9.766	Master	24.15	24.15	24.15
Before	144.3	144.3	Before	9.897	Before	21.87	21.87	21.87
After	144.8	144.8	After	9.612	After	20.67	20.67	20.67
	135.0 (Minimum)	150.3 (Maximum)		7.000 (Minimum)	11.00 (Maximum)		-28.89 (Minimum)	60.00 (Maximum)
Na Count Rate CPS								
Phase	Value	Value						
Master	50.19	50.19						
Before	49.39	49.39						
After	48.77	48.77						
	10.00 (Minimum)	100.0 (Maximum)						
Master: 13-Jul-2002 3:08			Before: 24-Jul-2002 12:59			After: 23-Aug-2002 23:04		

Hostile Natural Gamma Ray Sonde Wellsite Calibration		
Ratio Of Detector 1 To Detector 2		
Phase	Coincidence Count Rate Ratio	Value
Master	1.004	1.004
Before	1.010	1.010
After	1.003	1.003
	0.9500 (Minimum)	1.050 (Maximum)
Master: 13-Jul-2002 3:08		
Before: 24-Jul-2002 12:59		
After: 23-Aug-2002 23:04		

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 1 Calibration								
Na 511 Peak Set Point			Th Peak Loc			Th Peak Res %		
Phase	Value	Value	Phase	Value	Phase	Value	Value	Value
Master	41.00	41.00	Master	208.9	Master	8.227	8.227	8.227
	38.00 (Minimum)	42.00 (Maximum)		201.0 (Minimum)	218.3 (Maximum)		5.000 (Minimum)	9.000 (Maximum)
Background Count Rate CPS			Gain Ratio					
Phase	Value	Value	Phase	Value				
Master	24.67	24.67	Master	0.9793				
	20.00 (Minimum)	265.0 (Maximum)		0.9400 (Minimum)	1.060 (Maximum)			
Master: 13-Jul-2002 3:01								

Hostile Natural Gamma Ray Sonde Master Calibration

Detector 2 Calibration

Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value	
Master		41.00	Master		208.8	Master		8.191	
	38.00 (Minimum)	40.00 (Nominal)	42.00 (Maximum)	201.0 (Minimum)	209.6 (Nominal)	218.3 (Maximum)	5.000 (Minimum)	7.000 (Nominal)	9.000 (Maximum)
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value				
Master		22.68	Master		0.9792				
	20.00 (Minimum)	142.5 (Nominal)	265.0 (Maximum)	0.9400 (Minimum)	1.000 (Nominal)	1.060 (Maximum)			

Master: 13-Jul-2002 3:01

Company: Lamont Doherty
 Well: ODP Leg 204, Site 1247B
 Field: Hydrate Ridge
 Ocean: Pacific
 State: Oregon



Natural Gamma Ray
 Spectroscopy