

MAXIMUM STRING DIAMETER 3.88 IN
 MEASUREMENTS RELATIVE TO TOOL ZERO
 ALL LENGTHS IN METERS

Output DLIS Files


DEFAULT	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	25-Aug-2002 21:57	985.3 M	784.1 M
REDUCE	PI_LDL_APS_NGS_005LUP	FN:8	PRODUCER	25-Aug-2002 21:57	985.3 M	784.0 M


OP System Version: 10C0-306 MCM


DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		


PIP SUMMARY


Time Mark Every 60 S

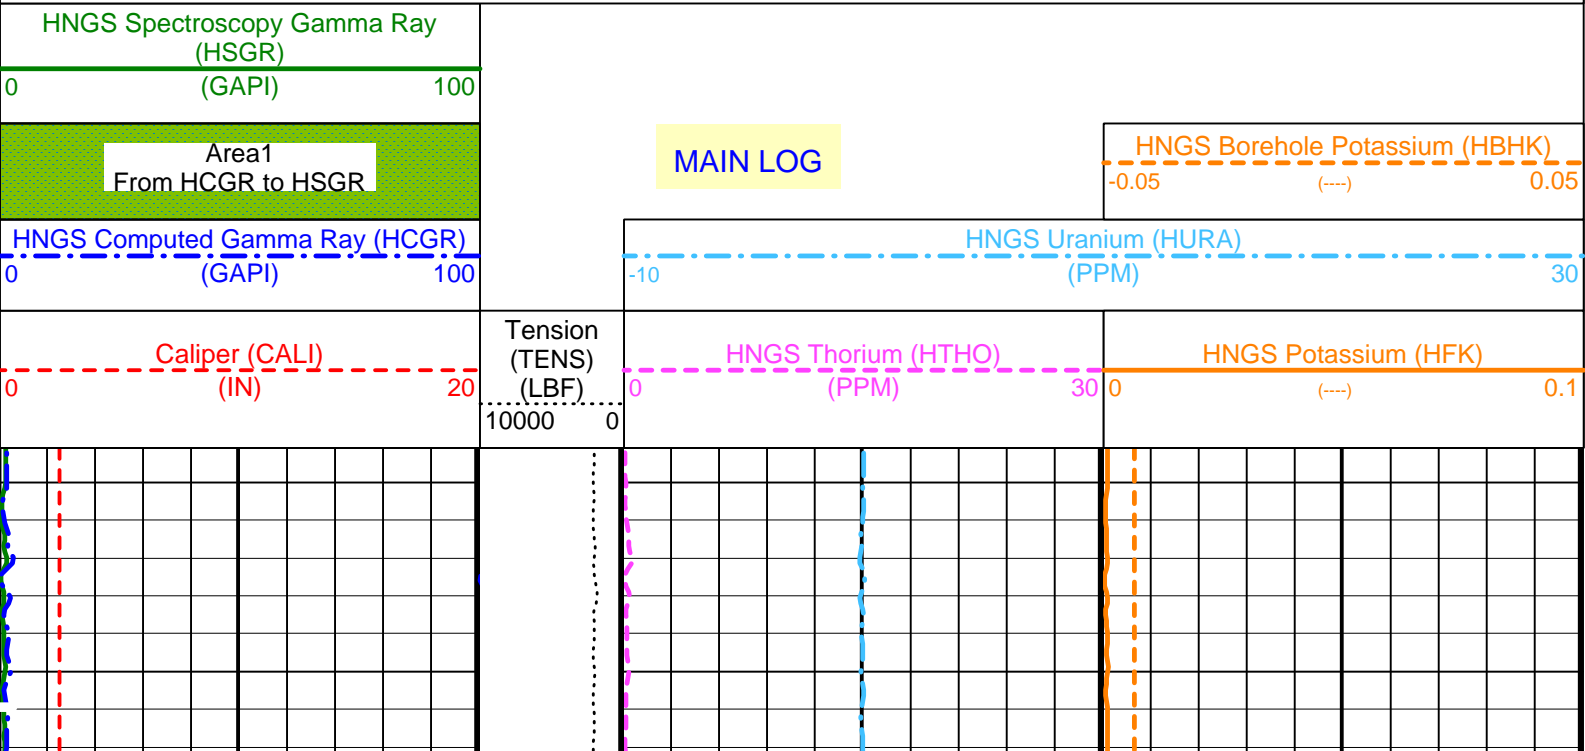

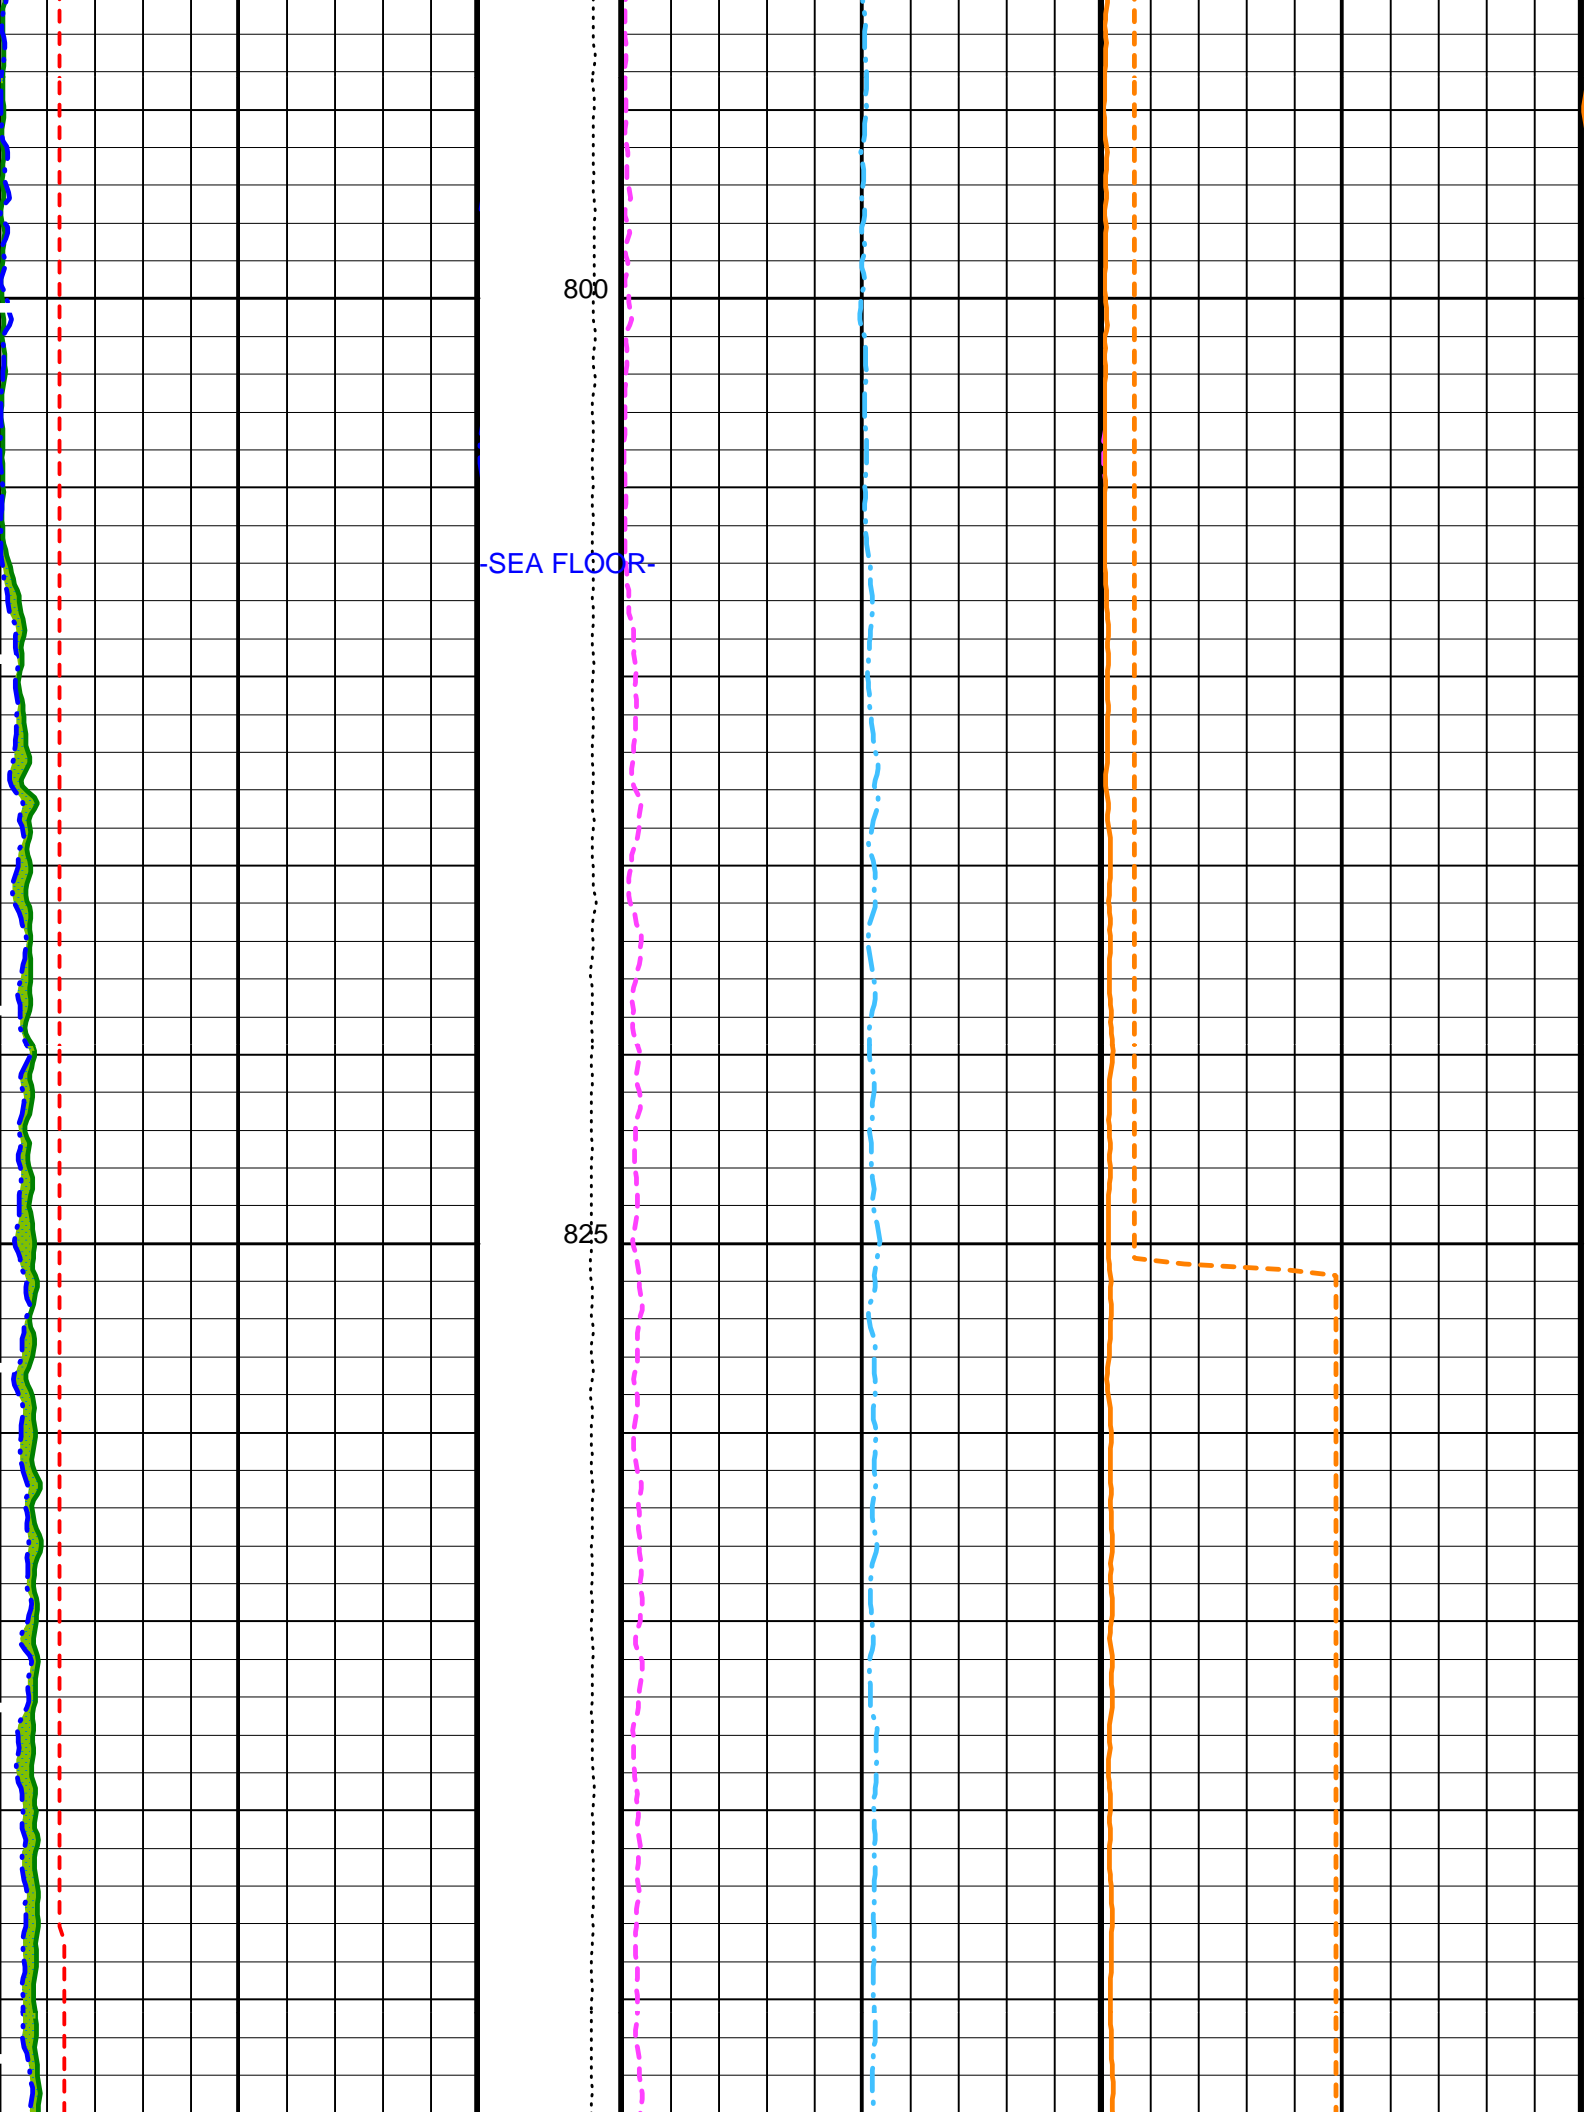

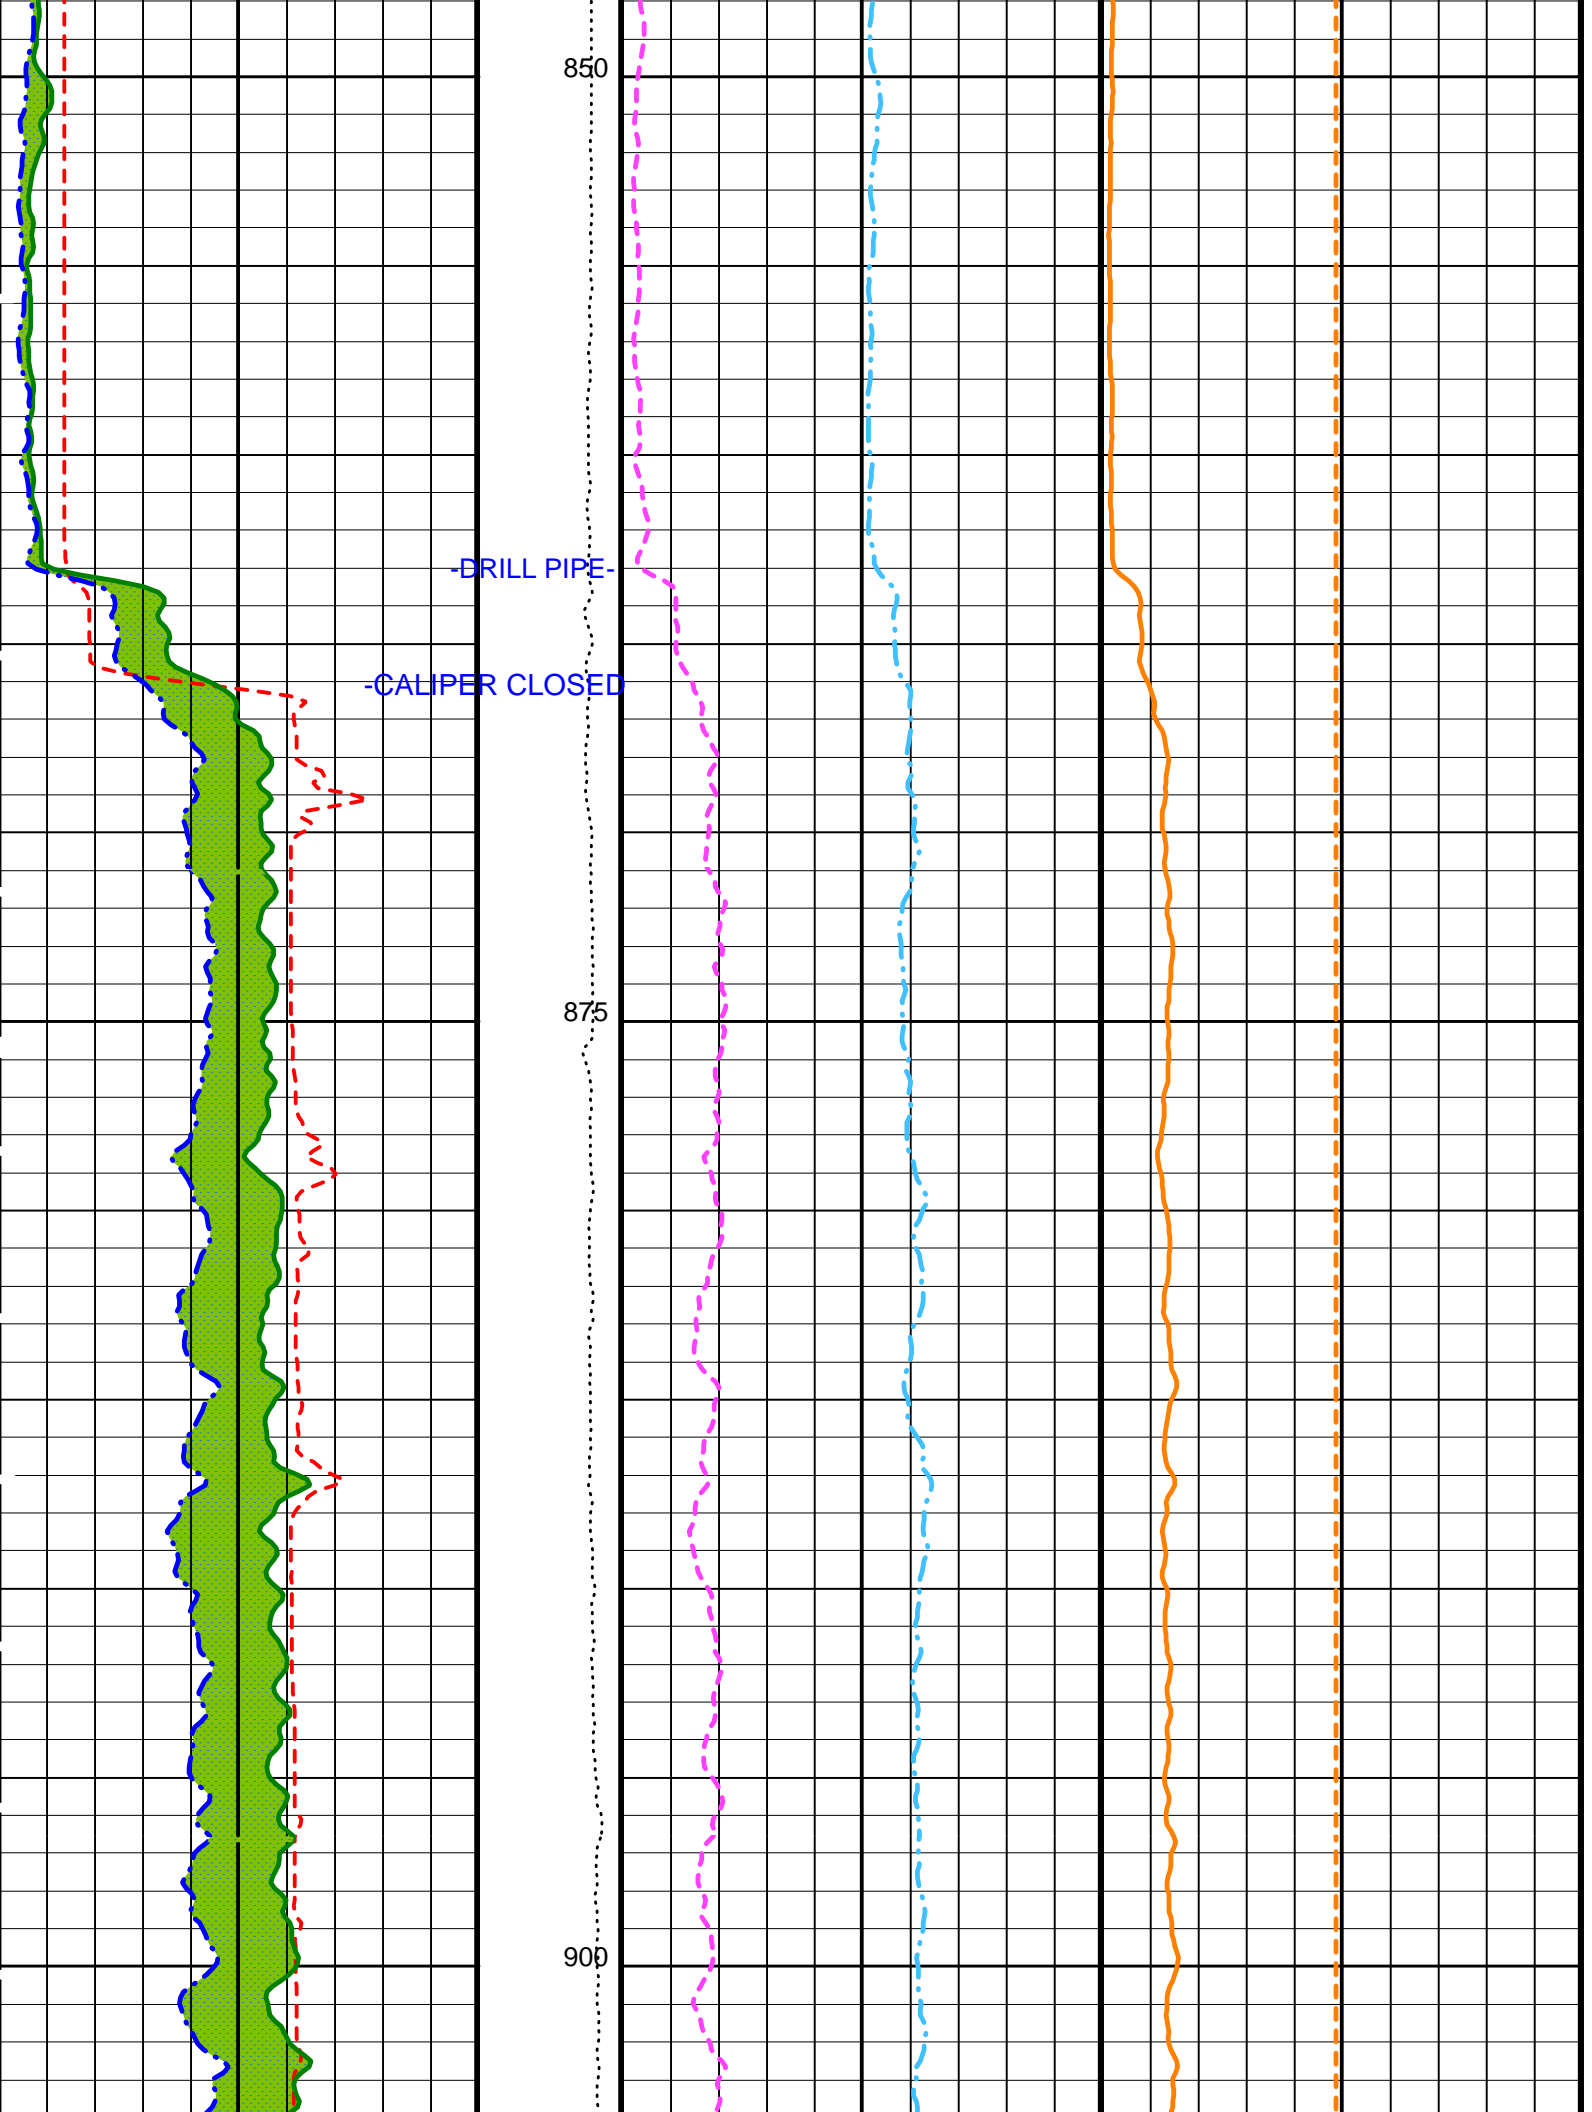

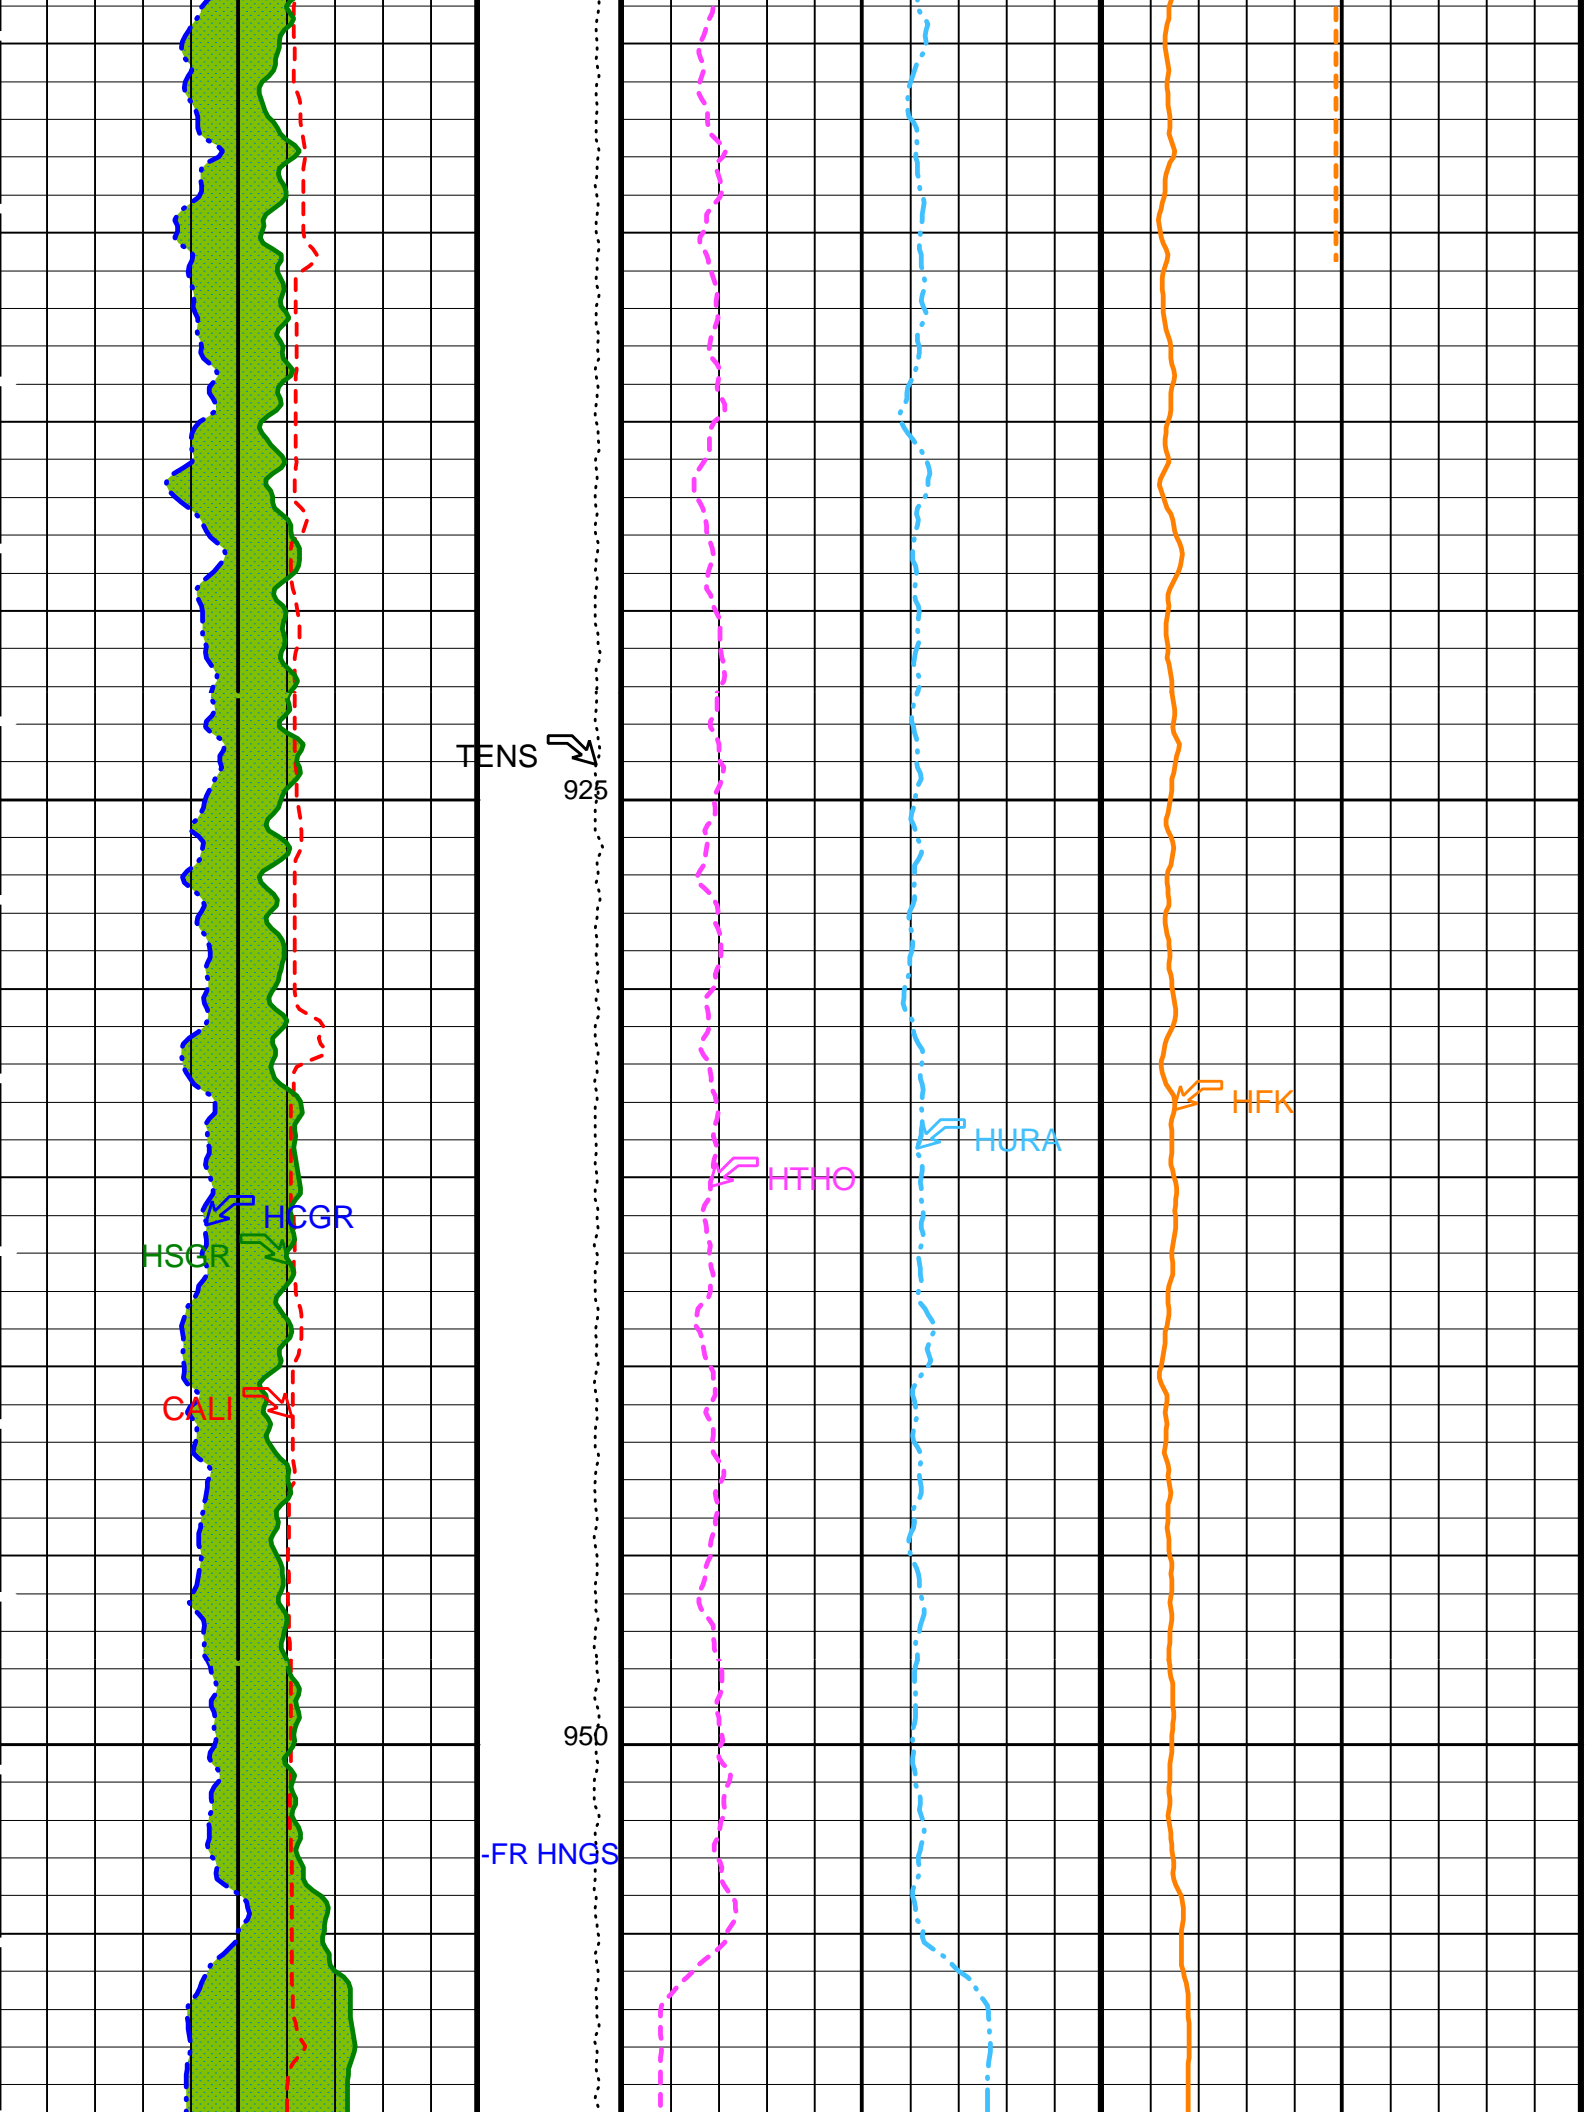

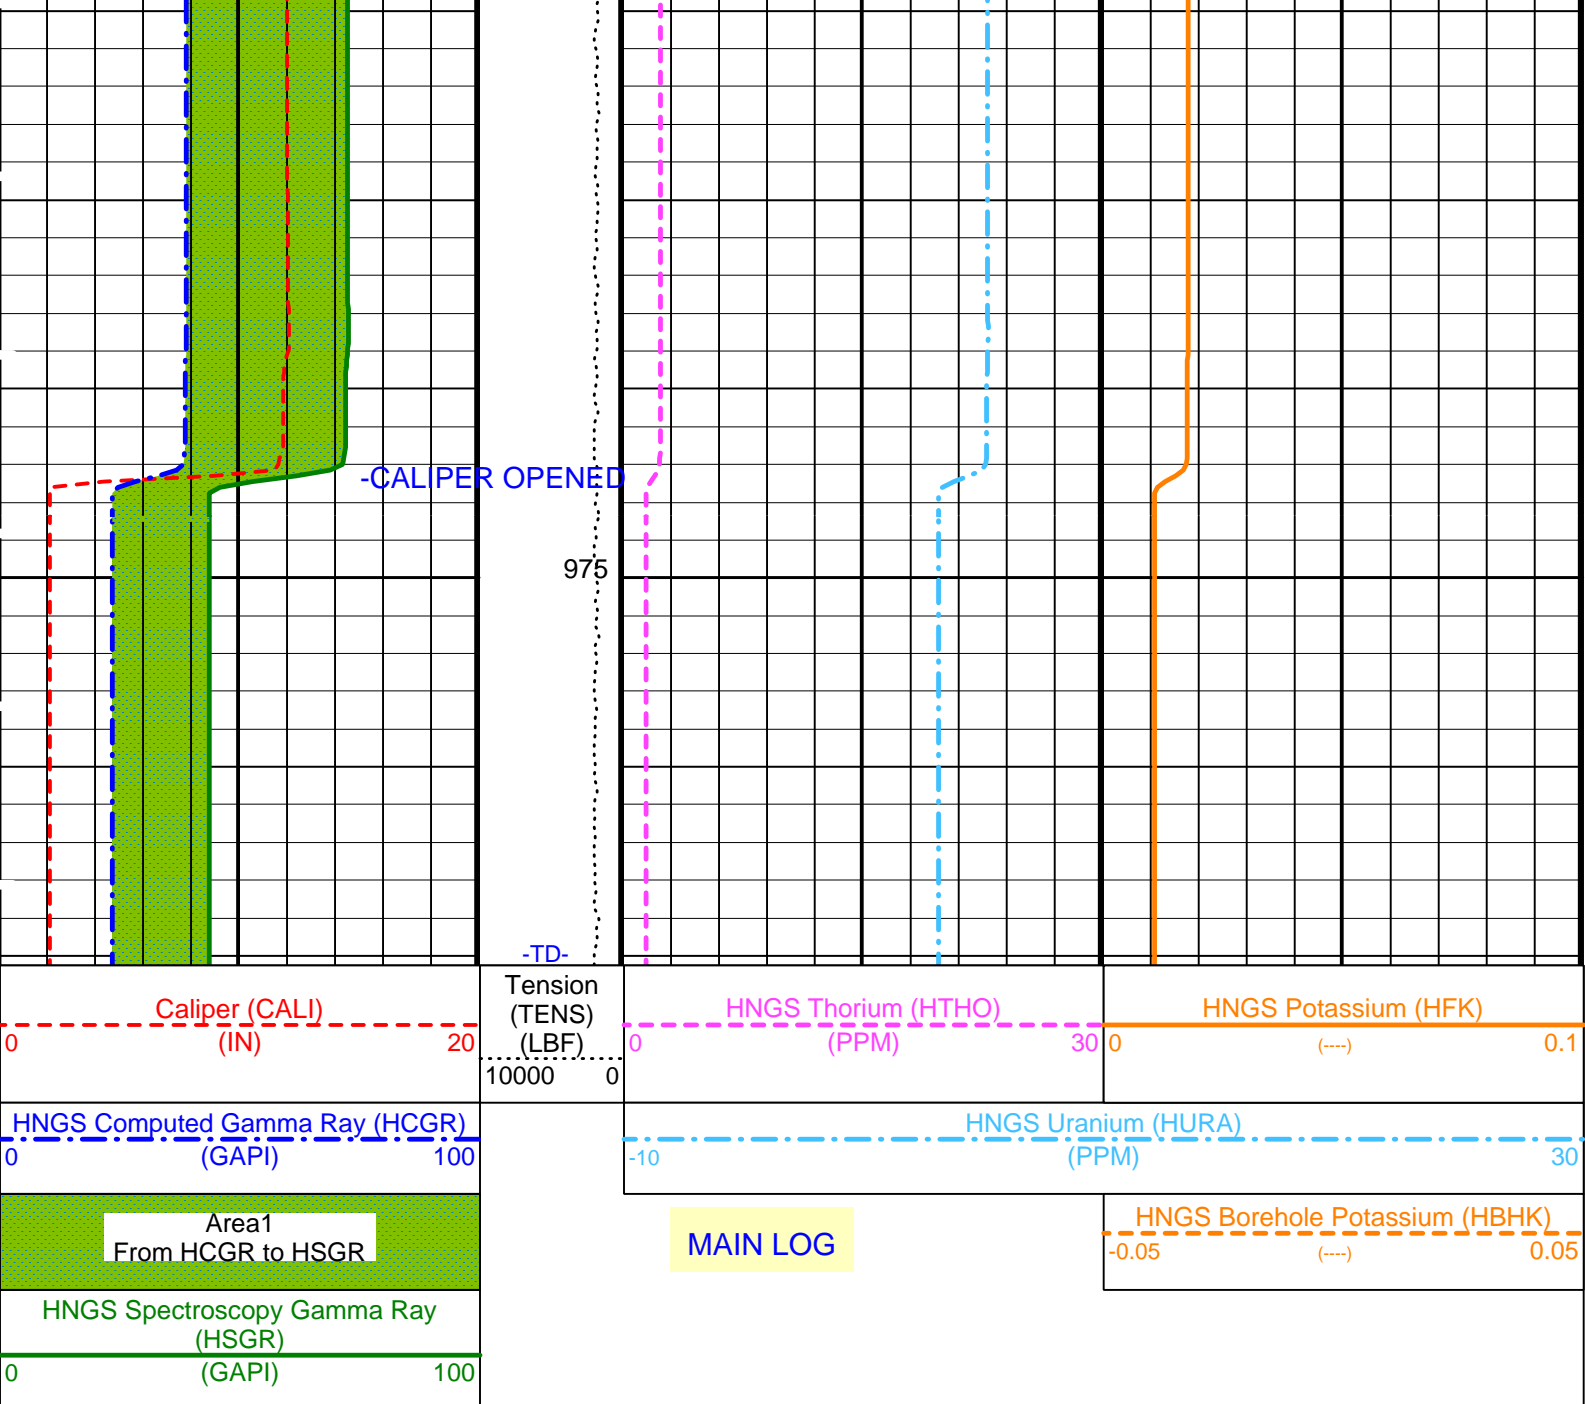

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value
	DIT-E: Dual Induction - E	
BHS	Borehole Status	OPEN
GCSE	Generalized Caliper Selection	CALI
	APS-BA: Accelerator-Porosity Tool	
BHS	Borehole Status	OPEN
GCSE	Generalized Caliper Selection	CALI
	HNGS-BA: Hostile Natural Gamma Ray Sonde	
BAR1	HNGS Detector 1 Barite Constant	1
BAR2	HNGS Detector 2 Barite Constant	1
BHK	HNGS Borehole Potassium Correction Concentration	0
BHS	Borehole Status	OPEN
CSD1	Inner Casing Outer Diameter	0 IN
CSD2	Outer Casing Outer Diameter	0 IN
CSW1	Inner Casing Weight	0 LB/F
CSW2	Outer Casing Weight	0 LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE
GCSE	Generalized Caliper Selection	CALI
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW
HANK	HNGS Borehole Potassium Running Average	0.02750454

HABK	HNGS Borehole Potassium Running Average	-0.00756454	60	IN
HALF	HNGS Alpha Filter Length		NONE	
HCRB	HNGS Apply Borehole Potassium Correction		NATU	
HMWM	Mud Weighting Material		YES	
HNPE	HNGS Processing Enable		1.3	CPS
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate		1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate		YES	
SGRC	HNGS Standard Gamma-Ray Correction Flag		ECCE	
TPOS	Tool Position		0.961934	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average		0.981195	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average			
System and Miscellaneous				
BS	Bit Size		11.438	IN
DFD	Drilling Fluid Density		1.10	G/C3

Format: HNGSYields Vertical Scale: 1:200 Graphics File Created: 25-Aug-2002 21:57

OP System Version: 10C0-306 MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	25-Aug-2002 21:57
REDUCE	PI_LDL_APS_NGS_005LUP	FN:8	PRODUCER	25-Aug-2002 21:57


Output DLIS Files


DEFAULT	PI_LDL_APS_NGS_006LUP	FN:9	PRODUCER	25-Aug-2002 22:37	985.3 M	855.0 M
REDUCE	PI_LDL_APS_NGS_006LUP	FN:10	PRODUCER	25-Aug-2002 22:37	985.3 M	853.9 M


OP System Version: 10C0-306 MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

PIP SUMMARY

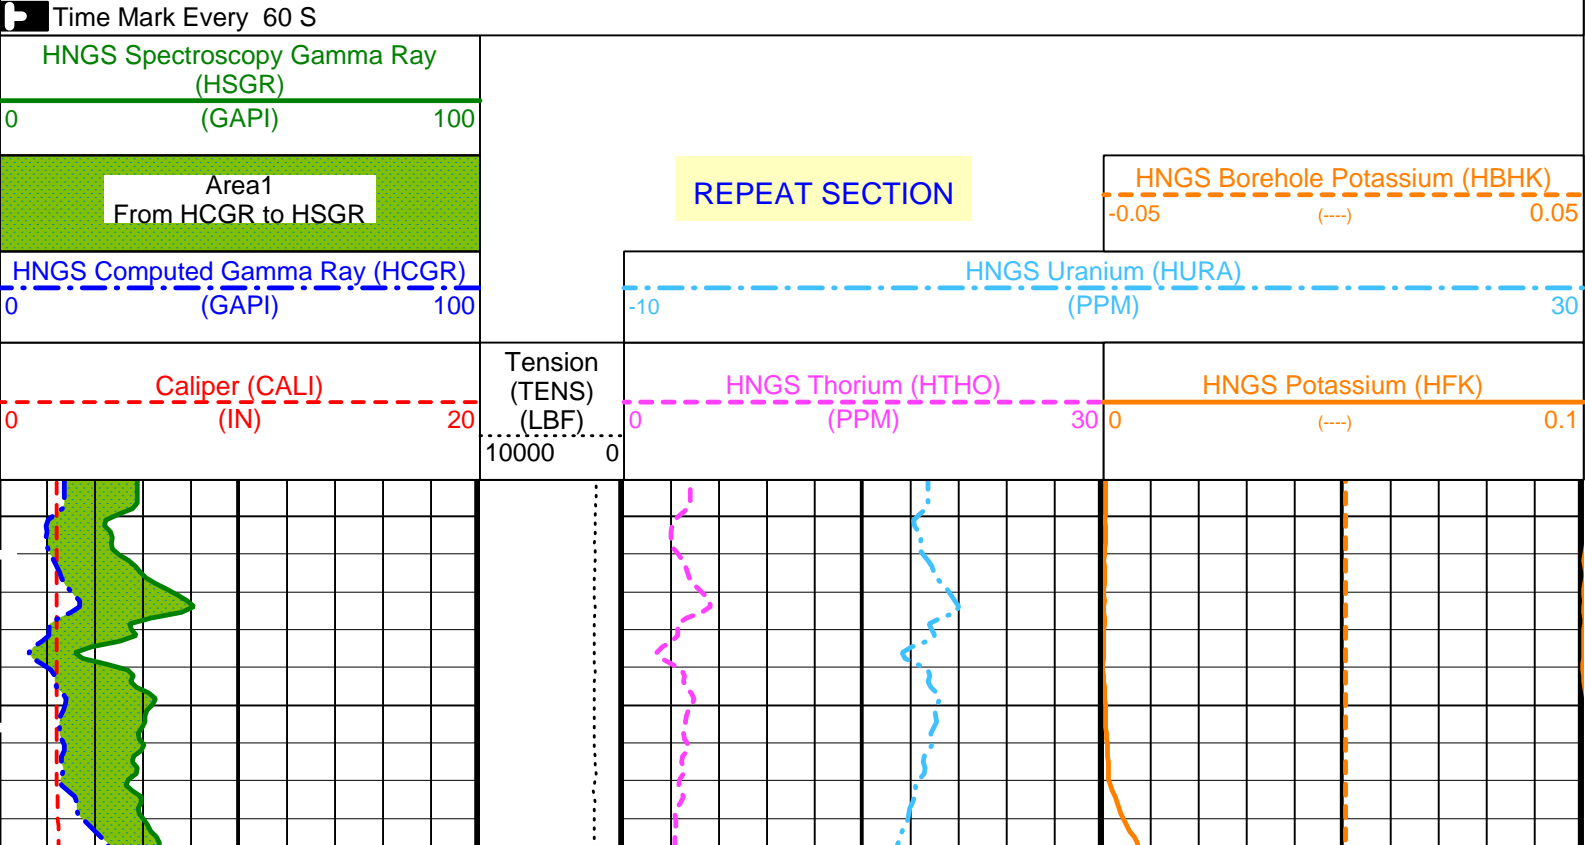


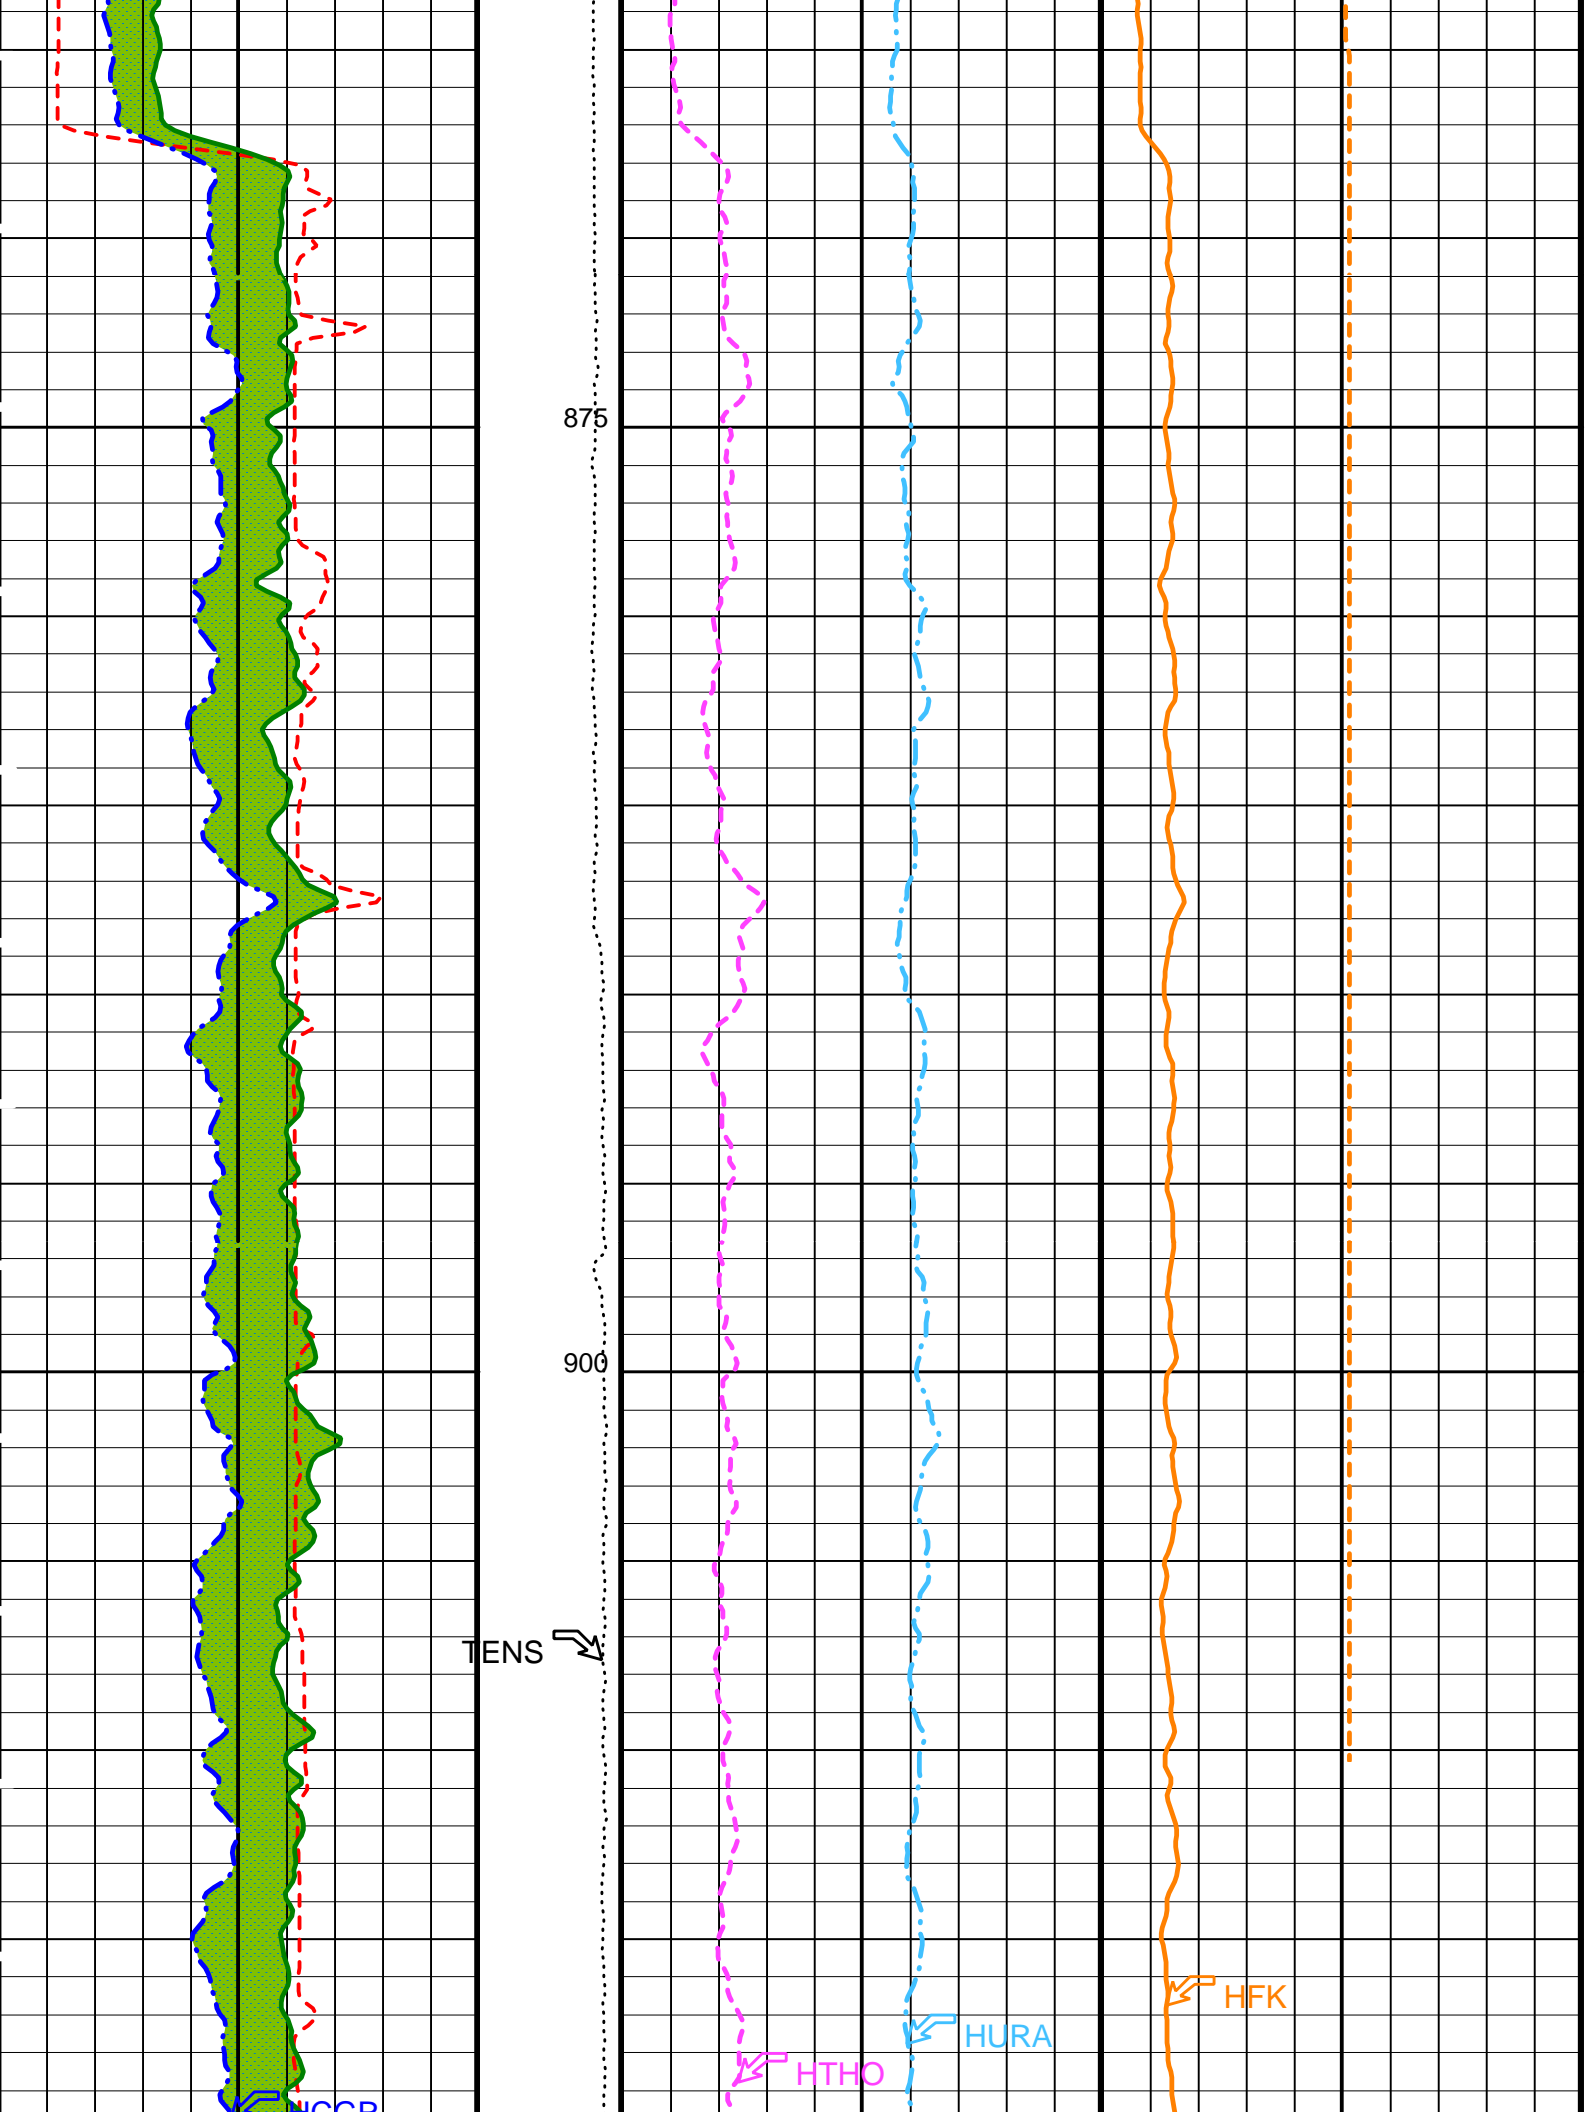


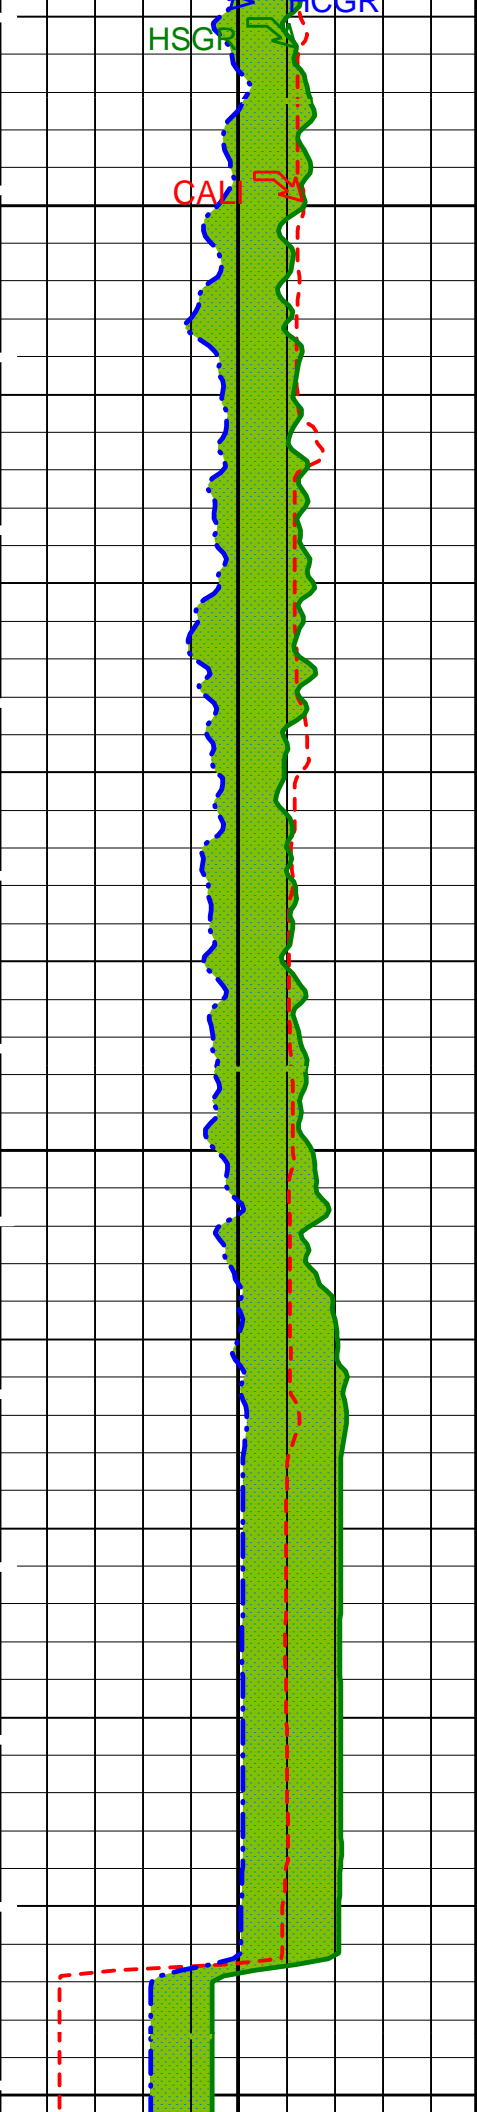

925

950

976

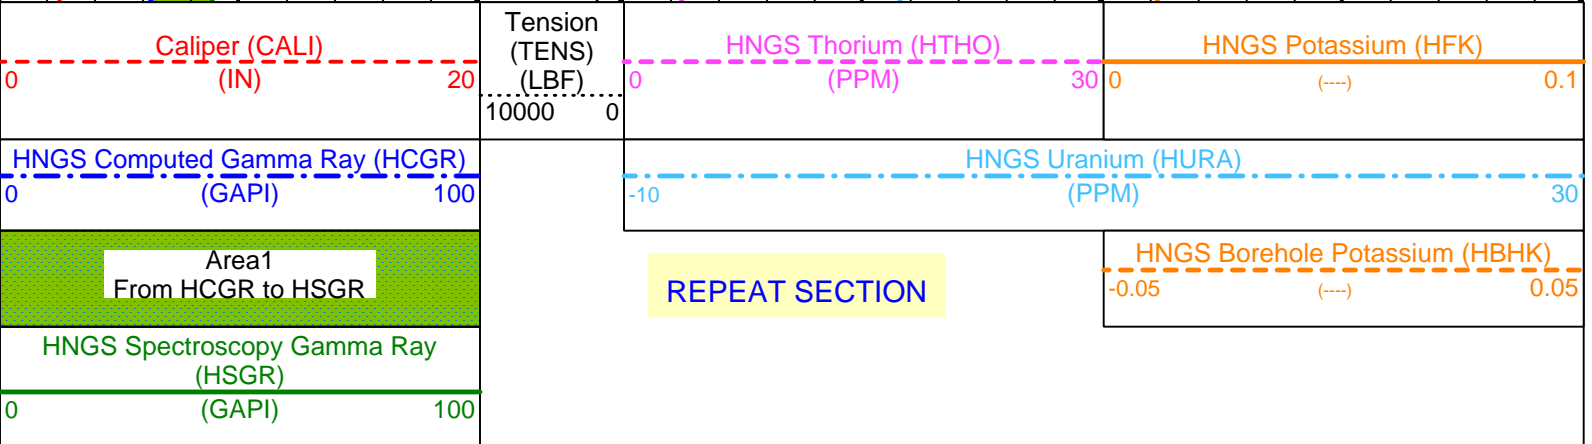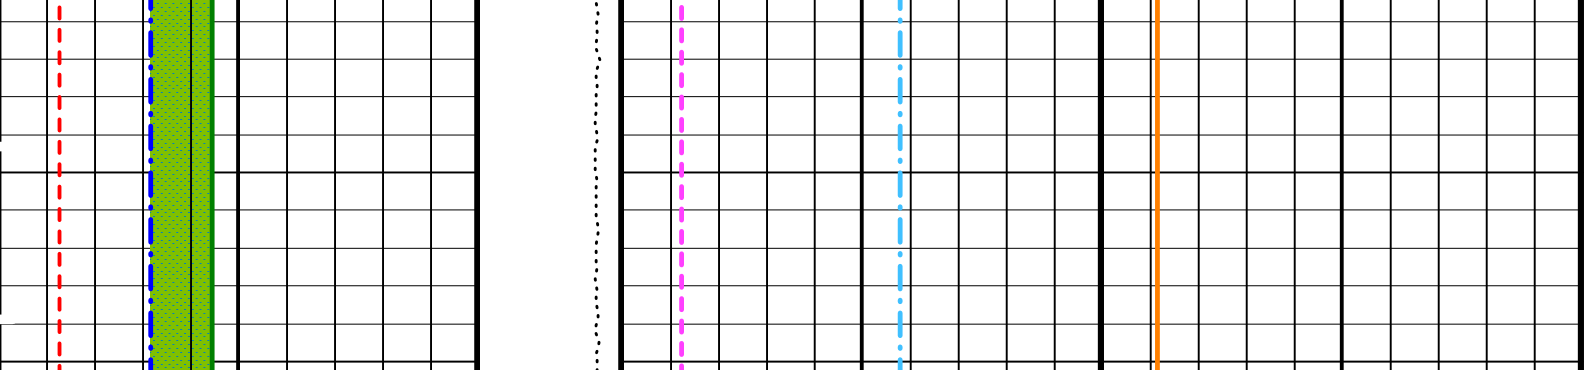

PIP SUMMARY

▶ Time Mark Every 60 S

Parameters

DLIS Name	Description	Value
DIT-E	Dual Induction - E	
BHS	Borehole Status	OPEN
GCSE	Generalized Caliper Selection	CALI
APS-BA	Accelerator-Porosity Tool	
BHS	Borehole Status	OPEN
GCSE	Generalized Caliper Selection	CALI
HNGS-BA	Hostile Natural Gamma Ray Sonde	
BAR1	HNGS Detector 1 Barite Constant	1
BAR2	HNGS Detector 2 Barite Constant	1
BHK	HNGS Borehole Potassium Correction Concentration	0
BHS	Borehole Status	OPEN
CSD1	Inner Casing Outer Diameter	0 IN
CSD2	Outer Casing Outer Diameter	0 IN
CSW1	Inner Casing Weight	0 LB/F
CSW2	Outer Casing Weight	0 LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE
GCSE	Generalized Caliper Selection	CALI
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW
HABK	HNGS Borehole Potassium Running Average	-0.0157628
HALF	HNGS Alpha Filter Length	60 IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE
HMWM	Mud Weighting Material	NATU
HNPE	HNGS Processing Enable	YES
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3 CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3 CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES
TPOS	Tool Position	ECCE
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.952792
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.948833
System and Miscellaneous		
BS	Bit Size	11.438 IN
DFD	Drilling Fluid Density	1.10 G/C3

Format: HNGSYields Vertical Scale: 1:200 Graphics File Created: 25-Aug-2002 22:37

OP System Version: 10C0-306
MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_006LUP	FN:9	PRODUCER	25-Aug-2002 22:37
REDUCE	PI_LDL_APS_NGS_006LUP	FN:10	PRODUCER	25-Aug-2002 22:37

Calibration and Check Summary

Measurement	Nominal	Master	Before	After	Change	Limit	Units
Hostile Environment Litho Density - A Wellsite Calibration - Background Measurement							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 20-Aug-2002 23:11							
LSW1 Background	100.0	88.67	86.74	87.05	0.3165	0.03000	CPS
LSW2 Background	105.0	93.18	91.70	90.17	-1.532	0.03000	CPS
LSW3 Background	210.0	177.4	176.2	173.3	-2.852	0.03000	CPS
LSW4 Background	290.0	236.8	236.6	234.2	-2.350	0.03000	CPS
LSW5 Background	610.0	518.0	517.3	517.7	0.3206	0.03000	CPS
SSW1 Background	100.0	83.02	84.95	84.57	-0.3811	0.03000	CPS
SSW2 Background	200.0	165.1	166.3	164.5	-1.828	0.03000	CPS
SSW3 Background	530.0	440.7	439.6	438.4	-1.202	0.03000	CPS
SSW4 Background	280.0	232.4	232.4	229.2	-3.199	0.03000	CPS
SSW5 Background	205.0	174.0	173.3	171.9	-1.433	0.03000	CPS
Hostile Environment Litho Density - A Wellsite Calibration - Tool Quality Control Information High Voltage							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 20-Aug-2002 23:11							
LS Bkg. High Voltage	1133	1133	1130	1130	0.5503	N/A	V
SS Bkg. High Voltage	1177	1177	1171	1171	-0.2373	N/A	V
Hostile Environment Litho Density - A Wellsite Calibration - Detectors Resolution From BKG Measurements							
Master: 12-Jun-2002 0:31 Before: 24-Jul-2002 17:39 After: 20-Aug-2002 23:11							
LS Background Resolution	1.000	1.032	1.032	1.031	-0.001574	N/A	
SS Background Resolution	1.000	0.9430	0.9416	0.9408	-0.0007873	N/A	
Hostile Environment Litho Density - A Wellsite Calibration - Caliper Calibration							
Before: 24-Jul-2002 17:38							
Caliper Small Ring	12.00	N/A	17.14	N/A	N/A	N/A	IN
Caliper Large Ring	15.25	N/A	21.07	N/A	N/A	N/A	IN
Accelerator-Porosity Tool Wellsite Calibration - Detector Background							
Master: 24-Jul-2002 9:08 Before: 25-Aug-2002 22:21 After: 20-Aug-2002 22:30							
Near Det Bkg Cntrate	30.00	32.30	32.55	33.34	0.7865	N/A	CPS
Far Det Bkg Cntrate	30.00	33.62	35.15	34.76	-0.3876	N/A	CPS
Array-1 Det Bkg Cntrate	30.00	28.88	28.78	29.28	0.5036	N/A	CPS
Array-2 Det Bkg Cntrate	30.00	29.64	29.62	30.01	0.3904	N/A	CPS
Array Therm Det Bkg Cntrate	30.00	32.75	32.75	32.59	-0.1626	N/A	CPS
Accelerator-Porosity Tool Wellsite Calibration - Calibration Ratios							
Master: 24-Jul-2002 9:08							
Near/Far Calibration Ratio	0.9250	0.9076	N/A	N/A	N/A	N/A	
Near/Array Calibration Ratio	1.030	1.066	N/A	N/A	N/A	N/A	
Near/Array Cal Ratio Up/Down	1.000	1.006	N/A	N/A	N/A	N/A	
Accelerator-Porosity Tool Wellsite Calibration - Tank Check							
Master: 24-Jul-2002 9:09							
Array-1 Standoff Porosity	11.75	11.51	N/A	N/A	N/A	N/A	PU
Array-2 Standoff Porosity	11.75	11.19	N/A	N/A	N/A	N/A	PU
Average Slowing Down Time	6.000	5.884	N/A	N/A	N/A	N/A	US
Array-1 SDT Ratio Up/Down	1.000	0.9901	N/A	N/A	N/A	N/A	
Array-2 SDT Ratio Up/Down	1.000	0.9732	N/A	N/A	N/A	N/A	
Sigma Formation	27.50	27.88	N/A	N/A	N/A	N/A	CU
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 1 Check							
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 20-Aug-2002 23:10							
Na 511 Peak Loc	40.00	40.59	40.60	40.61	0.002739	1.000	
Na 511 Peak Res	15.50	16.79	16.89	15.96	-0.9243	2.000	%
High Voltage	1150	1224	1220	1220	-0.09119	30.00	V
Na 1785 Peak Loc	142.6	145.1	146.3	145.9	-0.4483	7.000	
Na 1785 Peak Res	8.500	10.40	8.694	8.720	0.02588	2.000	%
Temperature	15.50	24.98	22.43	20.55	-1.880	N/A	DEGC
Na Count Rate	45.00	50.31	49.89	49.45	-0.4308	8.000	CPS
Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 2 Check							
Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 20-Aug-2002 23:10							
Na 511 Peak Loc	40.00	40.58	40.59	40.62	0.02345	1.000	
Na 511 Peak Res	15.50	16.72	16.53	16.77	0.2390	2.000	%

Na 511 Peak Res	15.00	18.72	18.33	18.77	0.2330	2.000	%
High Voltage	1150	1253	1250	1247	-3.122	30.00	V
Na 1785 Peak Loc	142.6	144.7	144.3	144.8	0.5048	7.000	
Na 1785 Peak Res	8.500	9.766	9.897	9.571	-0.3262	2.000	%
Temperature	15.50	24.15	21.87	20.77	-1.099	N/A	DEGC
Na Count Rate	45.00	50.19	49.39	49.43	0.03497	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Ratio Of Detector 1 To Detector 2

Master: 13-Jul-2002 3:08 Before: 24-Jul-2002 12:59 After: 20-Aug-2002 23:10

Coincidence Count Rate Ratio	1.000	1.004	1.010	1.000	-0.009243	0.05000
------------------------------	-------	-------	-------	-------	-----------	---------

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 1 Calibration

Master: 13-Jul-2002 3:01

Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	208.9	--	--	--	--	
Th Peak Res	7.000	8.227	--	--	--	--	%
Background Count Rate	142.5	24.67	--	--	--	--	CPS
Gain Ratio	1.000	0.9793	--	--	--	--	

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 2 Calibration

Master: 13-Jul-2002 3:01

Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	208.8	--	--	--	--	
Th Peak Res	7.000	8.191	--	--	--	--	%
Background Count Rate	142.5	22.68	--	--	--	--	CPS
Gain Ratio	1.000	0.9792	--	--	--	--	

Accelerator-Porosity Tool - Detector Plateau Settings :

Near Detector Plateau Setting	1748 V
Far Detector Plateau Setting	2052 V
Array Detector Plateau Setting	1969 V

Dual Induction - E / Equipment Identification

Primary Equipment:		
Dual Induction Sonde	DIS - HB	442
Dual Induction Cartridge	DIC - EB	438
Auxiliary Equipment:		
Mass Isolated Housing	MIH - ZA	417

Hostile Environment Litho Density - A / Equipment Identification

Primary Equipment:		
HOSTILE ENVIRONMENT LITHO DENSITY HIGH V	HLDV - A	10
HOSTILE ENVIRONMENT LITHO DENSITY CARTRI	HLDC - AA	11
Gamma Source Radioactive	GSR - Z	1846
Auxiliary Equipment:		
HOSTILE ENVIRONMENT LITHO DENSITY SONDE	HLDS - B	10
HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG	HEH - H	12
HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG	HEH - G	11
HOSTILE ENVIRONMENT LITHO DENSITY PAD	HLDP - B	10

Nuclear Porosity Lithology Cartridge - B / Equipment Identification

Primary Equipment:		
NPLC Cartridge	NPLC - B	79
Auxiliary Equipment:		
NPLC Housing	NPH - B	82

Accelerator-Porosity Tool / Equipment Identification

Primary Equipment:		
Accelerator-Porosity Sonde	APS - BA	22
Auxiliary Equipment:		
APSHousing	APHS - BA	22

Auxiliary Equipment:

Accelerator-Porosity Housing	APH - AC	22
APS Calibration Water Tank	SFT - 178	4722
APS Aluminium Calibrator Sleeve	SFT - 281	24

Hostile Natural Gamma Ray Sonde / Equipment Identification

Primary Equipment:

HNGS Sonde	HNGS - BA	77
------------	-----------	----

Auxiliary Equipment:

HNGS Sonde Housing	HNSH - BA	79
Gamma Source Radioactive	GSR - U	135

Hostile Natural Gamma Ray Sonde Wellsite Calibration




Detector 1 Check






Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.59	Master		16.79	Master		1224
Before		40.60	Before		16.89	Before		1220
After		40.61	After		15.96	After		1220
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		145.1	Master		10.40	Master		24.98
Before		146.3	Before		8.694	Before		22.43
After		145.9	After		8.720	After		20.55
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		50.31						
Before		49.89						
After		49.45						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 13-Jul-2002 3:08			Before: 24-Jul-2002 12:59			After: 20-Aug-2002 23:10		






Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 2 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.58	Master		16.72	Master		1253
Before		40.59	Before		16.53	Before		1250
After		40.62	After		16.77	After		1247
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		144.7	Master		9.766	Master		24.15
Before		144.3	Before		9.897	Before		21.87
After		144.8	After		9.571	After		20.77
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		50.19						
Before		49.39						
After		49.43						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 13-Jul-2002 3:08			Before: 24-Jul-2002 12:59			After: 20-Aug-2002 23:10		

Hostile Natural Gamma Ray Sonde Wellsite Calibration		
Ratio Of Detector 1 To Detector 2		
Phase	Coincidence Count Rate Ratio	Value
Master		1.004
Before		1.010
After		1.000
0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)		
Master: 13-Jul-2002 3:08		
Before: 24-Jul-2002 12:59		
After: 20-Aug-2002 23:10		

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 1 Calibration								
Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value
Master		41.00	Master		208.9	Master		8.227
38.00 (Minimum) 40.00 (Nominal) 42.00 (Maximum)			201.0 (Minimum) 209.6 (Nominal) 218.3 (Maximum)			5.000 (Minimum) 7.000 (Nominal) 9.000 (Maximum)		
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value			
Master		24.67	Master		0.9793			
20.00 (Minimum) 142.5 (Nominal) 265.0 (Maximum)			0.9400 (Minimum) 1.000 (Nominal) 1.060 (Maximum)					
Master: 13-Jul-2002 3:01								

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 2 Calibration								
Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value
Master		41.00	Master		208.8	Master		8.191
38.00 (Minimum) 40.00 (Nominal) 42.00 (Maximum)			201.0 (Minimum) 209.6 (Nominal) 218.3 (Maximum)			5.000 (Minimum) 7.000 (Nominal) 9.000 (Maximum)		
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value			
Master		22.68	Master		0.9792			
20.00 (Minimum) 142.5 (Nominal) 265.0 (Maximum)			0.9400 (Minimum) 1.000 (Nominal) 1.060 (Maximum)					
Master: 13-Jul-2002 3:01								

Company: Lamont Doherty

Schlumberger

Well: ODP Leg 204, Site 1250F

Field: Hydrate Ridge

Ocean: Pacific

State: Oregon

Natural Gamma Ray
Spectroscopy