

Company: Lamont Doherty

Well: ODP Leg 204, Site 1251H

Field: Hydrate Ridge

Ocean: Pacific State: Oregon

Phasor Induction

Natural Gamma Ray


Ocean: Pacific
 Field: Hydrate Ridge
 Location: W125* 4.4502'
 Well: ODP Leg 204, Site 1251H
 Company: Lamont Doherty

LOCATION		W125* 4.4502' N 44* 34.2109'	Elev.: K.B. 11.3 m G.L. 0 m D.F. 11 m
Permanent Datum:	MSL	Elev.: 0 m	
Log Measured From:	RKB	11.3 m above Perm. Datum	
Drilling Measured From:	RKB		
API Serial No.	Max. Hole Devi.	Longitude	Latitude

Logging Date	17-Aug-2002
Run Number	1
Depth Driller	1665 m
Schlumberger Depth	1455 m
Bottom Log Interval	1449 m
Top Log Interval	1219 m
Casing Driller Size @ Depth	0.000 in @ 1298 m
Casing Schlumberger	1298 m
Bit Size	9.875 in

Type Fluid In Hole		Septolite Salt Water Base	
Density	Viscosity	1.1 g/cm3	
Fluid Loss	PH		
Source Of Sample		Mud Pit	
RM @ Measured Temperature		0.322 ohm.m @ 27 degC	
RMF @ Measured Temperature		@ @	
RMC @ Measured Temperature		@ @	
Source RMF	RMC		
RM @ MRT	RMF @ MRT	0.407 @ 17	@ 17
Maximum Recorded Temperatures		17 degC	
Circulation Stopped	Time	17-Aug-2002	13:00
Logger On Bottom	Time	17-Aug-2002	18:36
Unit Number	Location	99	Houston-ODP
Recorded By		K. Swain	
Witnessed By		G. Guerin, S. Barr, T. Collett	

Logging Date	17-Aug-2002	Run 1	Run 2	Run
Run Number	1			
Depth Driller	1665 m			
Schlumberger Depth	1455 m			
Bottom Log Interval	1449 m			
Top Log Interval	1219 m			
Casing Driller Size @ Depth	0.000 in @ 1298 m			
Casing Schlumberger	1298 m			
Bit Size	9.875 in			
Type Fluid In Hole		Septolite Salt Water Base		
Density	Viscosity	1.1 g/cm3		
Fluid Loss	PH			
Source Of Sample		Mud Pit		
RM @ Measured Temperature		0.322 ohm.m @ 27 degC		
RMF @ Measured Temperature		@ @		
RMC @ Measured Temperature		@ @		
Source RMF	RMC			
RM @ MRT	RMF @ MRT	0.407 @ 17	@ 17	
Maximum Recorded Temperatures		17 degC		
Circulation Stopped	Time	17-Aug-2002	13:00	
Logger On Bottom	Time	17-Aug-2002	18:36	
Unit Number	Location	99	Houston-ODP	
Recorded By		K. Swain		
Witnessed By		G. Guerin, S. Barr, T. Collett		

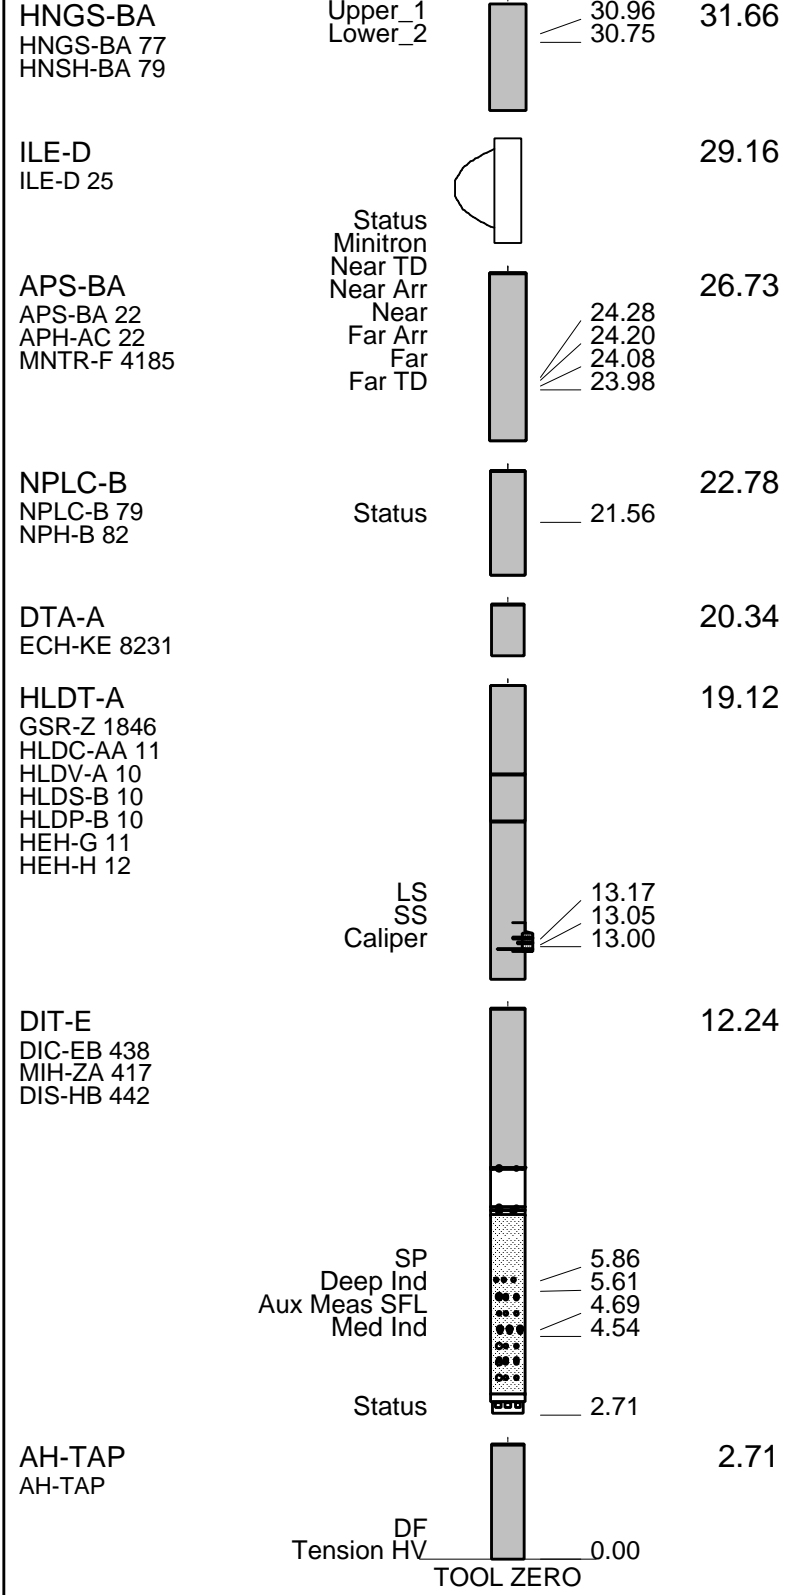

TOOL ZERO

MAXIMUM STRING DIAMETER 3.88 IN
 MEASUREMENTS RELATIVE TO TOOL ZERO
 ALL LENGTHS IN METERS

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_005LUP	FN:6	PRODUCER	17-Aug-2002 18:36	1456.2 M	1200.2 M
REDUCE	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	17-Aug-2002 18:36	1456.2 M	1198.5 M


OP System Version: 10C0-306


MCM


DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

PIP SUMMARY

Time Mark Every 60 S

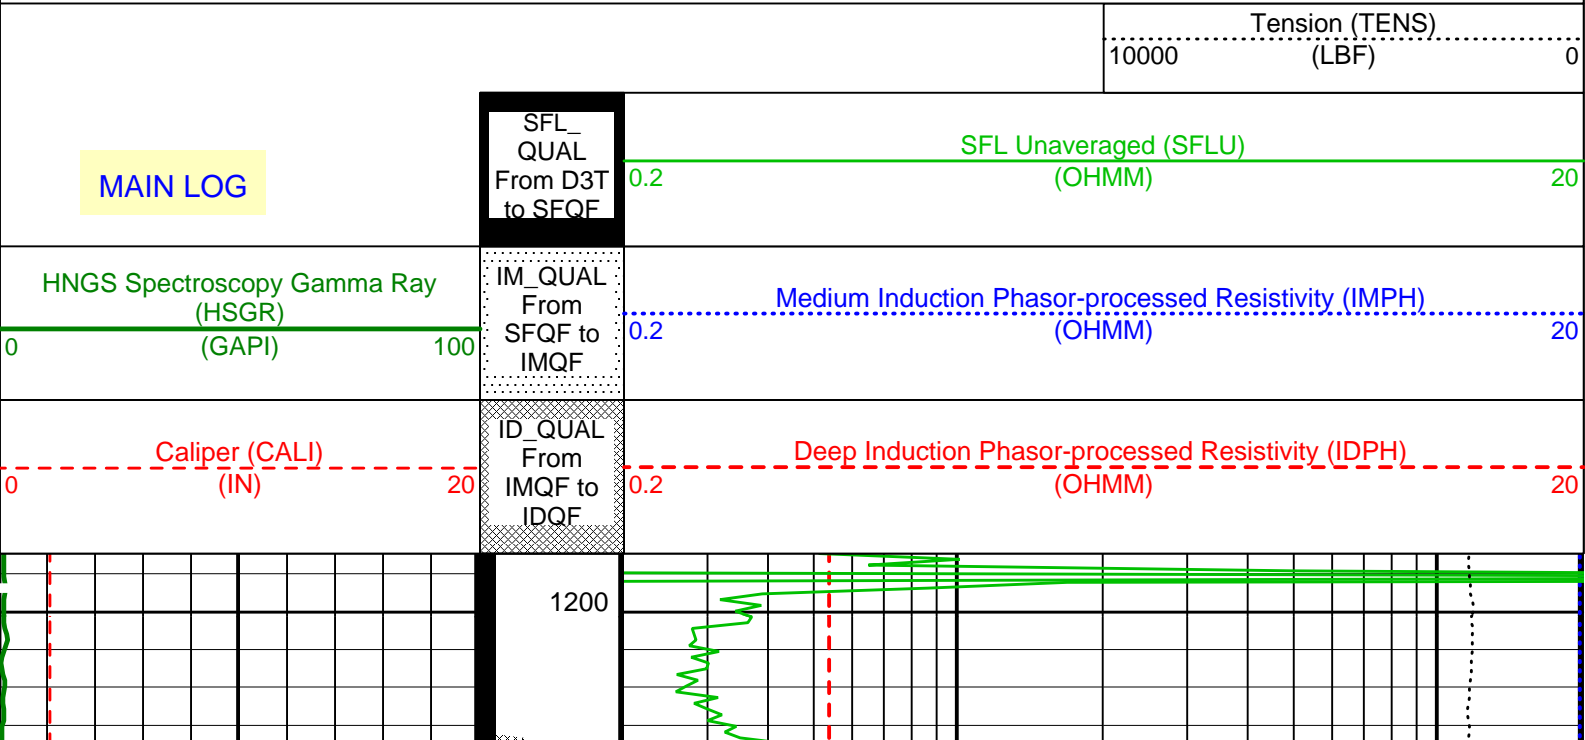

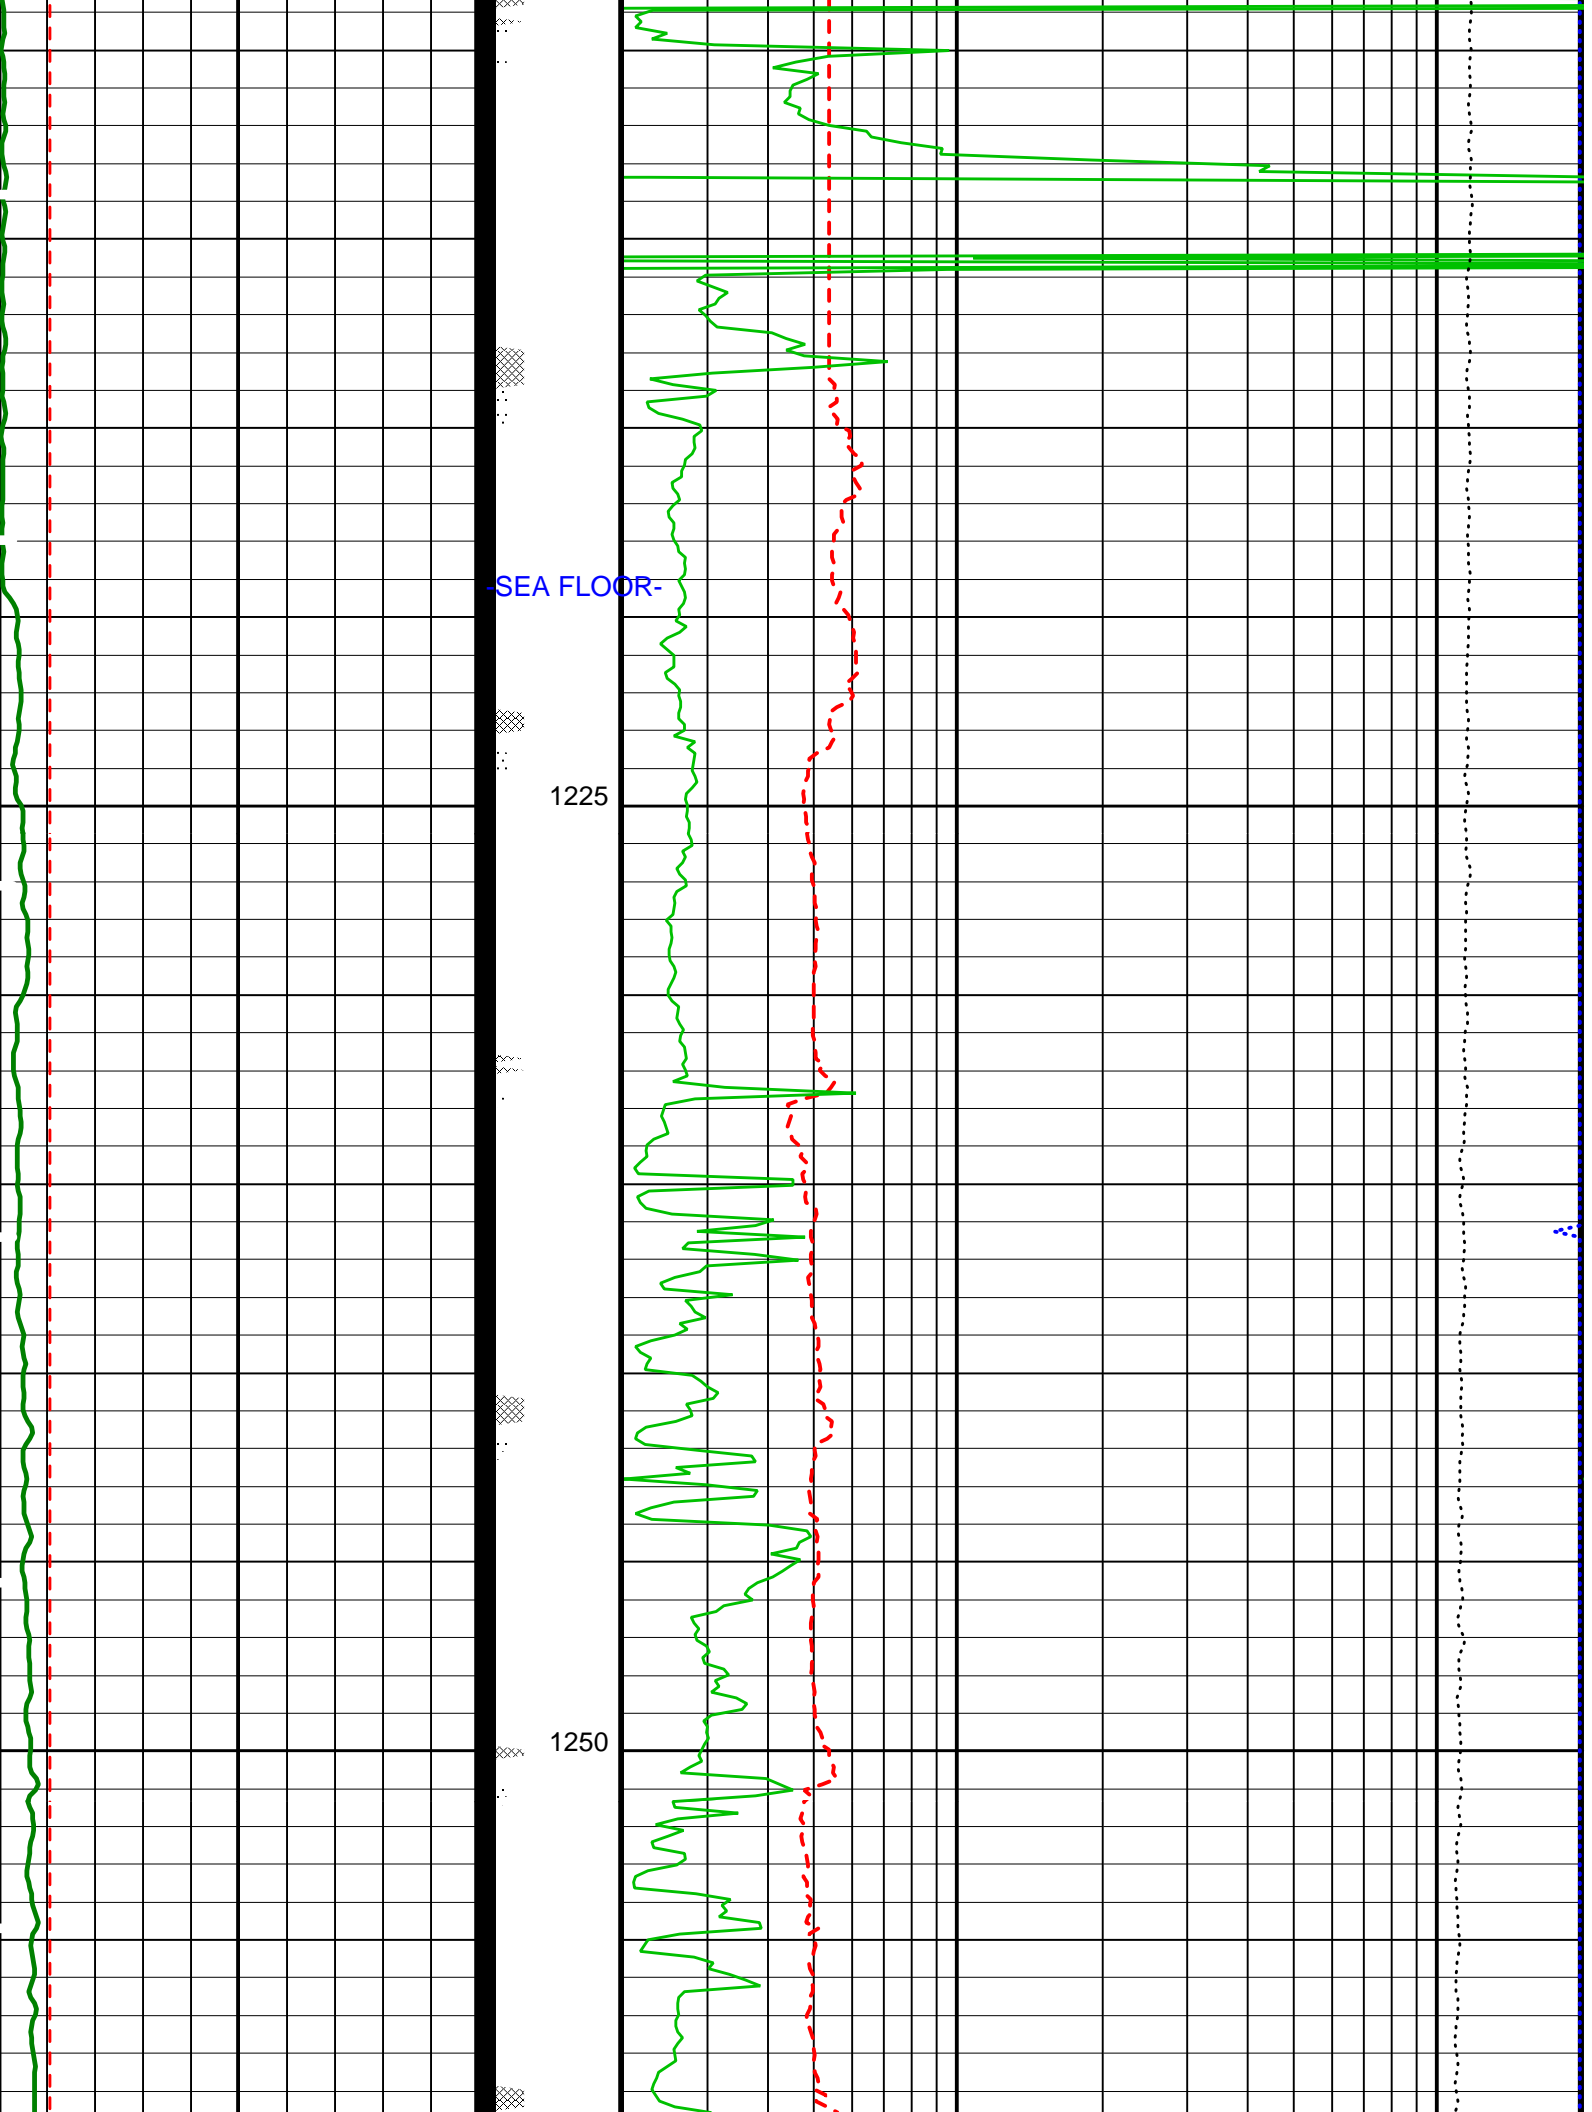

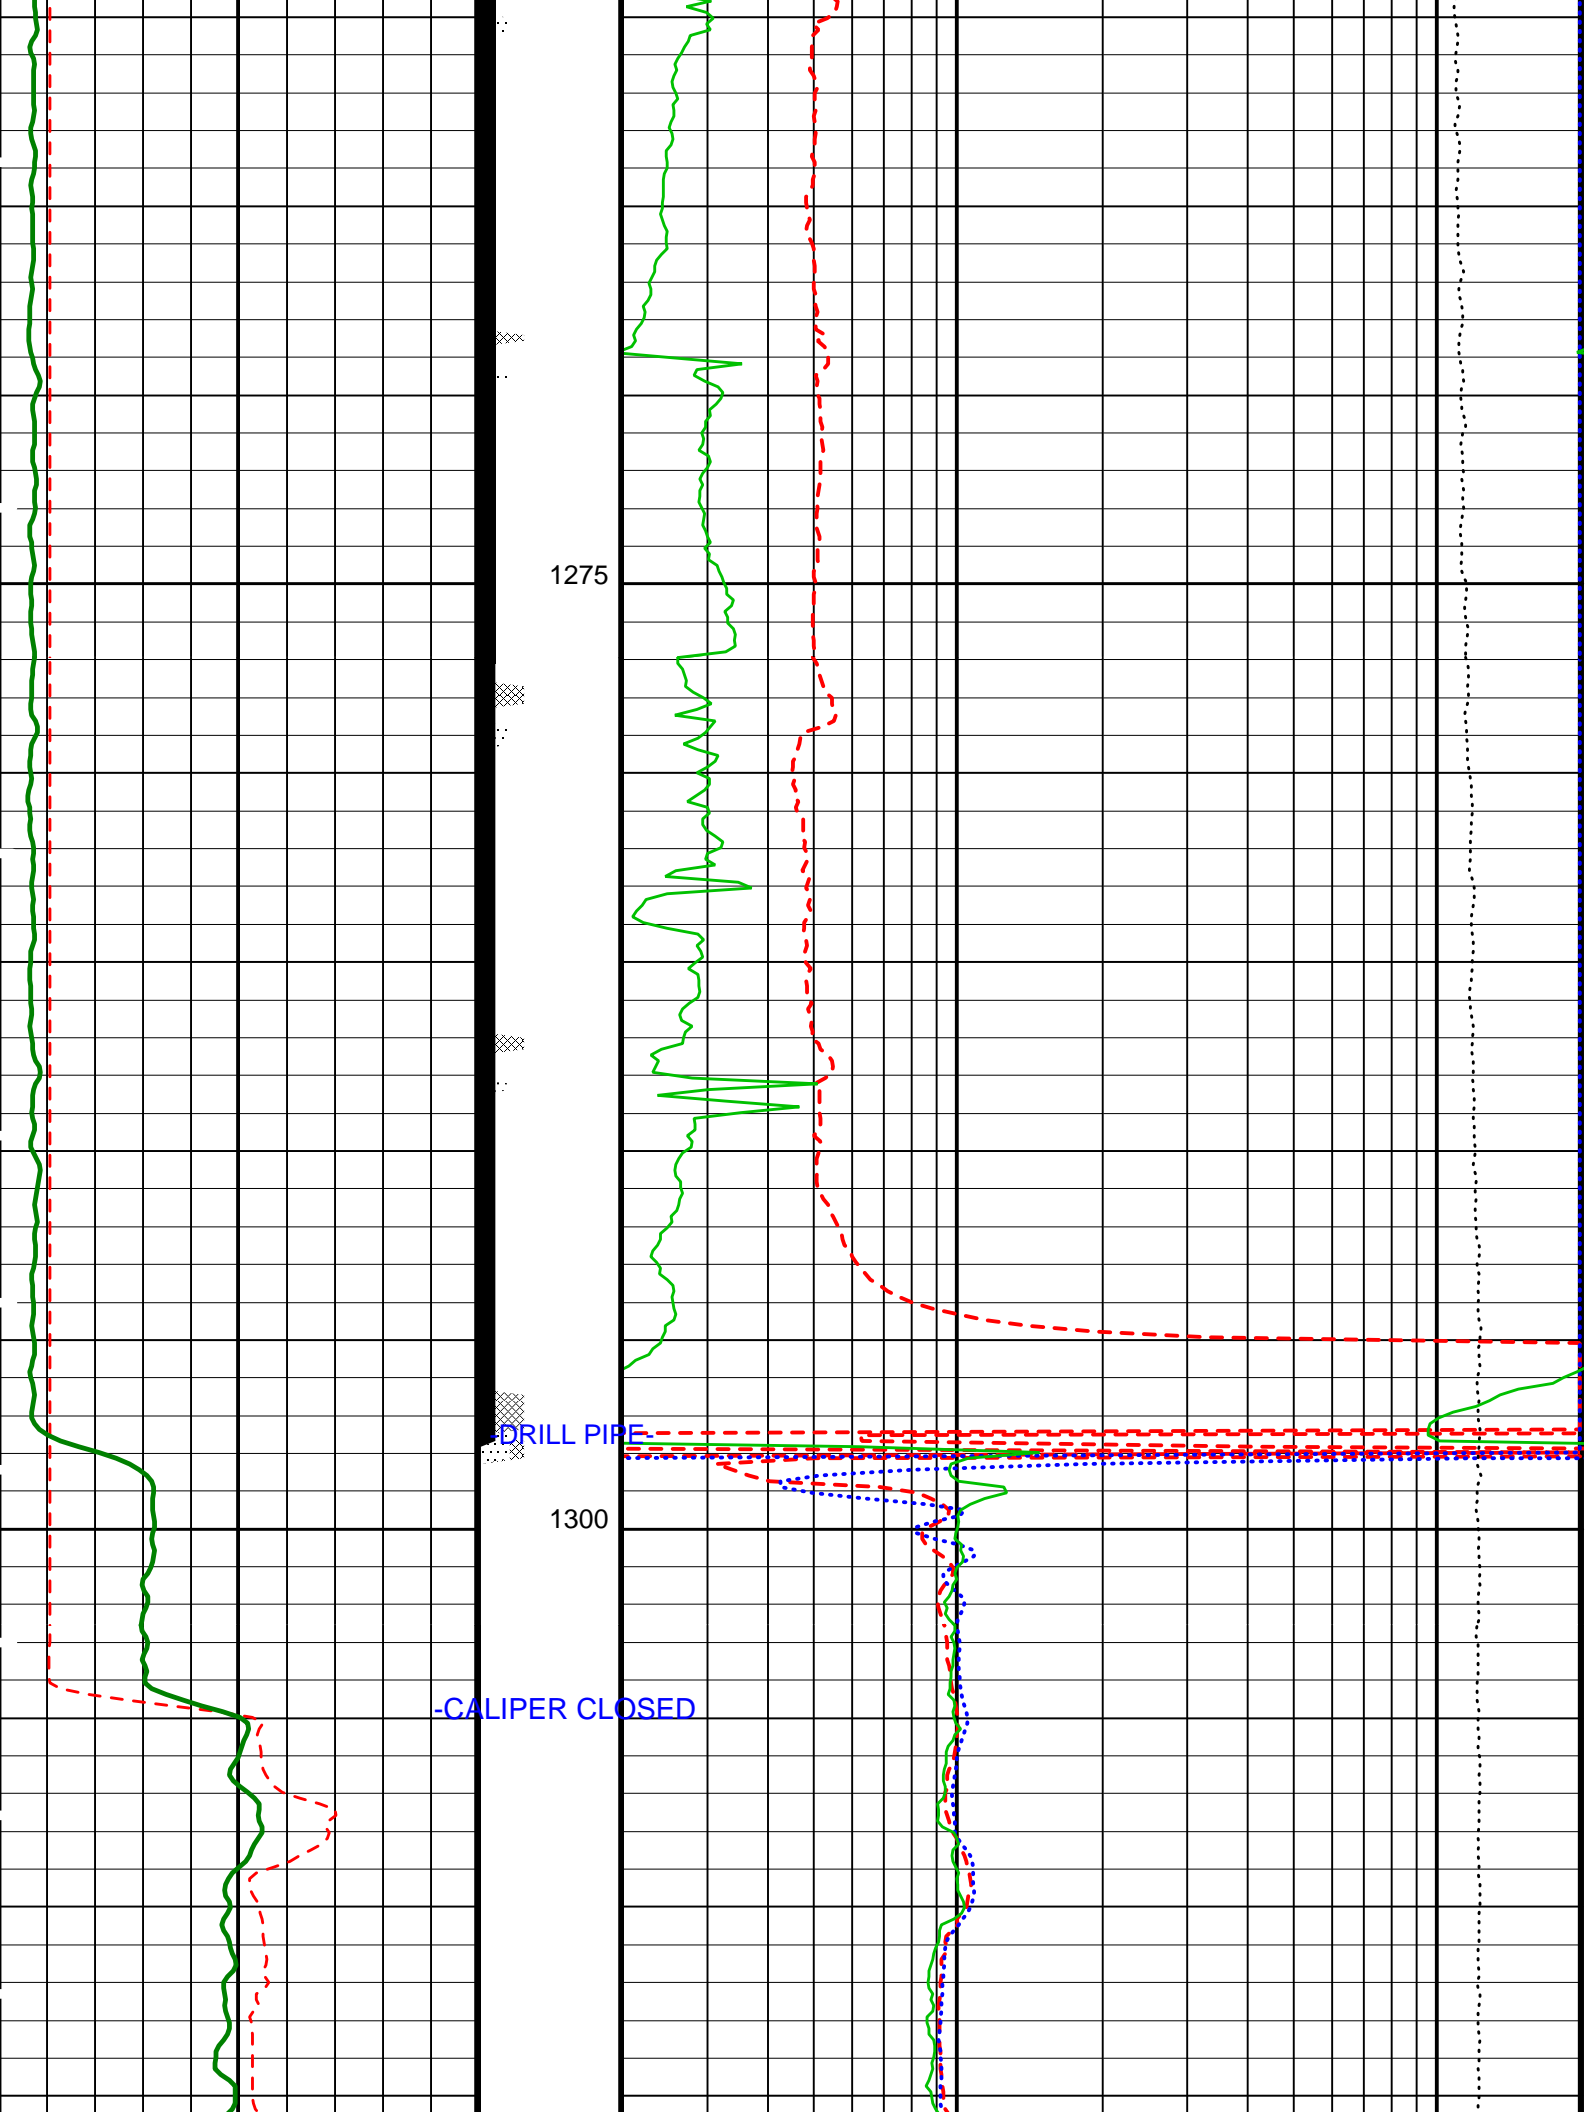


1275

1300


DRILL PIPE


-CALIPER CLOSED

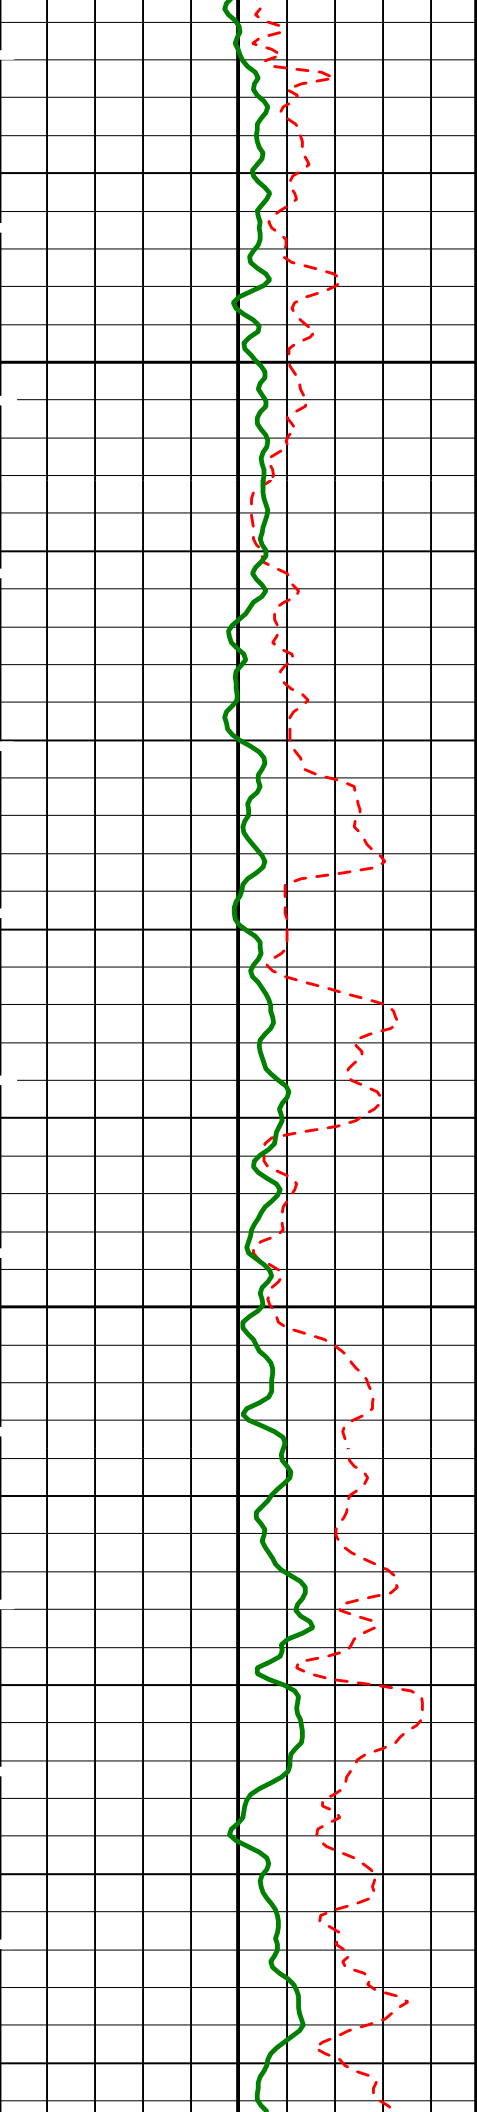

1325

1350

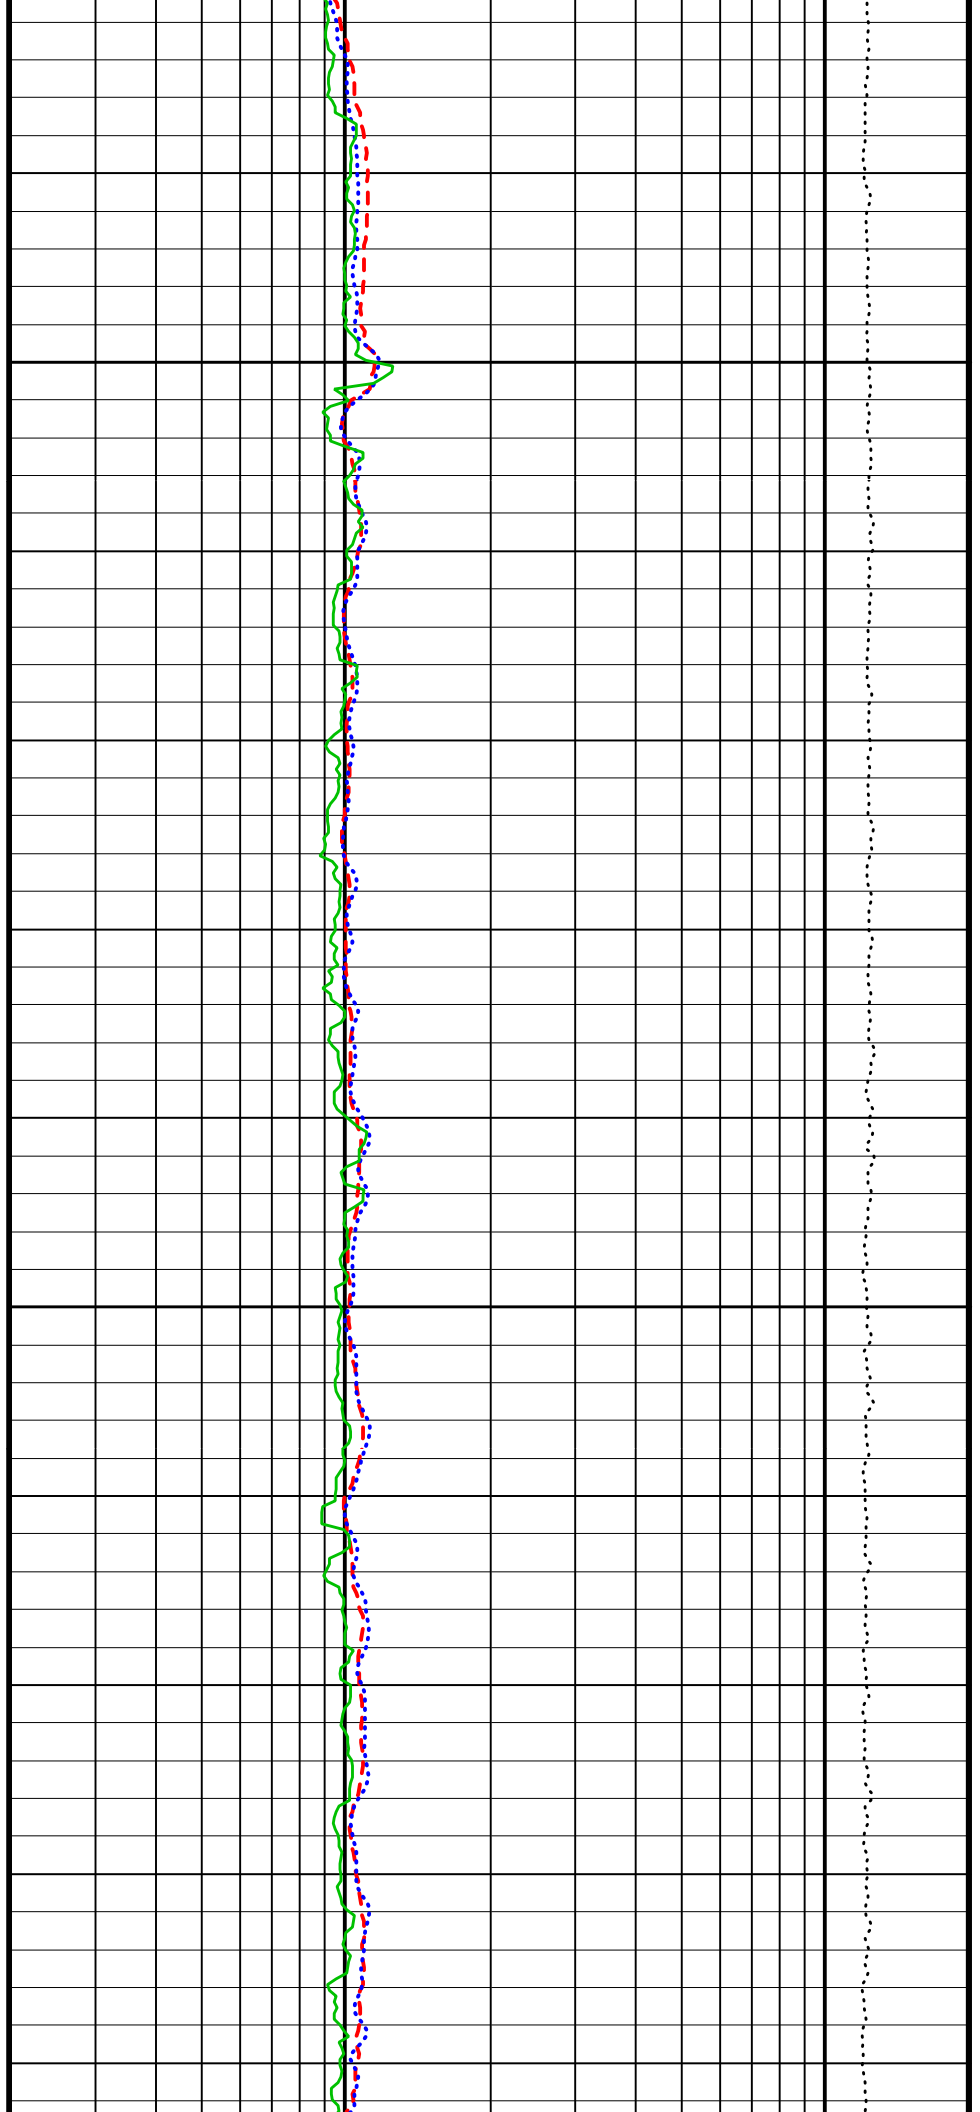

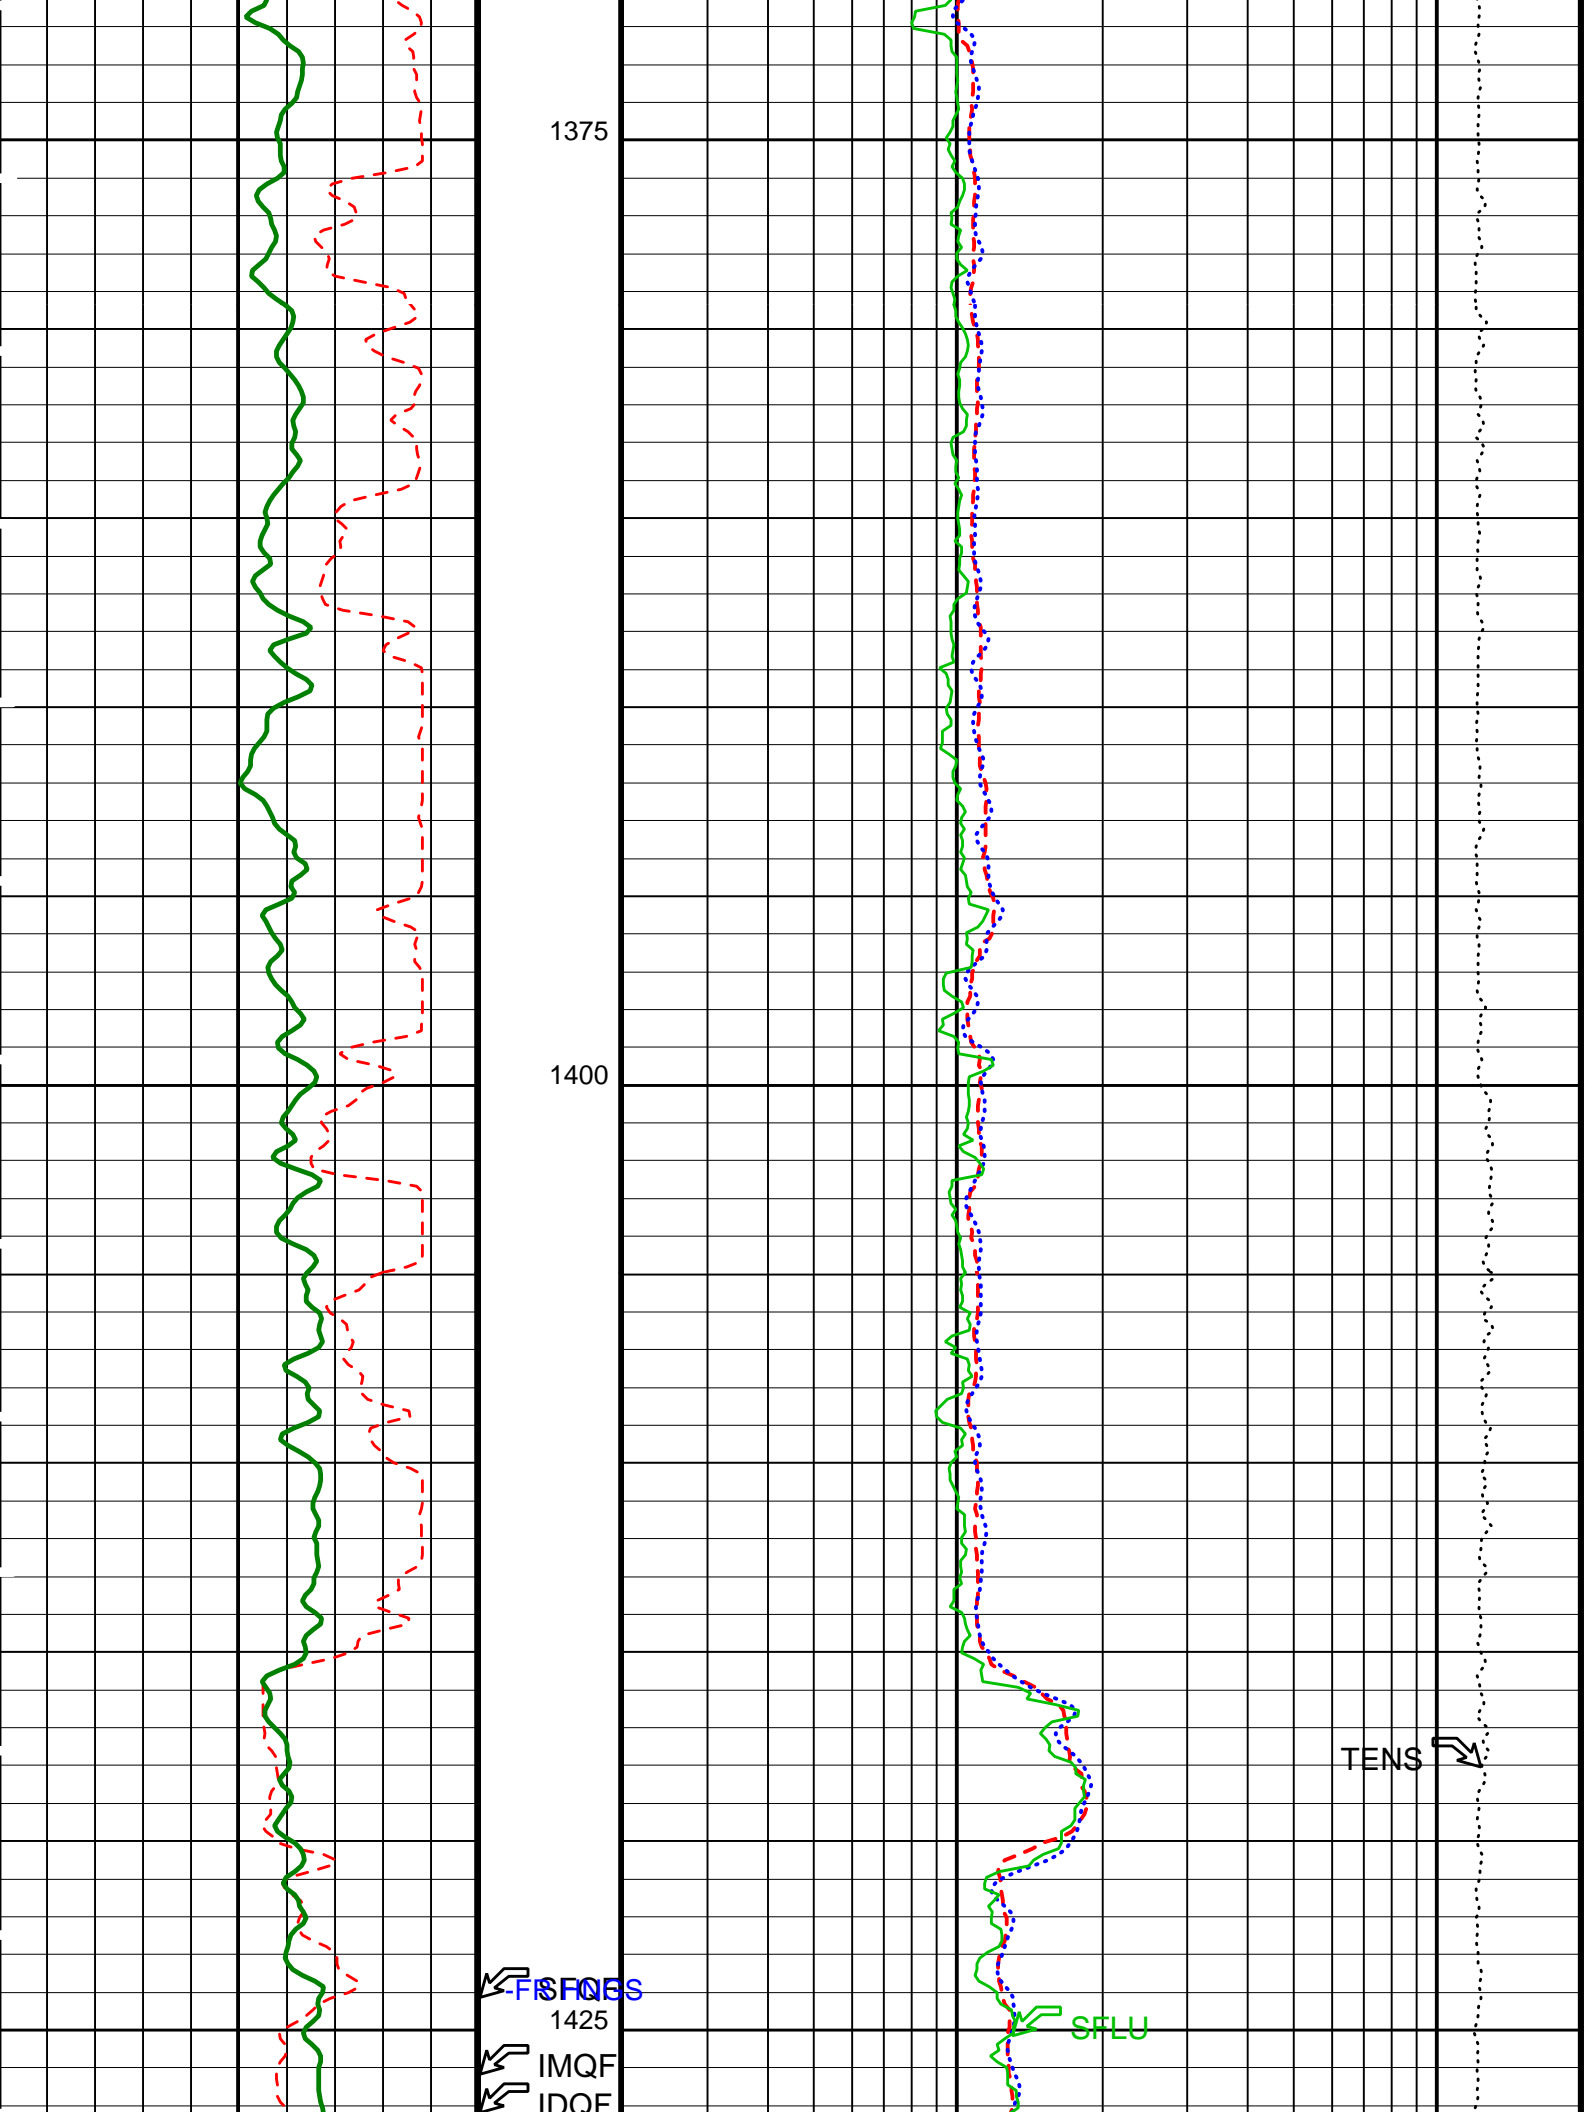

1375

1400

1425



FIS

IMQF

IDQF

SFLU

TENS

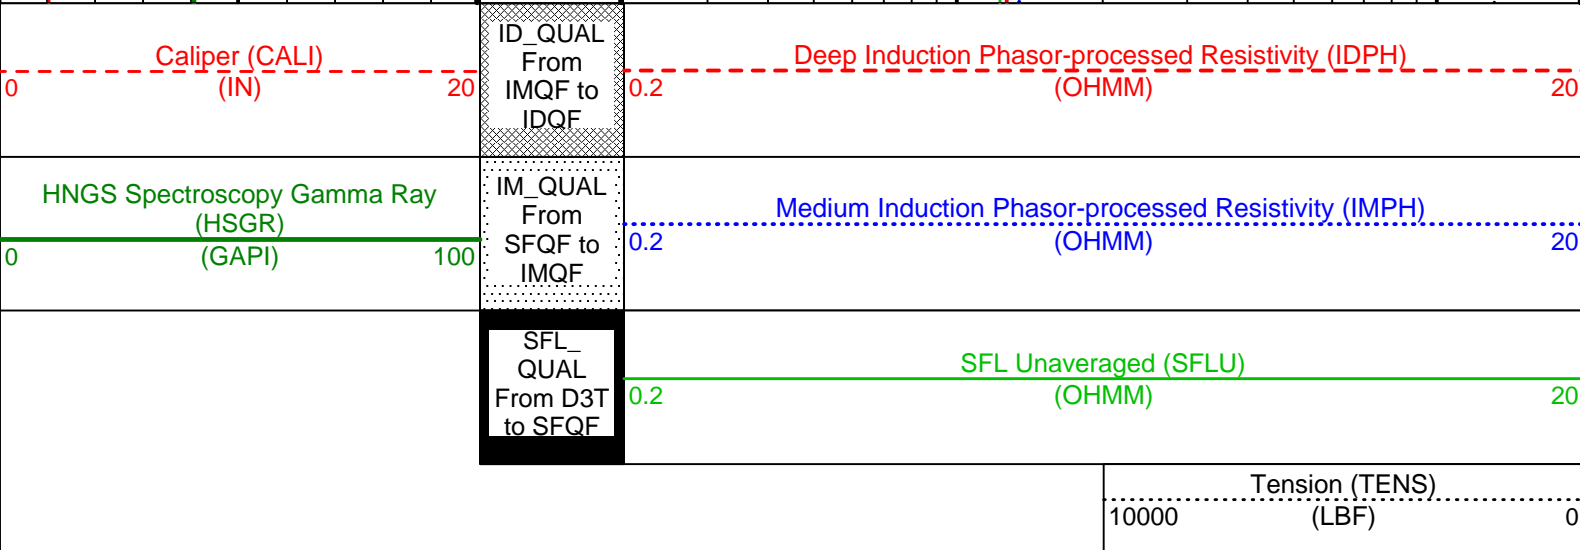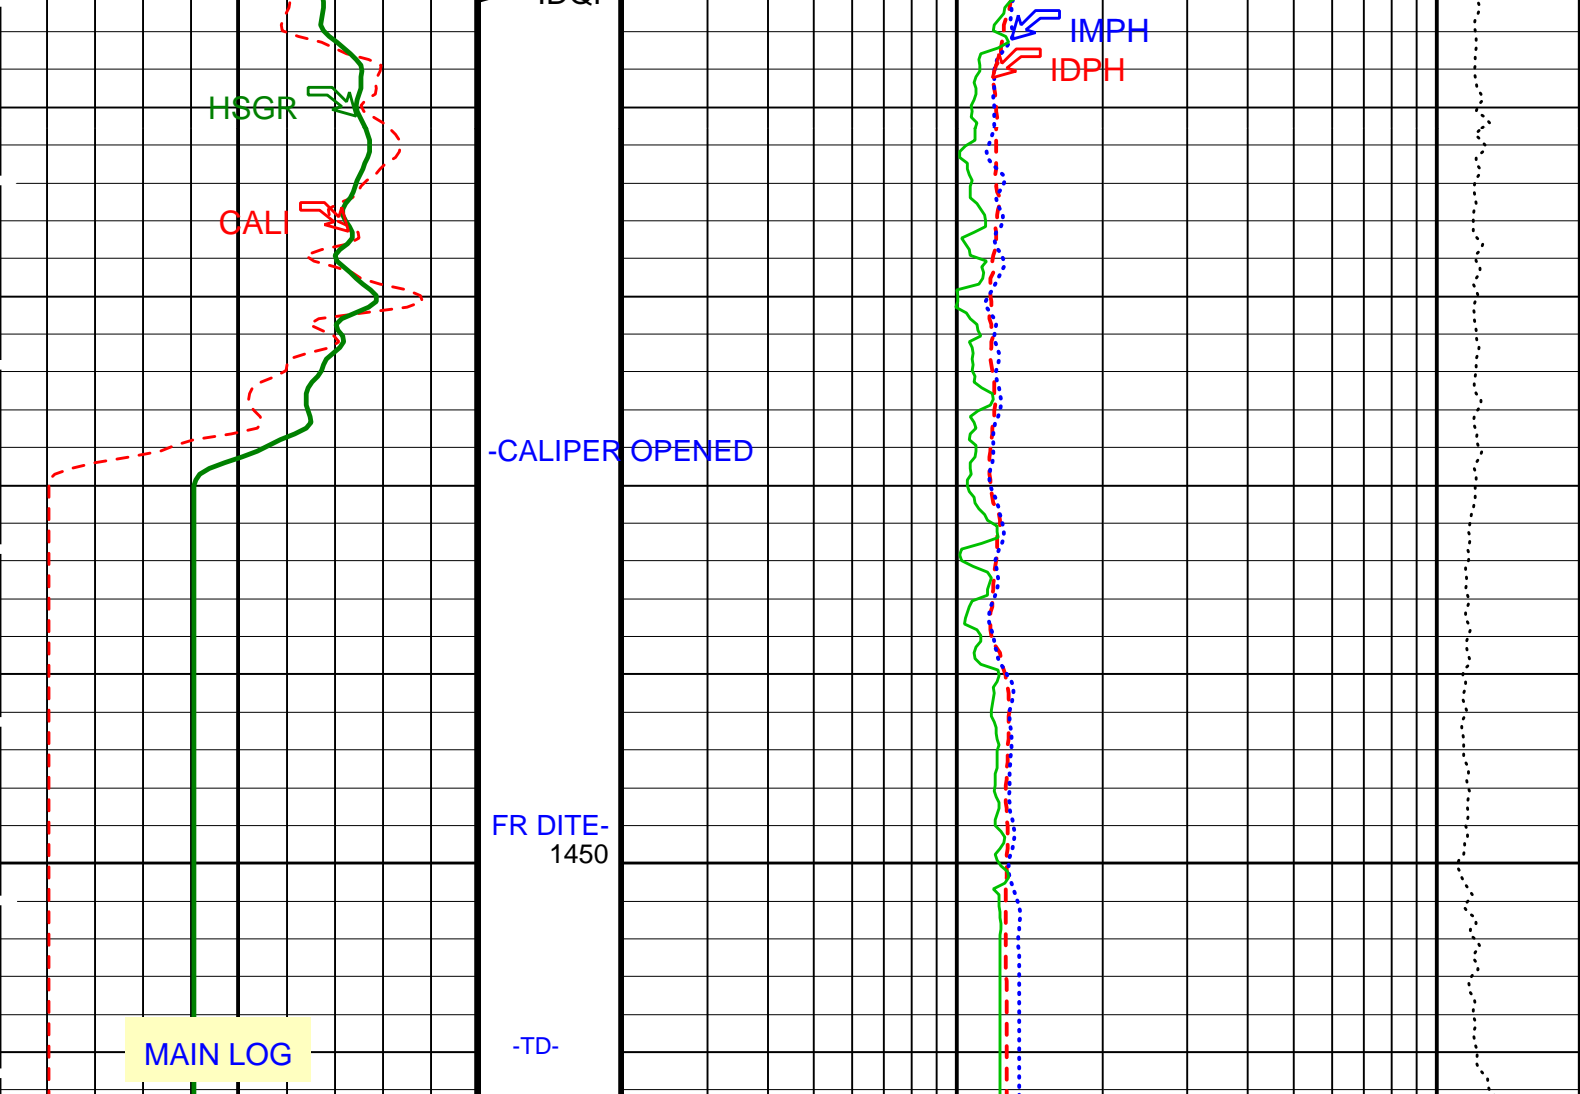

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value
DIT-E: Dual Induction - E		
BHS	Borehole Status	OPEN
BHT	Bottom Hole Temperature (used in calculations)	100 DEGC
DGF2	Deep 20 kHz Gain Factor	1.00789
DPH2	Deep 20 kHz Phase Shift	-0.152394 DEG
DRE2	Deep Real 20 kHz Sonde Error Correction	16.357 MM/M
DSR2	Deep Sigma Reference (20 kHz)	1843 MM/M
DXE2	Deep Quad 20 kHz Sonde Error Correction	64.6326 MM/M
GCSE	Generalized Caliper Selection	CALI
GDEV	Average Angular Deviation of Borehole from Normal	0 DEG

GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
IFRS	DIT-E Induction Frequency Selector	20	
IPHA	DIT-E Phasor Processing Mode	ALL	
IPRO	DIT-E Induction Processing Selector	PHASOR	
ITEN	DIT-E Temperature Enable	ENABLE	
MGF2	Medium 20 kHz Gain Factor	1.02964	
MPH2	Medium 20 kHz Phase Shift	-0.933067	DEG
MRE2	Medium Real 20 kHz Sonde Error Correction	-1.78642	MM/M
MSR2	Medium Sigma Reference (20 kHz)	3250	MM/M
MXE2	Medium Quad 20 kHz Sonde Error Correction	-34.2041	MM/M
SFCR	SFL Channel Ratio	1000	
SHT	Surface Hole Temperature	20	DEGC
APS-BA: Accelerator-Porosity Tool			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
SHT	Surface Hole Temperature	20	DEGC
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.00302511	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	NATU	
HNPE	HNGS Processing Enable	YES	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	1.3	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	ECCE	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.979098	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.987736	
System and Miscellaneous			
BS	Bit Size	9.875	IN
DFD	Drilling Fluid Density	1.10	G/C3
TD	Total Depth	-50000	M

Format: DITE_LogPhasor Vertical Scale: 1:200 Graphics File Created: 17-Aug-2002 18:36

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_005LUP	FN:6	PRODUCER	17-Aug-2002 18:36
REDUCE	PI_LDL_APS_NGS_005LUP	FN:7	PRODUCER	17-Aug-2002 18:36

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_008LUP	FN:10	PRODUCER	17-Aug-2002 20:13	1442.5 M	1291.2 M
REDUCE	PI_LDL_APS_NGS_008LUP	FN:11	PRODUCER	17-Aug-2002 20:13	1442.5 M	1291.2 M

OP System Version: 10C0-306

MCM



DIT-E 10C0-306
DTA-A 10C0-306
APS-BA OP10-KP1
DTC-H 10C0-306


HLDT-A 10C0-306
NPLC-B OP10-KP1
HNGS-BA OP10-KP1

PIP SUMMARY

Time Mark Every 60 S


Tension (TENS)
10000 (LBF) 0

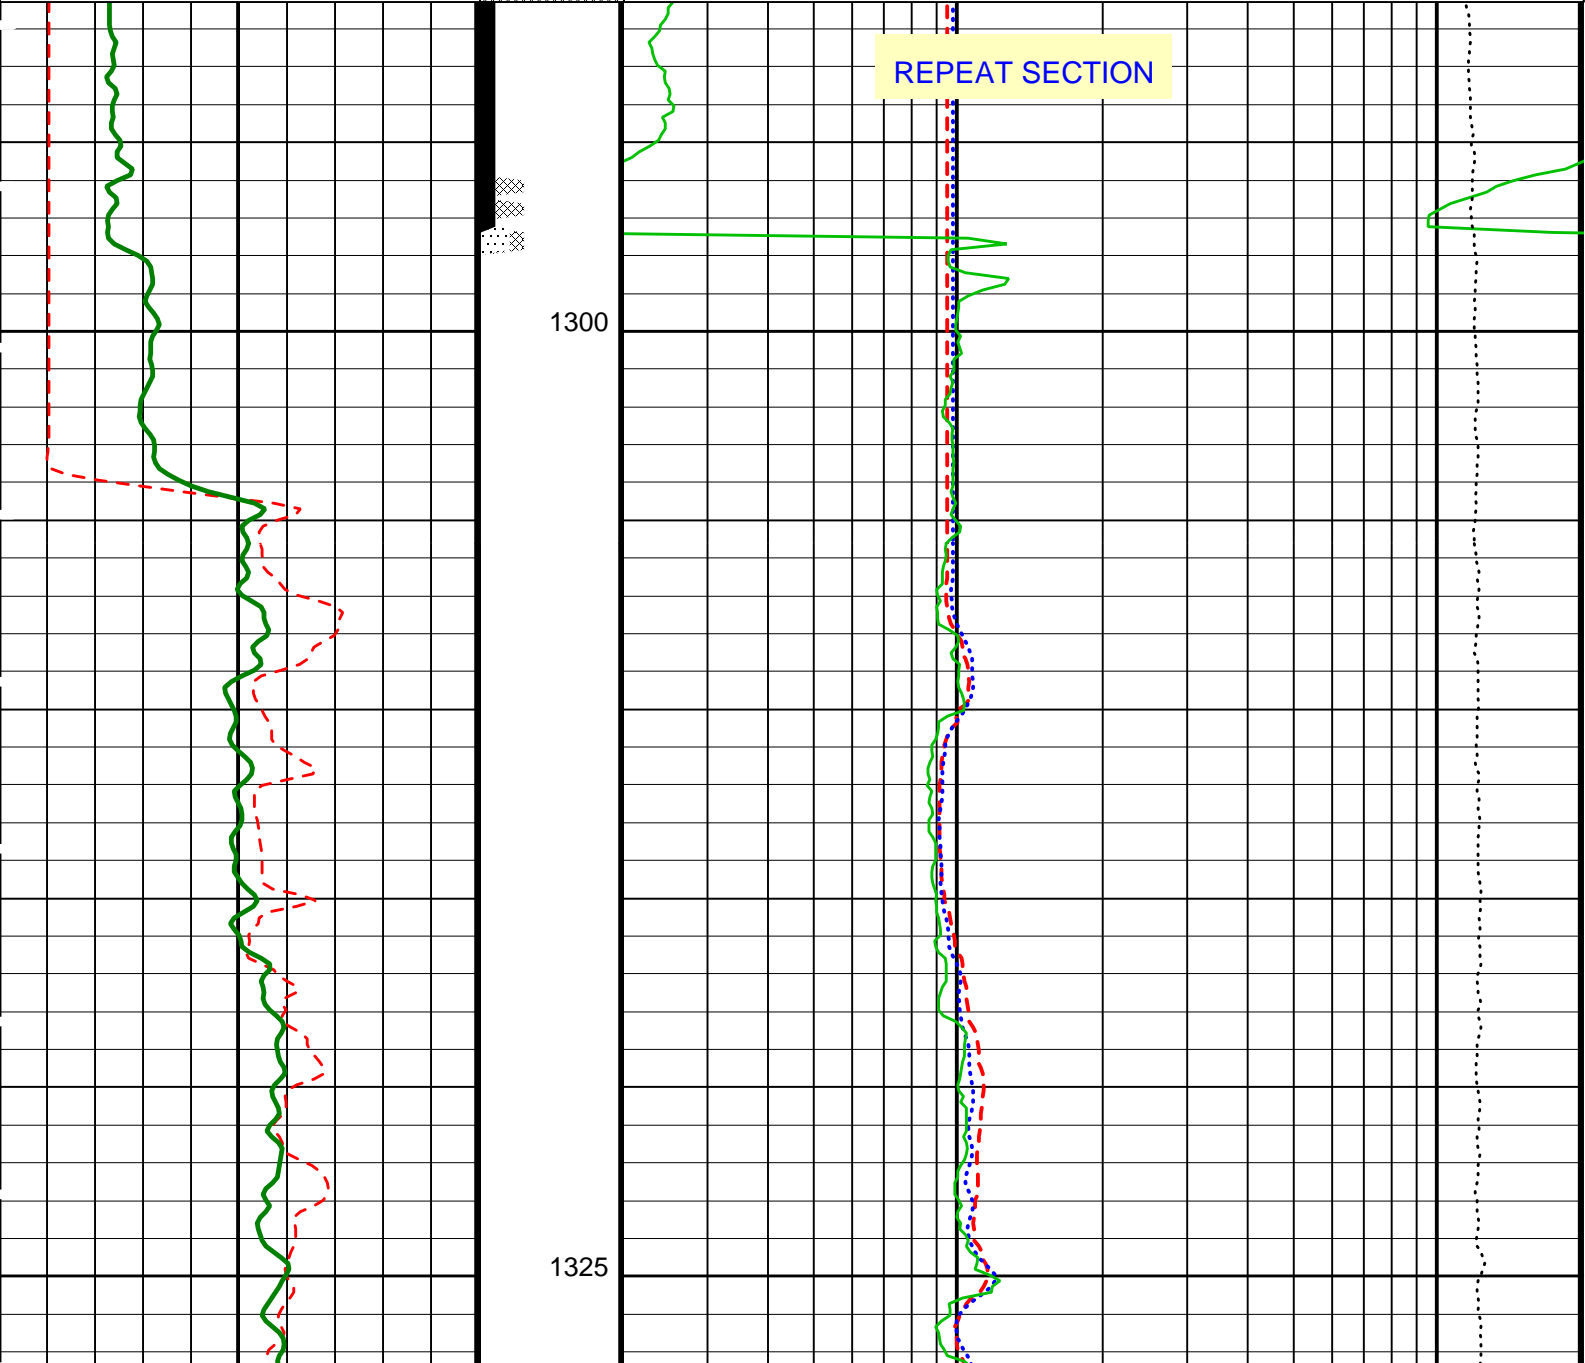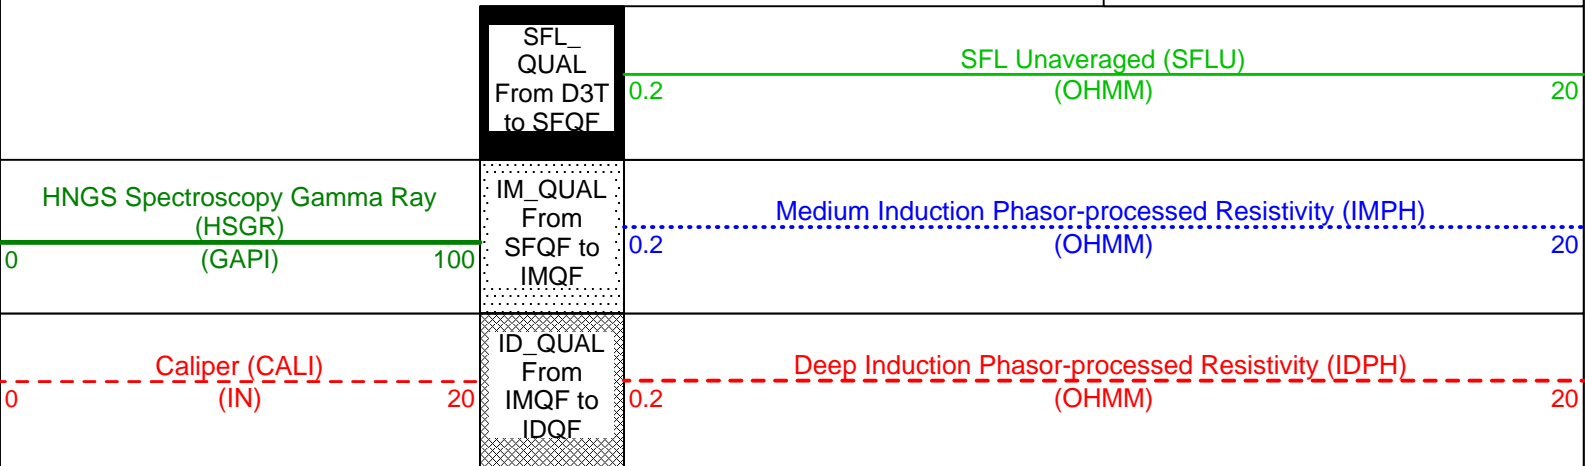


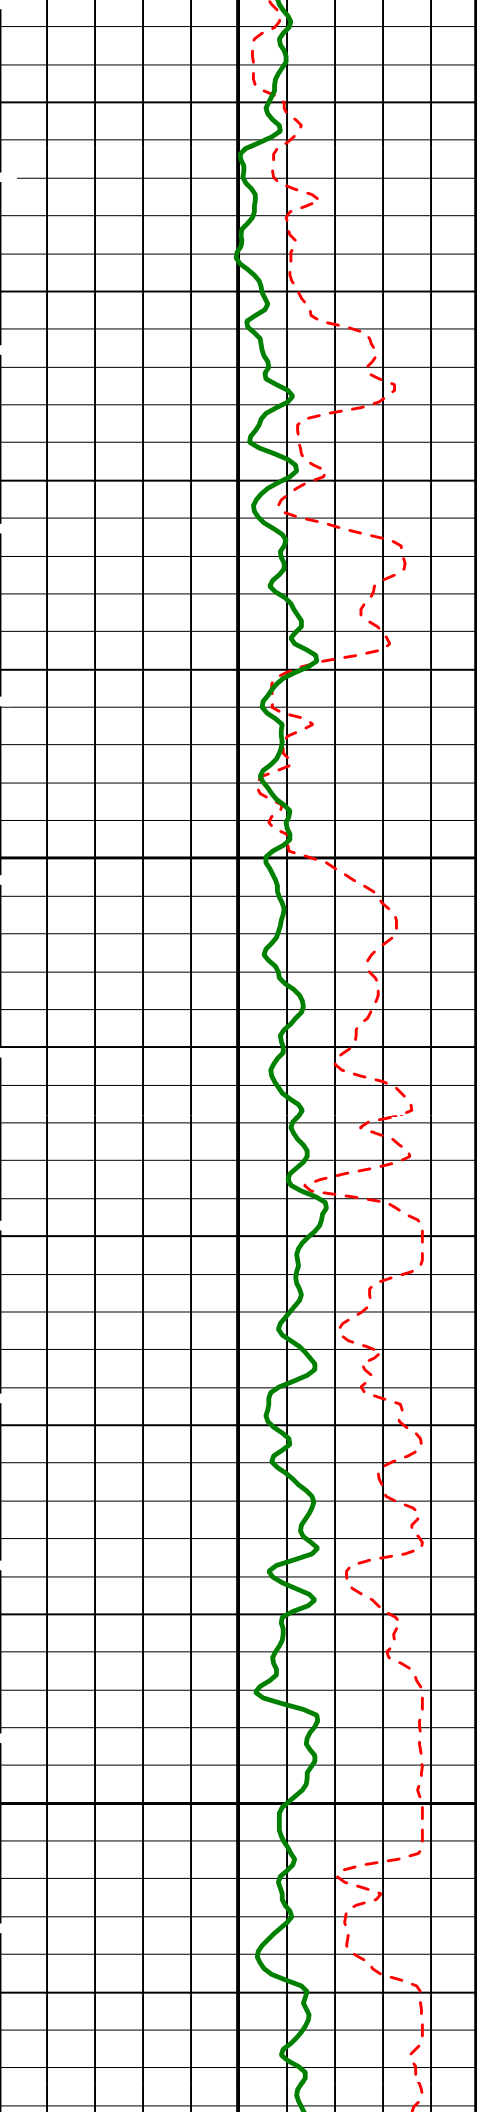

1350

1375

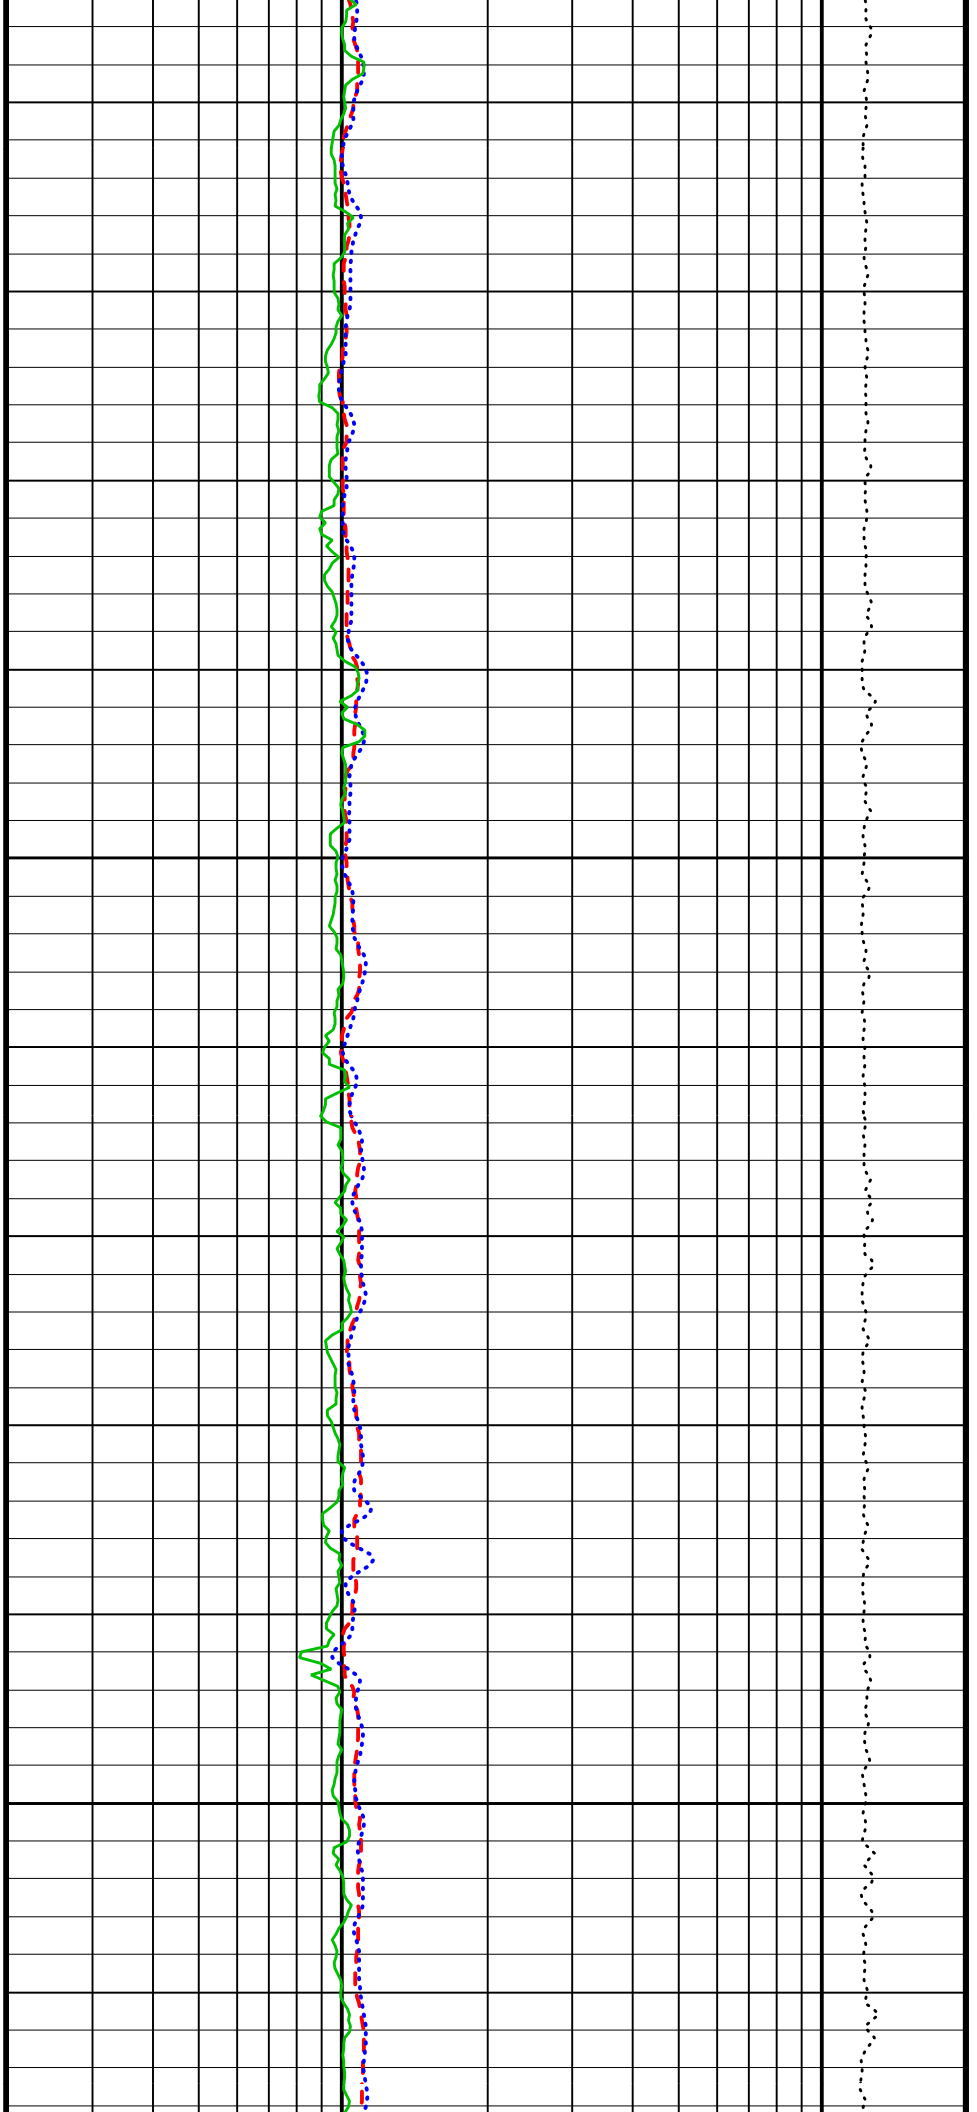

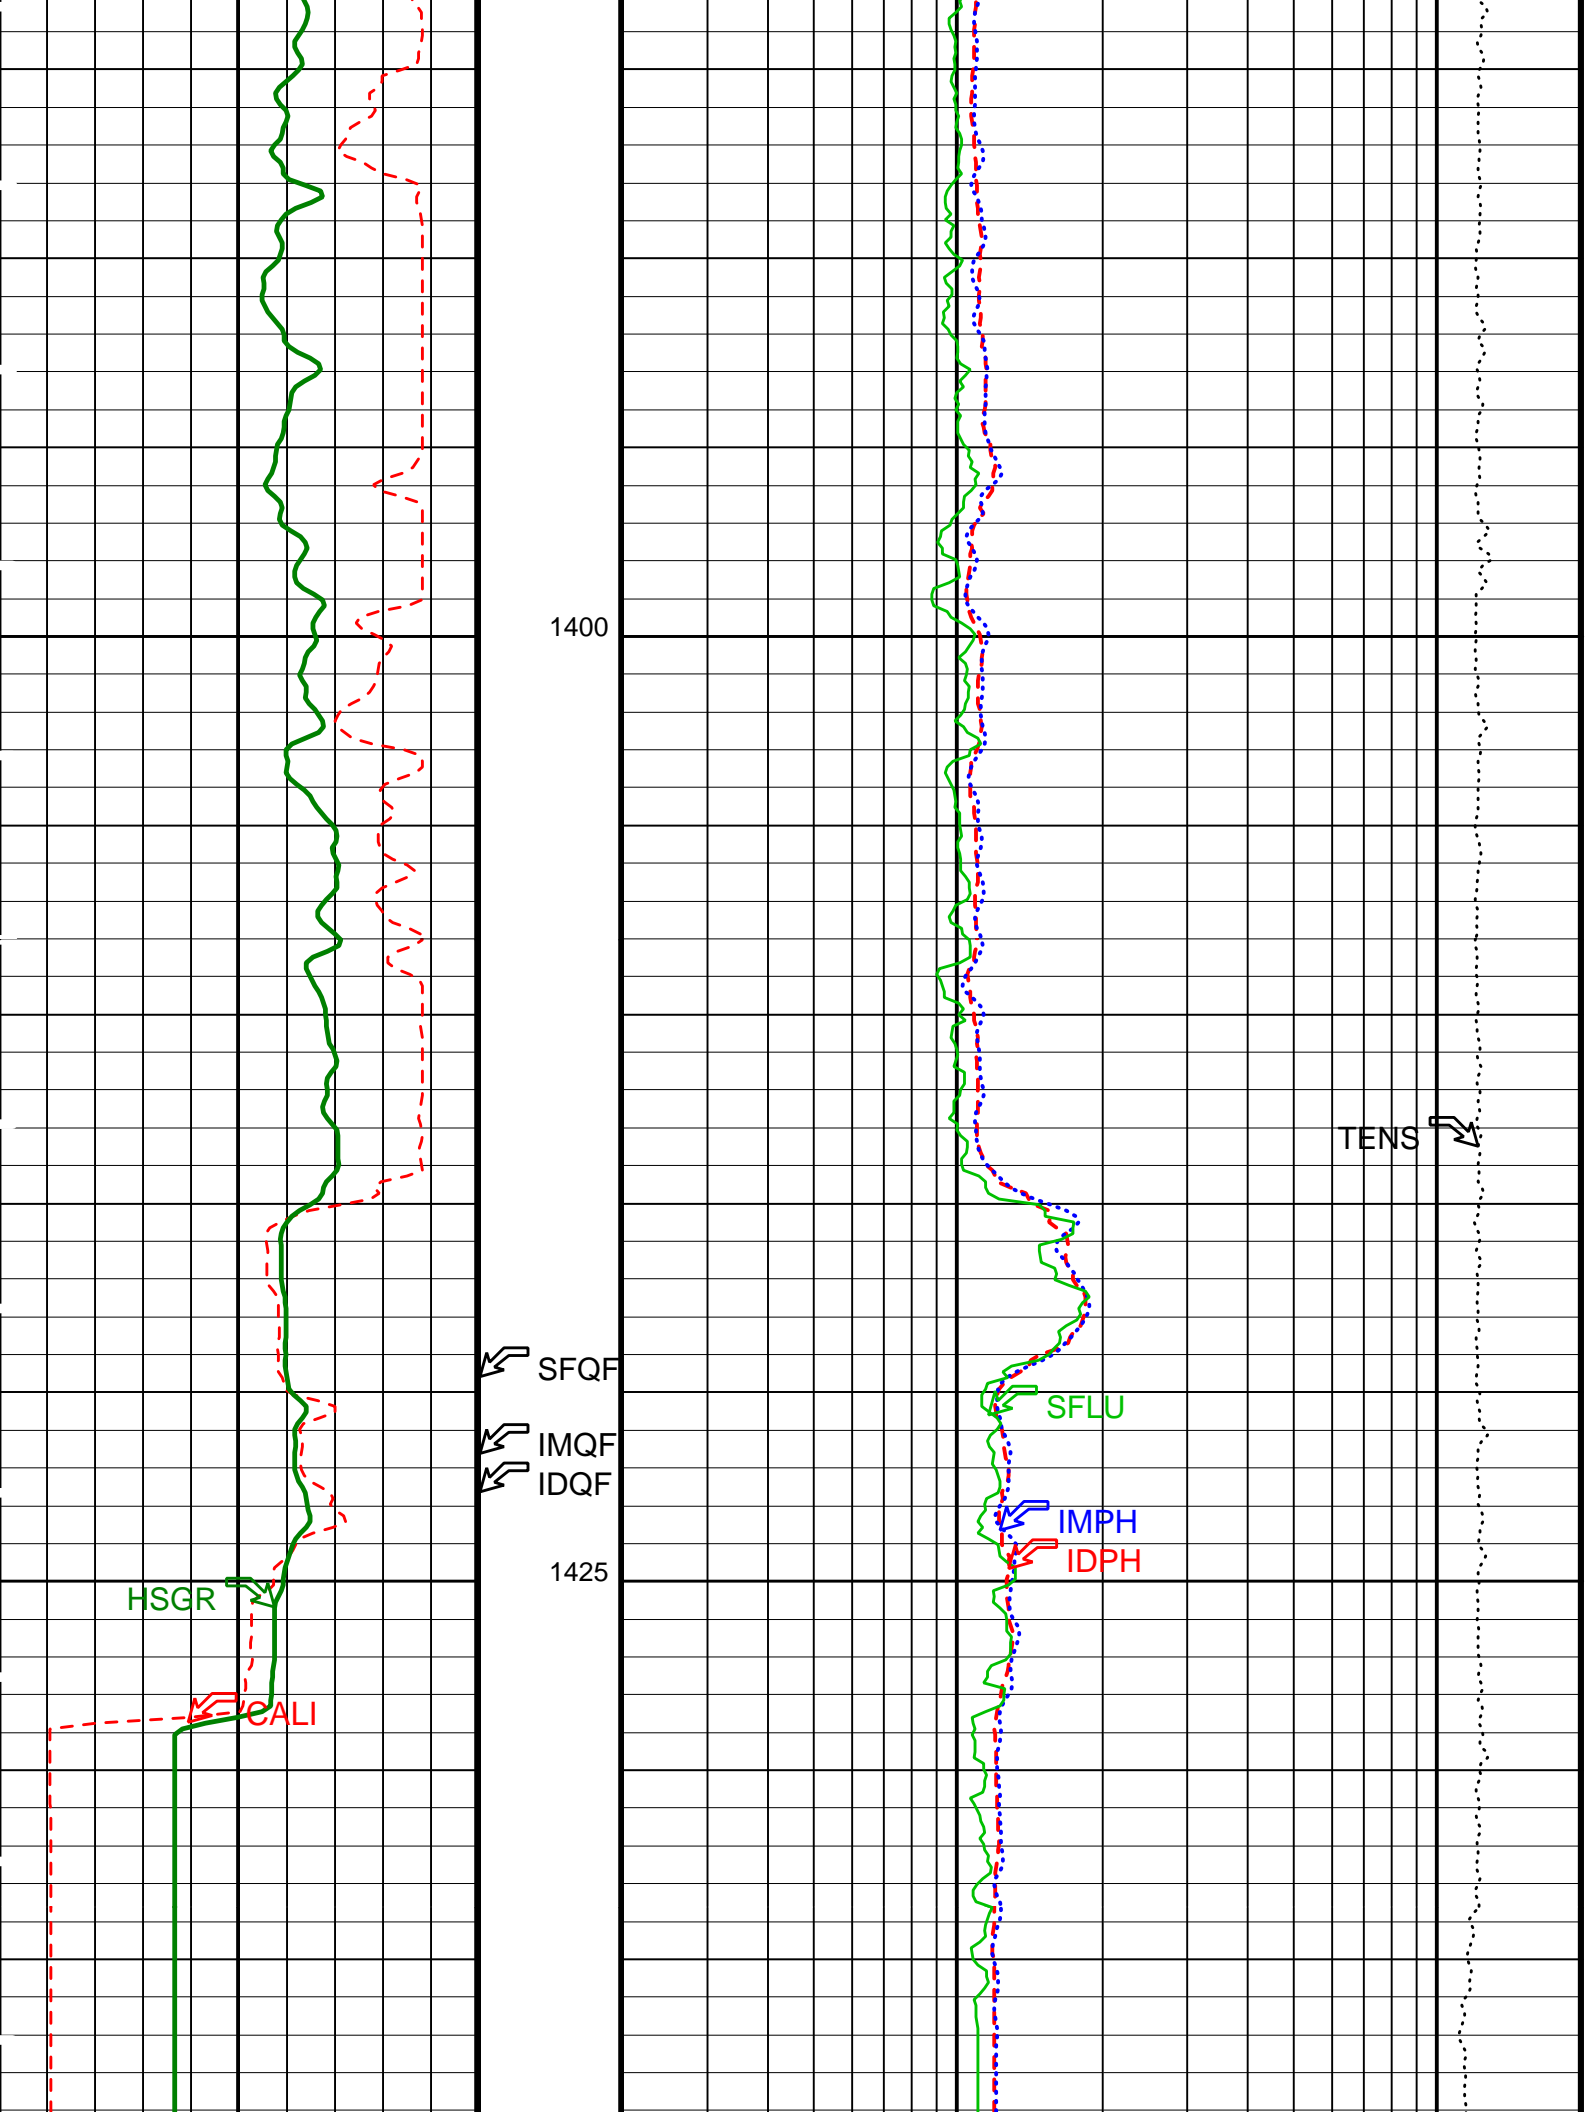

REPEAT SECTION

0	Caliper (CALI) (IN)	20	ID_QUAL From IMQF to IDQF	0.2	Deep Induction Phasor-processed Resistivity (IDPH) (OHMM)	20
0	HNGS Spectroscopy Gamma Ray (HSGR) (GAPI)	100	IM_QUAL From SFQF to IMQF	0.2	Medium Induction Phasor-processed Resistivity (IMPH) (OHMM)	20
0.2			SFL_QUAL From D3T to SFQF		SFL Unaveraged (SFLU) (OHMM)	20
10000					Tension (TENS) (LBF)	0

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value	
DIT-E: Dual Induction - E			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
DGF2	Deep 20 kHz Gain Factor	1.00789	
DPH2	Deep 20 kHz Phase Shift	-0.152394	DEG
DRE2	Deep Real 20 kHz Sonde Error Correction	16.357	MM/M
DSR2	Deep Sigma Reference (20 kHz)	1843	MM/M
DXE2	Deep Quad 20 kHz Sonde Error Correction	64.6326	MM/M
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
IFRS	DIT-E Induction Frequency Selector	20	
IPHA	DIT-E Phasor Processing Mode	ALL	
IPRO	DIT-E Induction Processing Selector	PHASOR	
ITEN	DIT-E Temperature Enable	ENABLE	
MGF2	Medium 20 kHz Gain Factor	1.02964	
MPH2	Medium 20 kHz Phase Shift	-0.933067	DEG
MRE2	Medium Real 20 kHz Sonde Error Correction	-1.78642	MM/M
MSR2	Medium Sigma Reference (20 kHz)	3250	MM/M
MXE2	Medium Quad 20 kHz Sonde Error Correction	-34.2041	MM/M
SFCR	SFL Channel Ratio	1000	
SHT	Surface Hole Temperature	20	DEGC
APS-BA: Accelerator-Porosity Tool			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
SHT	Surface Hole Temperature	20	DEGC
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	CALI	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HARK	HNGS Borehole Potassium Running Average	-0.0132519	

HADR	HNGS Borehole 1 Calcium Running Average	0.0132375	60	IN
HALF	HNGS Alpha Filter Length		NONE	
HCRB	HNGS Apply Borehole Potassium Correction		NATU	
HMWM	Mud Weighting Material		YES	
HNPE	HNGS Processing Enable		1.3	CPS
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate		1.3	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate		YES	
SGRC	HNGS Standard Gamma-Ray Correction Flag		20	DEGC
SHT	Surface Hole Temperature		ECCE	
TPOS	Tool Position		0.940387	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average		0.946835	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average			
System and Miscellaneous				
BS	Bit Size		9.875	IN
DFD	Drilling Fluid Density		1.10	G/C3
TD	Total Depth		-50000	M

Format: DITE_LogPhasor Vertical Scale: 1:200 Graphics File Created: 17-Aug-2002 20:13

OP System Version: 10C0-306 MCM

DIT-E	10C0-306	HLDT-A	10C0-306
DTA-A	10C0-306	NPLC-B	OP10-KP1
APS-BA	OP10-KP1	HNGS-BA	OP10-KP1
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_008LUP	FN:10	PRODUCER	17-Aug-2002 20:13
REDUCE	PI_LDL_APS_NGS_008LUP	FN:11	PRODUCER	17-Aug-2002 20:13

Calibration and Check Summary

Measurement	Nominal	Master	Before	After	Change	Limit	Units
Hostile Environment Litho Density - A Wellsite Calibration - Background Measurement							
Master: 11-Jun-2002 19:31 Before: 24-Jul-2002 12:39 After: 17-Aug-2002 22:47							
LSW1 Background	100.0	88.67	86.74	87.00	0.2697	0.03000	CPS
LSW2 Background	105.0	93.18	91.70	92.27	0.5778	0.03000	CPS
LSW3 Background	210.0	177.4	176.2	178.4	2.285	0.03000	CPS
LSW4 Background	290.0	236.8	236.6	234.4	-2.134	0.03000	CPS
LSW5 Background	610.0	518.0	517.3	519.6	2.307	0.03000	CPS
SSW1 Background	100.0	83.02	84.95	83.23	-1.720	0.03000	CPS
SSW2 Background	200.0	165.1	166.3	165.4	-0.9567	0.03000	CPS
SSW3 Background	530.0	440.7	439.6	439.0	-0.6002	0.03000	CPS
SSW4 Background	280.0	232.4	232.4	232.4	-0.07803	0.03000	CPS
SSW5 Background	205.0	174.0	173.3	174.2	0.8656	0.03000	CPS
Hostile Environment Litho Density - A Wellsite Calibration - Tool Quality Control Information High Voltage							
Master: 11-Jun-2002 19:31 Before: 24-Jul-2002 12:39 After: 17-Aug-2002 22:47							
LS Bkg. High Voltage	1133	1133	1130	1132	2.423	N/A	V
SS Bkg. High Voltage	1177	1177	1171	1173	2.729	N/A	V
Hostile Environment Litho Density - A Wellsite Calibration - Detectors Resolution From BKG Measurements							
Master: 11-Jun-2002 19:31 Before: 24-Jul-2002 12:39 After: 17-Aug-2002 22:47							
LS Background Resolution	1.000	1.032	1.032	1.045	0.01232	N/A	
SS Background Resolution	1.000	0.9430	0.9416	0.9470	0.005421	N/A	
Hostile Environment Litho Density - A Wellsite Calibration - Caliper Calibration							
Before: 24-Jul-2002 12:38							
Caliper Small Ring	12.00	N/A	17.14	N/A	N/A	N/A	IN
Caliper Large Ring	15.25	N/A	21.07	N/A	N/A	N/A	IN
Accelerator-Porosity Tool Wellsite Calibration - Detector Background							
Master: 24-Jul-2002 4:08 Before: 17-Aug-2002 19:06 After: 17-Aug-2002 21:56							
Near Det Bkg Cntrate	30.00	32.30	33.05	31.37	-1.683	N/A	CPS
Far Det Bkg Cntrate	30.00	33.62	31.89	33.37	1.480	N/A	CPS
Array-1 Det Bkg Cntrate	30.00	28.88	30.35	28.94	-1.405	N/A	CPS
Array-2 Det Bkg Cntrate	30.00	29.64	30.48	31.60	1.119	N/A	CPS
Array Therm Det Bkg Cntrate	30.00	32.75	32.38	34.97	2.589	N/A	CPS
Accelerator-Porosity Tool Wellsite Calibration - Calibration Ratios							
Master: 24-Jul-2002 4:08							
Near/Far Calibration Ratio	0.9250	0.9076	N/A	N/A	N/A	N/A	
Near/Array Calibration Ratio	1.030	1.066	N/A	N/A	N/A	N/A	

Near/Array Cal Ratio Up/Down	1.000	1.006	N/A	N/A	N/A	N/A	
Accelerator-Porosity Tool Wellsite Calibration - Tank Check							
Master: 24-Jul-2002 4:09							
Array-1 Standoff Porosity	11.75	11.51	N/A	N/A	N/A	N/A	PU
Array-2 Standoff Porosity	11.75	11.19	N/A	N/A	N/A	N/A	PU
Average Slowing Down Time	6.000	5.884	N/A	N/A	N/A	N/A	US
Array-1 SDT Ratio Up/Down	1.000	0.9901	N/A	N/A	N/A	N/A	
Array-2 SDT Ratio Up/Down	1.000	0.9732	N/A	N/A	N/A	N/A	
Sigma Formation	27.50	27.88	N/A	N/A	N/A	N/A	CU

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 1 Check							
Master: 12-Jul-2002 22:08 Before: 24-Jul-2002 7:59 After: 17-Aug-2002 22:42							
Na 511 Peak Loc	40.00	40.59	40.60	40.60	0.001640	1.000	
Na 511 Peak Res	15.50	16.79	16.89	16.43	-0.4574	2.000	%
High Voltage	1150	1224	1220	1220	0.04187	30.00	V
Na 1785 Peak Loc	142.6	145.1	146.3	145.2	-1.068	7.000	
Na 1785 Peak Res	8.500	10.40	8.694	9.013	0.3196	2.000	%
Temperature	15.50	24.98	22.43	20.67	-1.759	N/A	DEGC
Na Count Rate	45.00	50.31	49.89	49.45	-0.4335	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 2 Check							
Master: 12-Jul-2002 22:08 Before: 24-Jul-2002 7:59 After: 17-Aug-2002 22:42							
Na 511 Peak Loc	40.00	40.58	40.59	40.64	0.05220	1.000	
Na 511 Peak Res	15.50	16.72	16.53	16.53	0.0008736	2.000	%
High Voltage	1150	1253	1250	1247	-2.899	30.00	V
Na 1785 Peak Loc	142.6	144.7	144.3	144.9	0.6215	7.000	
Na 1785 Peak Res	8.500	9.766	9.897	9.235	-0.6618	2.000	%
Temperature	15.50	24.15	21.87	20.92	-0.9464	N/A	DEGC
Na Count Rate	45.00	50.19	49.39	49.20	-0.1973	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Ratio Of Detector 1 To Detector 2							
Master: 12-Jul-2002 22:08 Before: 24-Jul-2002 7:59 After: 17-Aug-2002 22:42							
Coincidence Count Rate Ratio	1.000	1.004	1.010	1.005	-0.004628	0.05000	

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 1 Calibration							
Master: 12-Jul-2002 22:01							
Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	208.9	--	--	--	--	
Th Peak Res	7.000	8.227	--	--	--	--	%
Background Count Rate	142.5	24.67	--	--	--	--	CPS
Gain Ratio	1.000	0.9793	--	--	--	--	

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 2 Calibration							
Master: 12-Jul-2002 22:01							
Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	208.8	--	--	--	--	
Th Peak Res	7.000	8.191	--	--	--	--	%
Background Count Rate	142.5	22.68	--	--	--	--	CPS
Gain Ratio	1.000	0.9792	--	--	--	--	

Accelerator-Porosity Tool - Detector Plateau Settings :							
Near Detector Plateau Setting	1748 V						
Far Detector Plateau Setting	2052 V						
Array Detector Plateau Setting	1969 V						

Dual Induction - E / Equipment Identification			
Primary Equipment:			
Dual Induction Sonde	DIS - HB	442	
Dual Induction Cartridge	DIC - EB	438	
Auxiliary Equipment:			
Mass Isolated Housing	MIH - ZA	417	

Dual Induction - E Wellsite Calibration											
Induction Electronics (10 kHz)											
Phase	ID Elect Real Offset 10 kHz	MM/M	Value	Phase	ID Elect Real Gain 10 kHz	Value	Phase	ID Elect Phase 10 kHz	DEG	Value	
Before			37.53	Before		0.9770	Before			10.63	
	-262.8 (Minimum)	37.15 (Nominal)	337.2 (Maximum)		0.8294 (Minimum)	0.9794 (Nominal)	1.171 (Maximum)		0.6325 (Minimum)	10.63 (Nominal)	20.63 (Maximum)
Phase	ID Elect Quad Offset 10 kHz	MM/M	Value	Phase	ID Elect Quad Gain 10 kHz	Value	Phase	IM Elect Phase 10 kHz	DEG	Value	

Before		22.25	Before		0.9660	Before		13.27
-277.5 (Minimum)	22.53 (Nominal)	322.5 (Maximum)	0.8193 (Minimum)	0.9693 (Nominal)	1.157 (Maximum)	3.310 (Minimum)	13.31 (Nominal)	23.31 (Maximum)
Phase	IM Elect Real Offset 10 kHz	MM/M	Value	Phase	IM Elect Real Gain 10 kHz	Value		
Before		96.05	Before		0.9527			
-453.5 (Minimum)	96.54 (Nominal)	646.5 (Maximum)	0.8074 (Minimum)	0.9574 (Nominal)	1.140 (Maximum)			
Phase	IM Elect Quad Offset 10 kHz	MM/M	Value	Phase	IM Elect Quad Gain 10 kHz	Value		
Before		94.74	Before		0.9503			
-454.8 (Minimum)	95.18 (Nominal)	645.2 (Maximum)	0.8055 (Minimum)	0.9555 (Nominal)	1.137 (Maximum)			

Before: 24-Jul-2002 8:24

Dual Induction - E Wellsite Calibration										
Induction Electronics (20 kHz)										
Phase	ID Elect Real Offset 20 kHz	MM/M	Value	Phase	ID Elect Real Gain 20 kHz	Value	Phase	ID Elect Phase 20 kHz	DEG	Value
Before		14.85	Before		1.004	Before		9.036		
-110.3 (Minimum)	14.68 (Nominal)	139.7 (Maximum)	0.8551 (Minimum)	1.005 (Nominal)	1.207 (Maximum)	-5.718 (Minimum)	9.282 (Nominal)	24.28 (Maximum)		
Phase	ID Elect Quad Offset 20 kHz	MM/M	Value	Phase	ID Elect Quad Gain 20 kHz	Value	Phase	IM Elect Phase 20 kHz	DEG	Value
Before		8.842	Before		0.9923	Before		12.07		
-115.9 (Minimum)	9.089 (Nominal)	134.1 (Maximum)	0.8445 (Minimum)	0.9945 (Nominal)	1.192 (Maximum)	-2.653 (Minimum)	12.35 (Nominal)	27.35 (Maximum)		
Phase	IM Elect Real Offset 20 kHz	MM/M	Value	Phase	IM Elect Real Gain 20 kHz	Value				
Before		39.82	Before		1.010					
-184.7 (Minimum)	40.31 (Nominal)	265.3 (Maximum)	0.8587 (Minimum)	1.009 (Nominal)	1.212 (Maximum)					
Phase	IM Elect Quad Offset 20 kHz	MM/M	Value	Phase	IM Elect Quad Gain 20 kHz	Value				
Before		39.36	Before		1.007					
-185.2 (Minimum)	39.80 (Nominal)	264.8 (Maximum)	0.8566 (Minimum)	1.007 (Nominal)	1.209 (Maximum)					

Before: 24-Jul-2002 7:54

Dual Induction - E Wellsite Calibration										
Induction Electronics (40 kHz)										
Phase	ID Elect Real Offset 40 kHz	MM/M	Value	Phase	ID Elect Real Gain 40 kHz	Value	Phase	ID Elect Phase 40 kHz	DEG	Value
Before		9.741	Before		0.9887	Before		27.54		
-75.43 (Minimum)	9.570 (Nominal)	94.57 (Maximum)	0.8395 (Minimum)	0.9895 (Nominal)	1.185 (Maximum)	9.068 (Minimum)	29.07 (Nominal)	49.07 (Maximum)		
Phase	ID Elect Quad Offset 40 kHz	MM/M	Value	Phase	ID Elect Quad Gain 40 kHz	Value	Phase	IM Elect Phase 40 kHz	DEG	Value
Before		5.856	Before		0.9765	Before		31.11		
-79.10 (Minimum)	5.897 (Nominal)	90.90 (Maximum)	0.8281 (Minimum)	0.9781 (Nominal)	1.169 (Maximum)	12.68 (Minimum)	32.68 (Nominal)	52.68 (Maximum)		
Phase	IM Elect Real Offset 40 kHz	MM/M	Value	Phase	IM Elect Real Gain 40 kHz	Value				
Before		26.08	Before		1.025					
-103.8 (Minimum)	26.19 (Nominal)	156.2 (Maximum)	0.8673 (Minimum)	1.017 (Nominal)	1.224 (Maximum)					
Phase	IM Elect Quad Offset 40 kHz	MM/M	Value	Phase	IM Elect Quad Gain 40 kHz	Value				
Before		25.86	Before		1.022					
-104.1 (Minimum)	25.92 (Nominal)	155.9 (Maximum)	0.8649 (Minimum)	1.015 (Nominal)	1.221 (Maximum)					

Before: 24-Jul-2002 8:26

Dual Induction - E Wellsite Calibration						
SFL Electronics						
Phase	SFL Voltage Offset	MV	Value	Phase	SFL Voltage Gain	Value
Before		1.196	Before		1.016	
-15.00 (Minimum)	0 (Nominal)	15.00 (Maximum)	0.8500 (Minimum)	1.000 (Nominal)	1.200 (Maximum)	
Phase	SFL Current Offset	MA	Value	Phase	SFL Current Gain	Value
Before		0.005420	Before		0.9940	
-0.6000 (Minimum)	0 (Nominal)	0.6000 (Maximum)	0.8500 (Minimum)	1.000 (Nominal)	1.200 (Maximum)	

Before: 24-Jul-2002 7:55

Dual Induction - E Wellsite Calibration

Electronics Calibration Changes Files/Depth Intervals:

Phase	ID (R > 27 OHM-M) MM/M	Value	Phase	ID (R < 27 OHM-M) %	Value	Phase	SFL (R < 1 OHM-M) OHMM	Value
After	EXCEEDS LIMIT	1.725	After		0.0003296	After		0.0006499
	0 (Minimum) 0 (Nominal) 0.7500 (Maximum)			0 (Minimum) 0 (Nominal) 2.000 (Maximum)			0 (Minimum) 0 (Nominal) 0.02000 (Maximum)	
Phase	IM (R > 27 OHM-M) MM/M	Value	Phase	IM (R < 27 OHM-M) %	Value			
After	EXCEEDS LIMIT	2.793	After		0.0002653			
	0 (Minimum) 0 (Nominal) 0.7500 (Maximum)			0 (Minimum) 0 (Nominal) 2.000 (Maximum)				
Phase	SFL (R > 27 OHM-M) MM/M	Value	Phase	SFL (R < 27 OHM-M) %	Value			
After		0	After		0.0005378			
	0 (Minimum) 0 (Nominal) 0.7500 (Maximum)			0 (Minimum) 0 (Nominal) 2.000 (Maximum)				

After: 17-Aug-2002 21:48

Dual Induction - E Master Calibration

Test Loop Calibration: Calibration of Internal Reference to Test Loop Standard

Phase	Deep 10 kHz Gain Factor	Value	Phase	Deep 20 kHz Gain Factor	Value	Phase	Deep 40 kHz Gain Factor	Value
Master		0.9956	Master		1.008	Master		1.026
	0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)			0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)			0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)	
Phase	Medium 10 kHz Gain Factor	Value	Phase	Medium 20 kHz Gain Factor	Value	Phase	Medium 40 kHz Gain Factor	Value
Master		1.022	Master		1.030	Master		1.061
	0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)			0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)			0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)	
Phase	Deep 10 kHz Phase Shift	Value	Phase	Deep 20 kHz Phase Shift	Value	Phase	Deep 40 kHz Phase Shift	Value
Master		0.1143	Master		-0.1524	Master		-1.426
	-1.500 (Minimum) 0 (Nominal) 1.500 (Maximum)			-2.000 (Minimum) 0 (Nominal) 2.000 (Maximum)			-4.000 (Minimum) -1.000 (Nominal) 2.000 (Maximum)	
Phase	Medium 10 kHz Phase Shift	Value	Phase	Medium 20 kHz Phase Shift	Value	Phase	Medium 40 kHz Phase Shift	Value
Master		-0.2558	Master		-0.9331	Master		-2.461
	-1.500 (Minimum) 0 (Nominal) 1.500 (Maximum)			-3.000 (Minimum) -1.000 (Nominal) 1.000 (Maximum)			-5.000 (Minimum) -2.000 (Nominal) 1.000 (Maximum)	

Master: Calibration out of date 5-Oct-2001 21:50

Dual Induction - E Master Calibration

Sonde Error Corrections: Correction for sonde response in zero conductivity environment. (Normalized to 25C).

Phase	Real Deep 10 kHz S.E. Corr.	Value	Phase	Real Deep 20 kHz S.E. Corr.	Value	Phase	Real Deep 40 kHz S.E. Corr.	Value
Master		44.95	Master		16.36	Master		4.690
	-50.00 (Minimum) 0 (Nominal) 125.0 (Maximum)			-30.00 (Minimum) 0 (Nominal) 30.00 (Maximum)			-15.00 (Minimum) 0 (Nominal) 15.00 (Maximum)	
Phase	Quad Deep 10 kHz S.E. Corr.	Value	Phase	Quad Deep 20 kHz S.E. Corr.	Value	Phase	Quad Deep 40 kHz S.E. Corr.	Value
Master		108.9	Master		64.63	Master		46.10
	-250.0 (Minimum) 0 (Nominal) 350.0 (Maximum)			-125.0 (Minimum) 0 (Nominal) 200.0 (Maximum)			-75.00 (Minimum) 0 (Nominal) 125.0 (Maximum)	
Phase	Real Medium 10 kHz S.E. Corr.	Value	Phase	Real Medium 20 kHz S.E. Corr.	Value	Phase	Real Medium 40 kHz S.E. Corr.	Value
Master		20.73	Master		-1.786	Master		-10.46
	-50.00 (Minimum) 0 (Nominal) 140.0 (Maximum)			-50.00 (Minimum) 0 (Nominal) 50.00 (Maximum)			-30.00 (Minimum) 0 (Nominal) 30.00 (Maximum)	
Phase	Quad Medium 10 kHz S.E. Corr.	Value	Phase	Quad Medium 20 kHz S.E. Corr.	Value	Phase	Quad Medium 40 kHz S.E. Corr.	Value
Master		-105.8	Master		-34.20	Master		11.45
	-1300 (Minimum) 0 (Nominal) 1300 (Maximum)			-650.0 (Minimum) 0 (Nominal) 650.0 (Maximum)			-350.0 (Minimum) 0 (Nominal) 350.0 (Maximum)	

Master: Calibration out of date 5-Oct-2001 22:22

Hostile Environment Litho Density - A / Equipment Identification

Primary Equipment:

HOSTILE ENVIRONMENT LITHO DENSITY HIGH V
 HOSTILE ENVIRONMENT LITHO DENSITY CARTRI
 Gamma Source Radioactive

HLDV - A 10
 HLDC - AA 11
 GSR - Z 1846

Auxiliary Equipment:

HOSTILE ENVIRONMENT LITHO DENSITY SONDE

HLDS - B 10

HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG
 HOSTILE ENVIRONMENT ELECTRONICS CARTRIDG
 HOSTILE ENVIRONMENT LITHO DENSITY PAD

HEH - H 12
 HEH - G 11
 HLDP - B 10

Nuclear Porosity Lithology Cartridge - B / Equipment Identification

Primary Equipment:
 NPLC Cartridge NPLC - B 79

Auxiliary Equipment:
 NPLC Housing NPH - B 82

Accelerator-Porosity Tool / Equipment Identification

Primary Equipment:
 Accelerator-Porosity Sonde APS - BA 22
 APS Minitron MNTR - F 4185

Auxiliary Equipment:
 Accelerator-Porosity Housing APH - AC 22
 APS Calibration Water Tank SFT - 178 4722
 APS Aluminium Calibrator Sleeve SFT - 281 24

Hostile Natural Gamma Ray Sonde / Equipment Identification

Primary Equipment:
 HNGS Sonde HNGS - BA 77

Auxiliary Equipment:
 HNGS Sonde Housing HNSH - BA 79
 Gamma Source Radioactive GSR - U 135

Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 1 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.59	Master		16.79	Master		1224
Before		40.60	Before		16.89	Before		1220
After		40.60	After		16.43	After		1220
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Phase	Na 1785 Peak Loc	Value	Phase	Na 1785 Peak Res %	Value	Phase	Temperature DEGC	Value
Master		145.1	Master		10.40	Master		24.98
Before		146.3	Before		8.694	Before		22.43
After		145.2	After		9.013	After		20.67
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Phase	Na Count Rate CPS	Value						
Master		50.31						
Before		49.89						
After		49.45						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 12-Jul-2002 22:08			Before: 24-Jul-2002 7:59			After: 17-Aug-2002 22:42		

Hostile Natural Gamma Ray Sonde Wellsite Calibration

Detector 2 Check

Phase	Na 511 Peak Loc	Value	Phase	Na 511 Peak Res %	Value	Phase	High Voltage V	Value
Master		40.58	Master		16.72	Master		1253
Before		40.59	Before		16.53	Before		1250

After		40.64	After		9.235	16.53	After		20.92	1247	
37.50 (Minimum)	40.00 (Nominal)	42.50 (Maximum)	12.00 (Minimum)	15.50 (Nominal)	19.00 (Maximum)	900.0 (Minimum)	1150 (Nominal)	1600 (Maximum)			
Phase	Na 1785 Peak Loc		Value	Phase	Na 1785 Peak Res %		Value	Phase	Temperature DEGC		Value
Master		144.7	Master		9.766	Master		24.15			
Before		144.3	Before		9.897	Before		21.87			
After		144.9	After		9.235	After		20.92			
135.0 (Minimum)	142.6 (Nominal)	150.3 (Maximum)	7.000 (Minimum)	8.500 (Nominal)	11.00 (Maximum)	-28.89 (Minimum)	15.50 (Nominal)	60.00 (Maximum)			
Phase	Na Count Rate CPS		Value								
Master		50.19									
Before		49.39									
After		49.20									
10.00 (Minimum)	45.00 (Nominal)	100.0 (Maximum)									
Master: 12-Jul-2002 22:08			Before: 24-Jul-2002 7:59				After: 17-Aug-2002 22:42				

Hostile Natural Gamma Ray Sonde Wellsite Calibration		
Ratio Of Detector 1 To Detector 2		
Phase	Coincidence Count Rate Ratio	Value
Master		1.004
Before		1.010
After		1.005
0.9500 (Minimum)	1.000 (Nominal)	1.050 (Maximum)
Master: 12-Jul-2002 22:08		
Before: 24-Jul-2002 7:59		
After: 17-Aug-2002 22:42		

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 1 Calibration								
Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value
Master		41.00	Master		208.9	Master		8.227
38.00 (Minimum)	40.00 (Nominal)	42.00 (Maximum)	201.0 (Minimum)	209.6 (Nominal)	218.3 (Maximum)	5.000 (Minimum)	7.000 (Nominal)	9.000 (Maximum)
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value			
Master		24.67	Master		0.9793			
20.00 (Minimum)	142.5 (Nominal)	265.0 (Maximum)	0.9400 (Minimum)	1.000 (Nominal)	1.060 (Maximum)			
Master: 12-Jul-2002 22:01								

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 2 Calibration								
Phase	Na 511 Peak Set Point	Value	Phase	Th Peak Loc	Value	Phase	Th Peak Res %	Value
Master		41.00	Master		208.8	Master		8.191
38.00 (Minimum)	40.00 (Nominal)	42.00 (Maximum)	201.0 (Minimum)	209.6 (Nominal)	218.3 (Maximum)	5.000 (Minimum)	7.000 (Nominal)	9.000 (Maximum)
Phase	Background Count Rate CPS	Value	Phase	Gain Ratio	Value			
Master		22.68	Master		0.9792			
20.00 (Minimum)	142.5 (Nominal)	265.0 (Maximum)	0.9400 (Minimum)	1.000 (Nominal)	1.060 (Maximum)			
Master: 12-Jul-2002 22:01								

Well: ODP Leg 204, Site 1251H
Field: Hydrate Ridge
Ocean: Pacific
State: Oregon

Phasor Induction

Natural Gamma Ray