

Company: Lamont Doherty

Well: ODP Leg 207 Site 1257A

Field: Demarara Rise

Country: Venezuela

Ocean: Atlantic

Country: Venezuela
Field: Demarara Rise
Location: 9.4538 Deg North, 54.342 Deg V
Well: ODP Leg 207 Site 1257A
Company: Lamont Doherty

HLDS/APS Porosity Natural Gamma Ray		9.4538 Deg North, 54.342 Deg West	Elev.: K.B. 11.3 m G.L. -2962 m D.F. 11 m
Permanent Datum:		MSL	Elev.: 0 m
Log Measured From:		DES	11.3 m above Perm. Datum
Drilling Measured From:		DES	
API Serial No.	Max. Hole Devi.	Longitude	Latitude

Logging Date	18-Jan-2003
Run Number	1
Depth Driller	3246 m
Schlumberger Depth	3249 m
Bottom Log Interval	3234 m
Top Log Interval	2962 m
Casing Driller Size @ Depth	0.000 in @ 3032 m
Casing Schlumberger	3036 m
Bit Size	11.438 in
Type Fluid In Hole	Sepiolite Salt Water
Density	1.1 g/cm3
Fluid Loss	PH
Source Of Sample	Mudpit
RM @ Measured Temperature	0.258 ohm.m @ 32 degC
RMF @ Measured Temperature	@ @
RMC @ Measured Temperature	@ @
Source RMF	RMC
RM @ MRT	0.415 @ 12 @ 12
Maximum Recorded Temperatures	12 degC
Circulation Stopped	Time
Logger On Bottom	18-Jan-2003 18:53
Unit Number	99 Houston, TX ODP
Recorded By	K. Swain
Witnessed By	B. Rea, F. Heidersdorf

Logging Date	Run 1	Run 2	Run
Run Number			
Depth Driller			
Schlumberger Depth			
Bottom Log Interval			
Top Log Interval			
Casing Driller Size @ Depth	@		
Casing Schlumberger			
Bit Size			
Type Fluid In Hole			
Density			
Fluid Loss	PH		
Source Of Sample			
RM @ Measured Temperature	@		
RMF @ Measured Temperature	@ @		
RMC @ Measured Temperature	@ @		
Source RMF	RMC		
RM @ MRT	@ @ 12 @ 12		
Maximum Recorded Temperatures			
Circulation Stopped	Time		
Logger On Bottom	Time		
Unit Number	Location		
Recorded By			
Witnessed By			

Logging Date	18-Jan-2003
Run Number	1
Depth Driller	3246 m
Schlumberger Depth	3249 m
Bottom Log Interval	3234 m
Top Log Interval	2962 m
Casing Driller Size @ Depth	0.000 in @ 3032 m
Casing Schlumberger	3036 m
Bit Size	11.438 in
Type Fluid In Hole	Sepiolite Salt Water
Density	1.1 g/cm3
Fluid Loss	PH
Source Of Sample	Mudpit
RM @ Measured Temperature	0.258 ohm.m @ 32 degC
RMF @ Measured Temperature	@ @
RMC @ Measured Temperature	@ @
Source RMF	RMC
RM @ MRT	0.415 @ 12 @ 12
Maximum Recorded Temperatures	12 degC
Circulation Stopped	Time
Logger On Bottom	18-Jan-2003 18:53
Unit Number	99 Houston, TX ODP
Recorded By	K. Swain
Witnessed By	B. Rea, F. Heidersdorf

DISCLAIMER

THE USE OF AND RELIANCE UPON THIS RECORDED-DATA BY THE HEREIN NAMED COMPANY (AND ANY OF ITS AFFILIATES, PARTNERS, REPRESENTATIVES, AGENTS, CONSULTANTS AND EMPLOYEES) IS SUBJECT TO THE TERMS AND CONDITIONS AGREED UPON BETWEEN SCHLUMBERGER AND THE COMPANY, INCLUDING: (a) RESTRICTIONS ON USE OF THE RECORDED-DATA; (b) DISCLAIMERS AND WAIVERS OF WARRANTIES AND REPRESENTATIONS REGARDING COMPANY'S USE OF AND RELIANCE UPON THE RECORDED-DATA; AND (c) CUSTOMER'S FULL AND SOLE RESPONSIBILITY FOR ANY INFERENCE DRAWN OR DECISION MADE IN CONNECTION WITH THE USE OF THIS RECORDED-DATA.

OTHER SERVICES1
 OS1: FMS/LSS
 OS2: DITE
 OS3: WST
 OS4:
 OS5:

OTHER SERVICES2
 OS1:
 OS2:
 OS3:
 OS4:
 OS5:

REMARKS: RUN NUMBER 1
 Hole cored with APS/XCB, 11 7/16 bit.
 Sea Floor at:2962 mbrf.
 Log measured in meters below rig floor.
 Lamont TAP tool run at bottom of DITE for temperature/pressure data.
 Wireline heave compensator used on all runs.
 Sepiolite mud was used to displace the hole.
 Driller TD= 3246 mbrf.
 Schlumberger TD= 3249 mbrf.
 Drill pipe Schlumberger= 3036mbrf.
 See Lamont TAP tool for bottom hole temperature.

REMARKS: RUN NUMBER 2

RUN 1
 SERVICE ORDER #:
 PROGRAM VERSION: 10C0-306
 FLUID LEVEL:

RUN 2
 SERVICE ORDER #:
 PROGRAM VERSION:
 FLUID LEVEL:

LOGGED INTERVAL	START	STOP



LOGGED INTERVAL	START	STOP


EQUIPMENT DESCRIPTION

RUN 1
SURFACE EQUIPMENT
 SFT-281 24
 SFT-178 4722
 GSR-U 135
 WITM (DTS)-A

RUN 2

DOWNHOLE EQUIPMENT

LEH-QT		37.79
AH-MGT		36.90

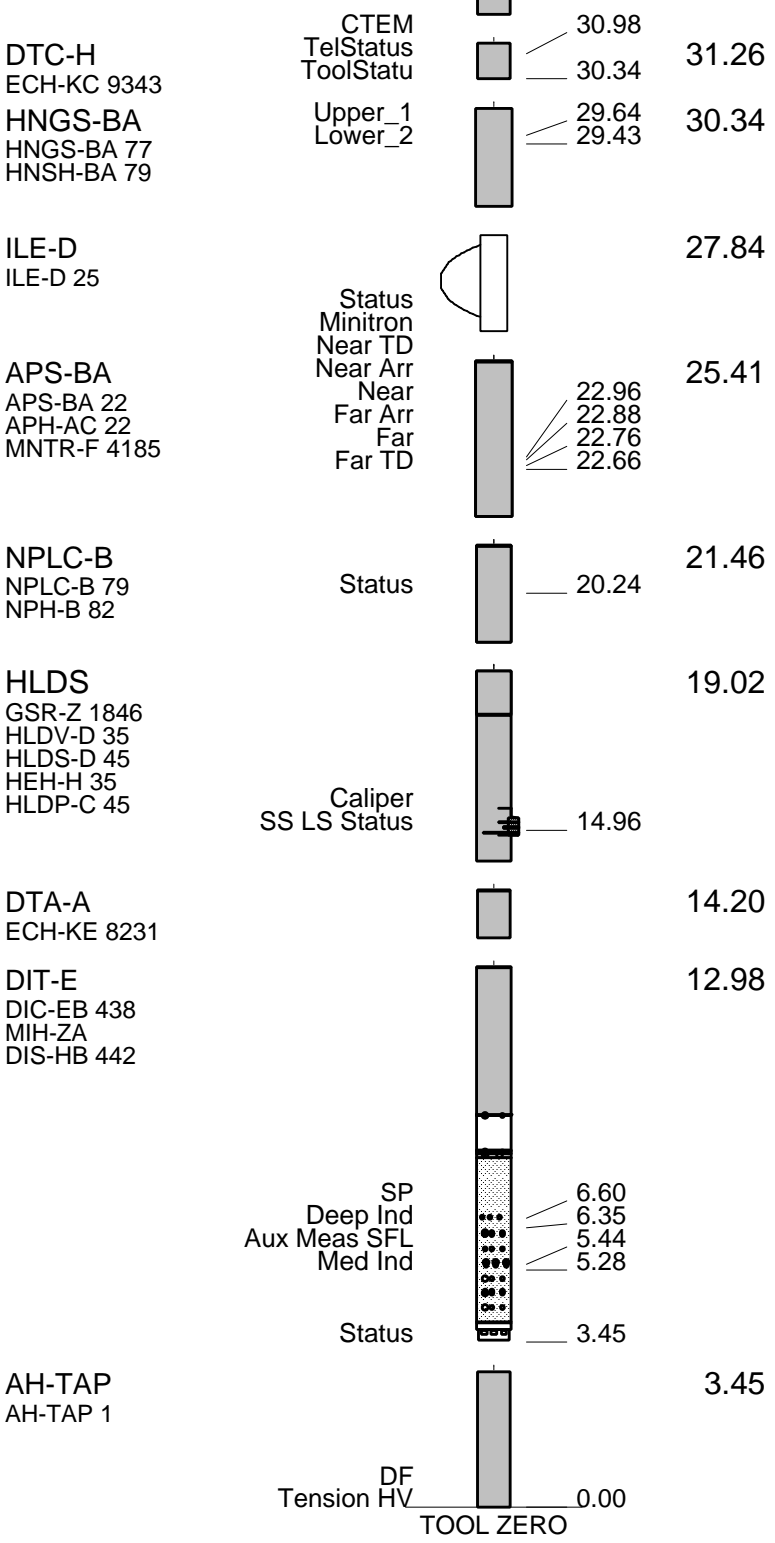

TOOL ZERO

MAXIMUM STRING DIAMETER 3.88 IN
 MEASUREMENTS RELATIVE TO TOOL ZERO
 ALL LENGTHS IN METERS

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_011LUP	FN:13	PRODUCER	18-Jan-2003 18:53	3250.7 M	2941.3 M
REDUCE	PI_LDL_APS_NGS_011LUP	FN:14	PRODUCER	18-Jan-2003 18:53	3250.7 M	2941.3 M



OP System Version: 10C0-306


MCM


DIT-E	10C0-306	DTA-A	10C0-306
HLDS	SPC-2277-NUCL_b	NPLC-B	OP10-KP1
APS-BA	SPC-2277-NUCL_b	HNGS-BA	SPC-2277-NUCL_b
DTC-H	10C0-306		


PIP SUMMARY

Time Mark Every 60 S

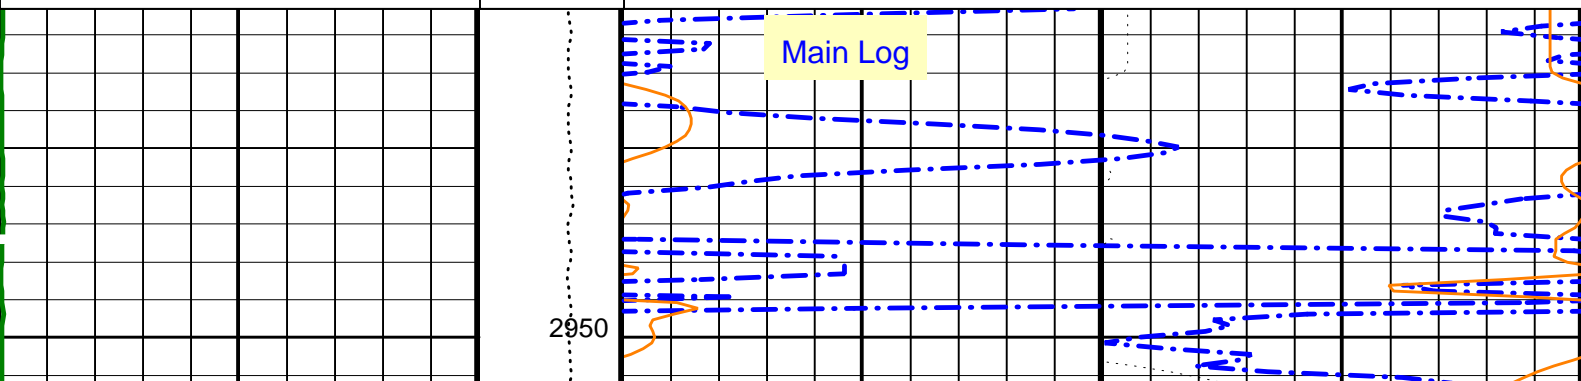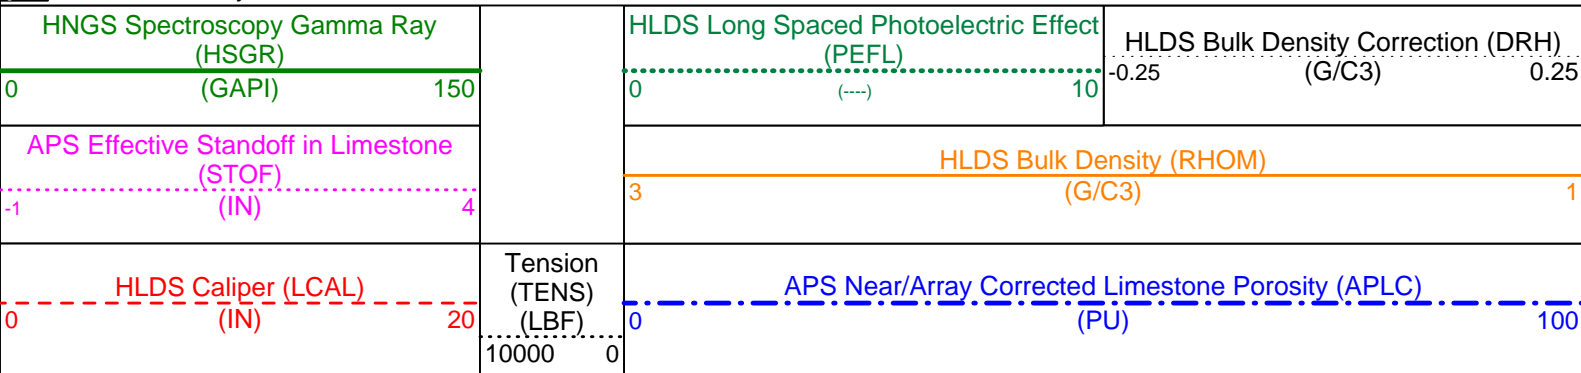

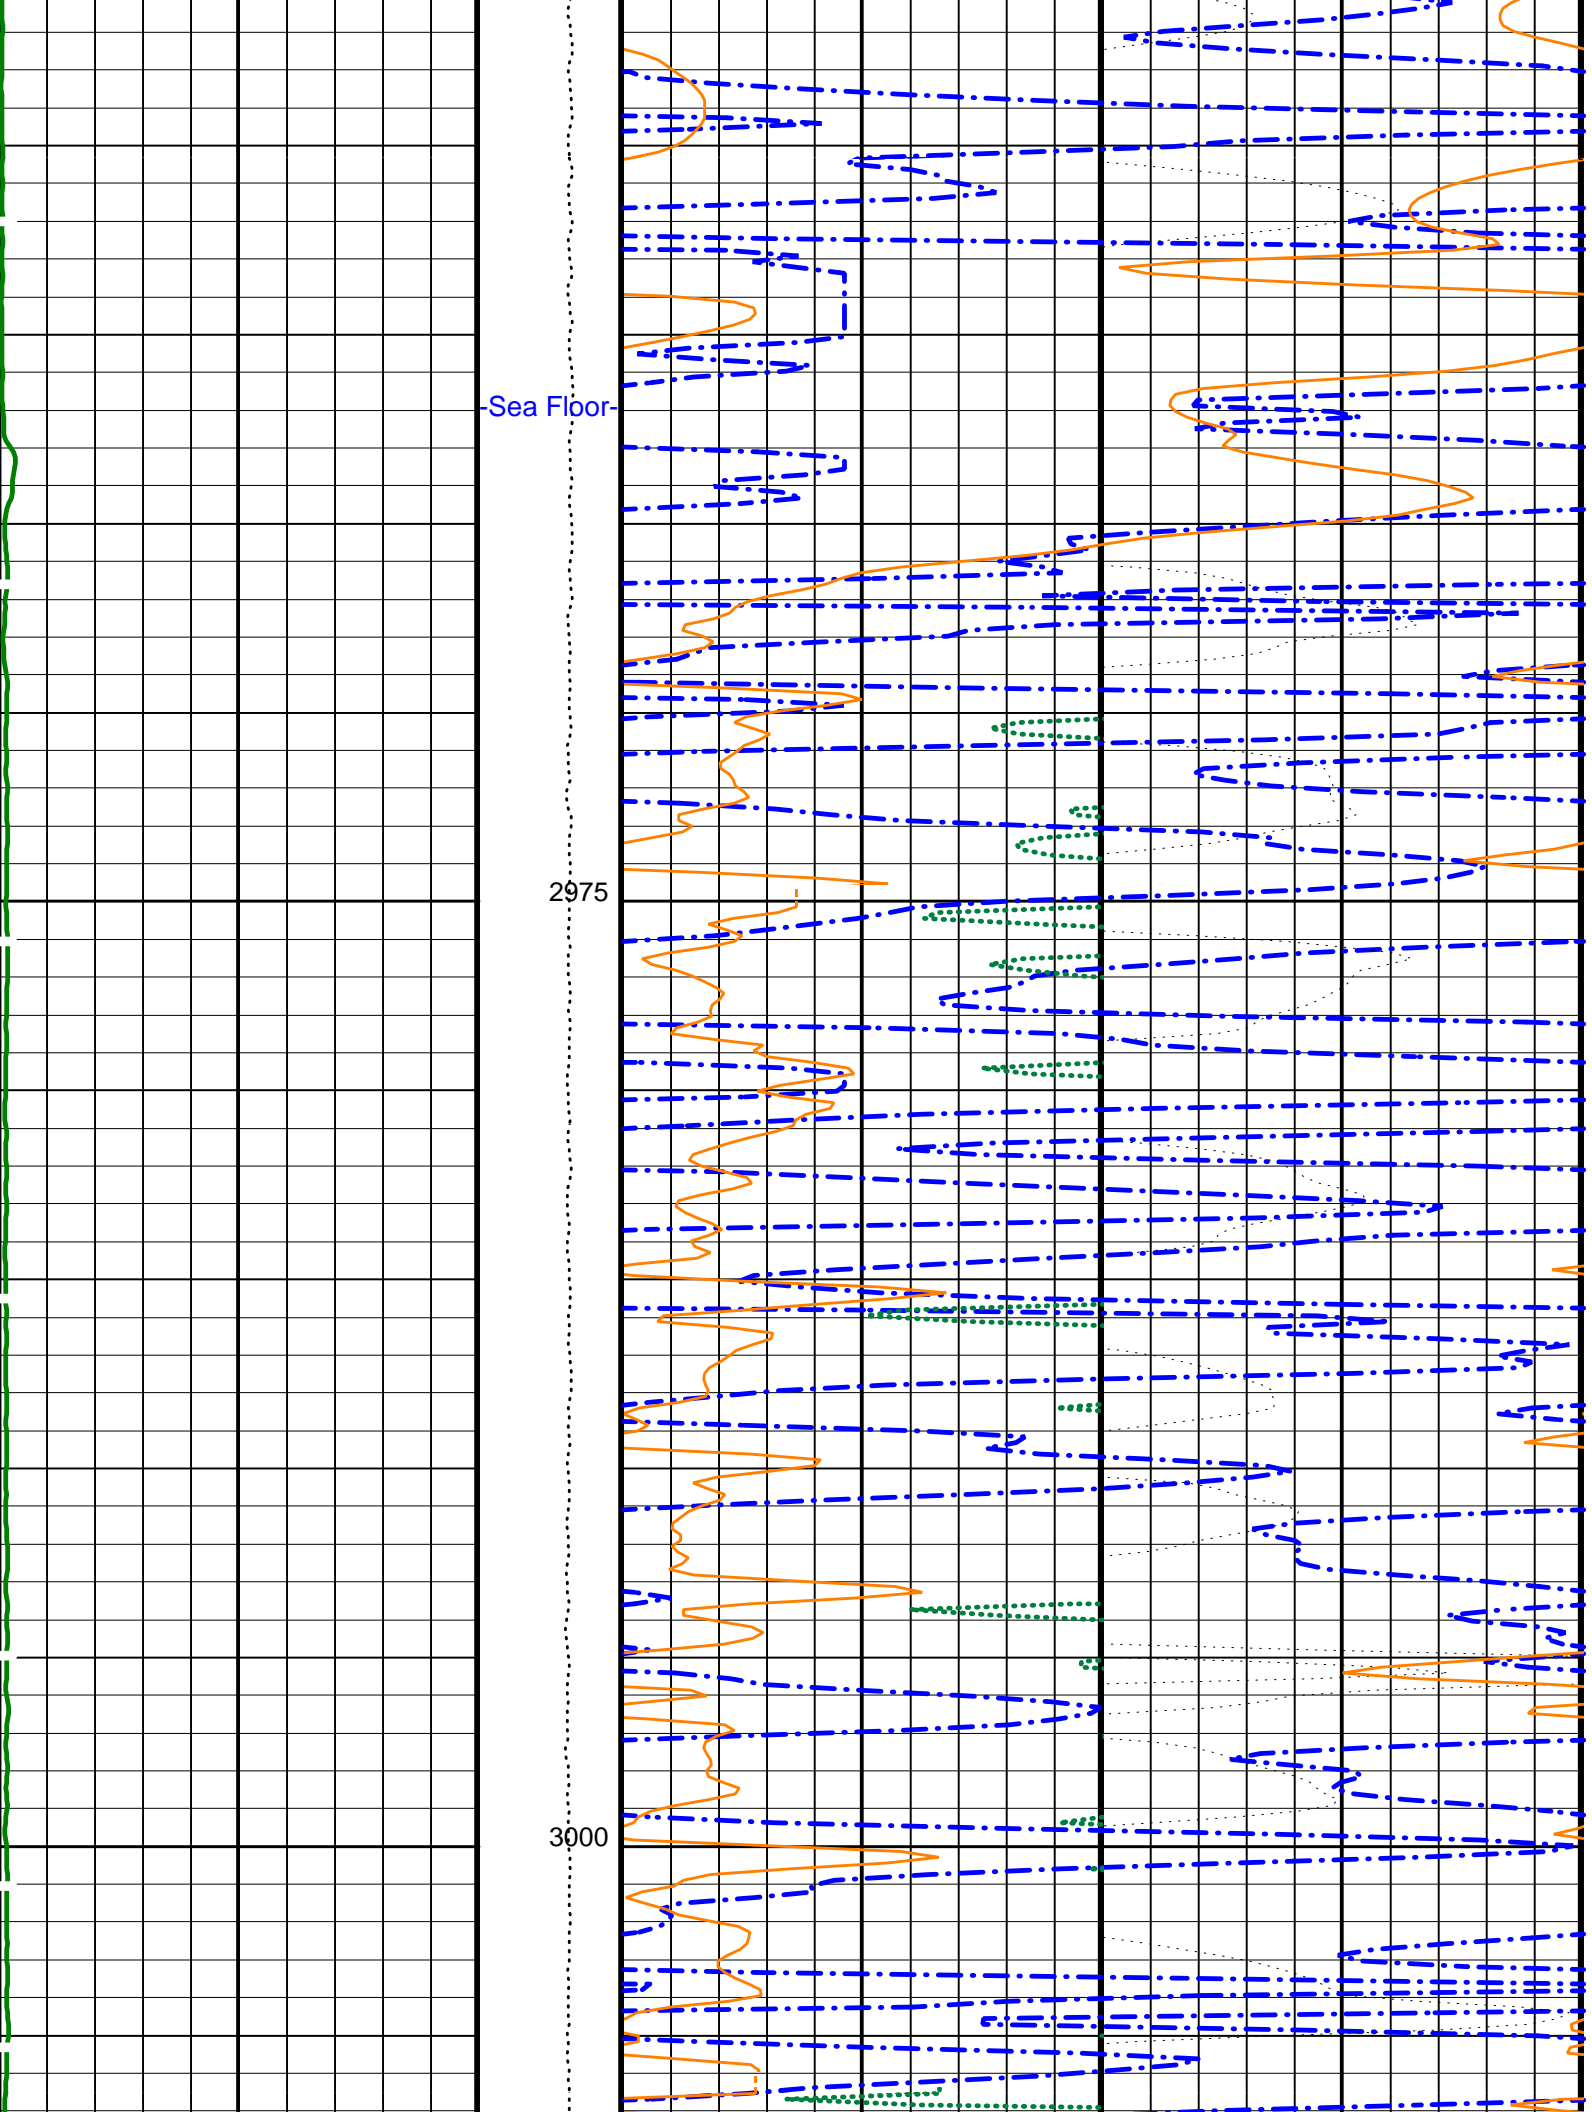


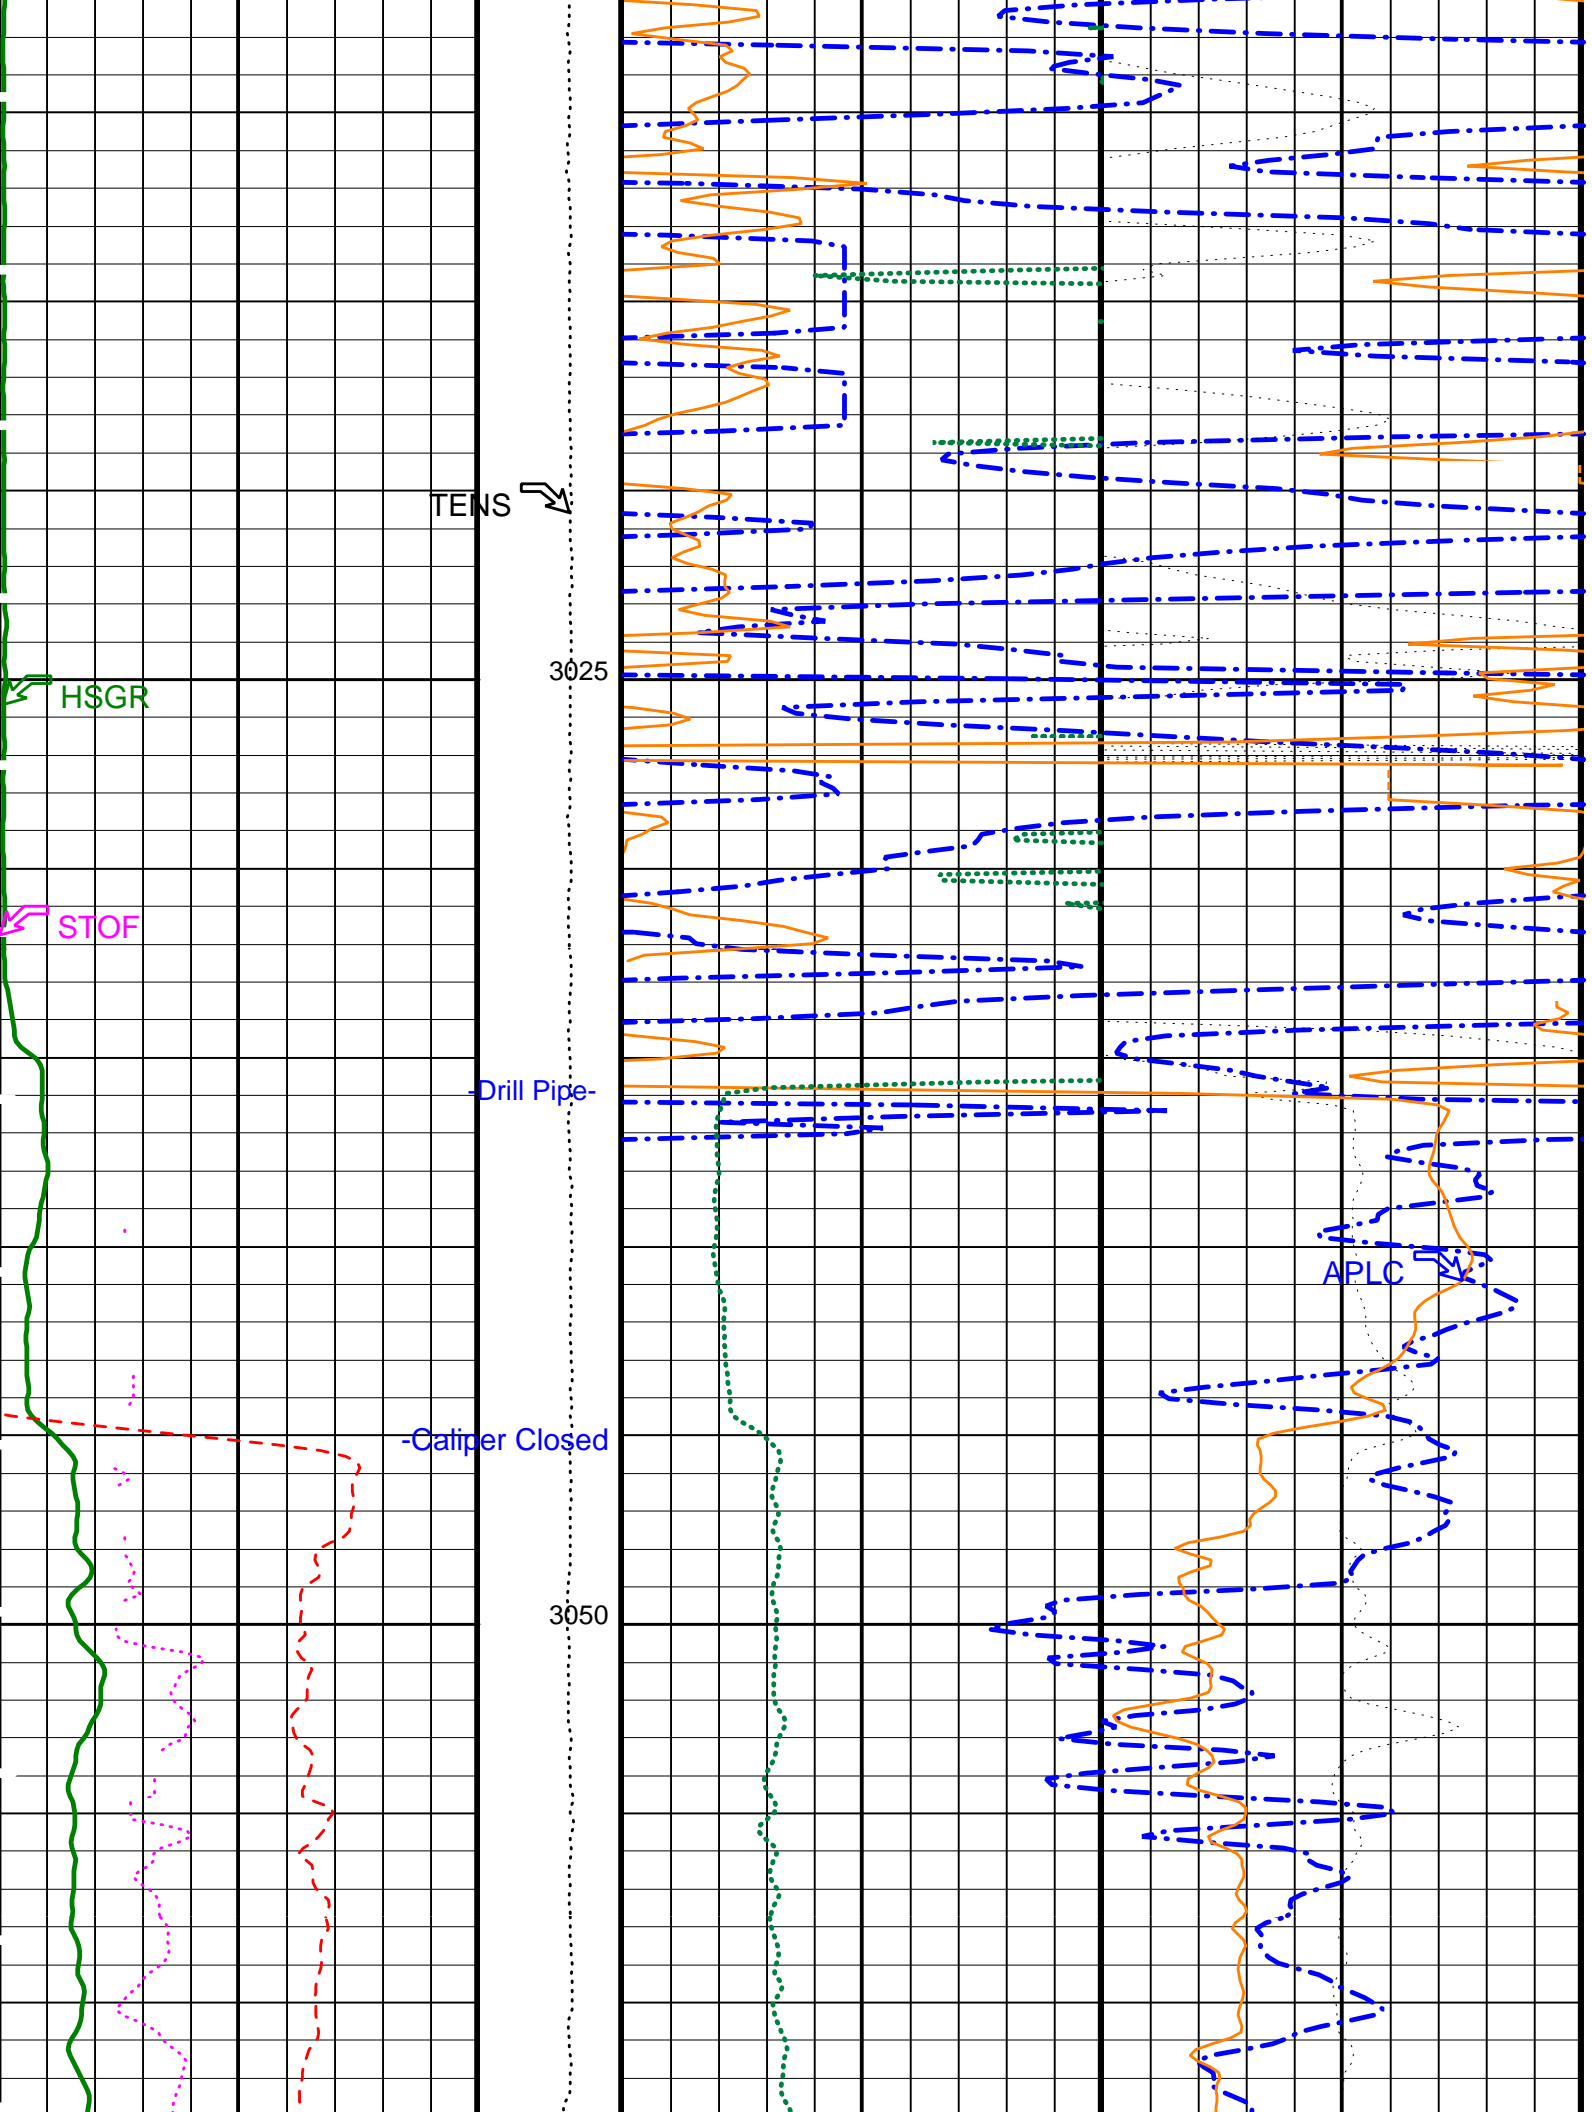


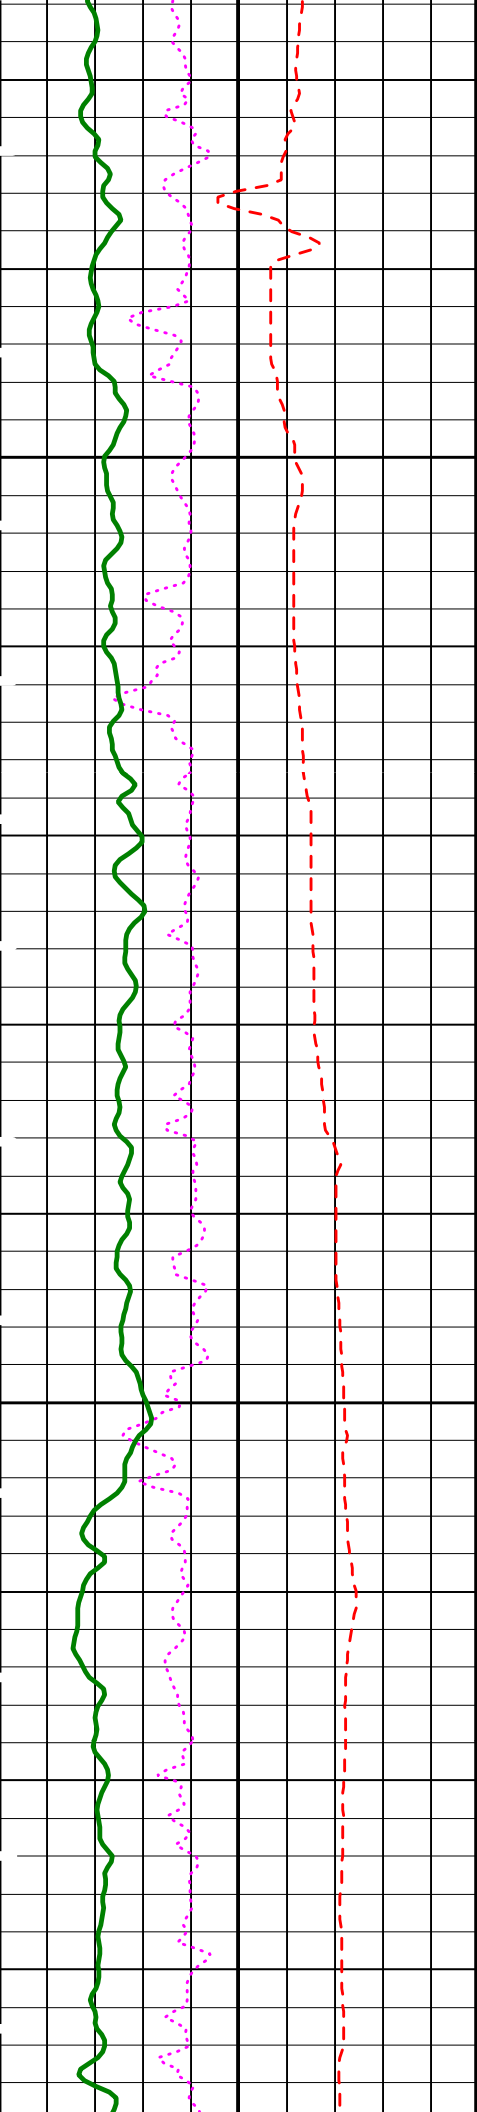

3075

3100

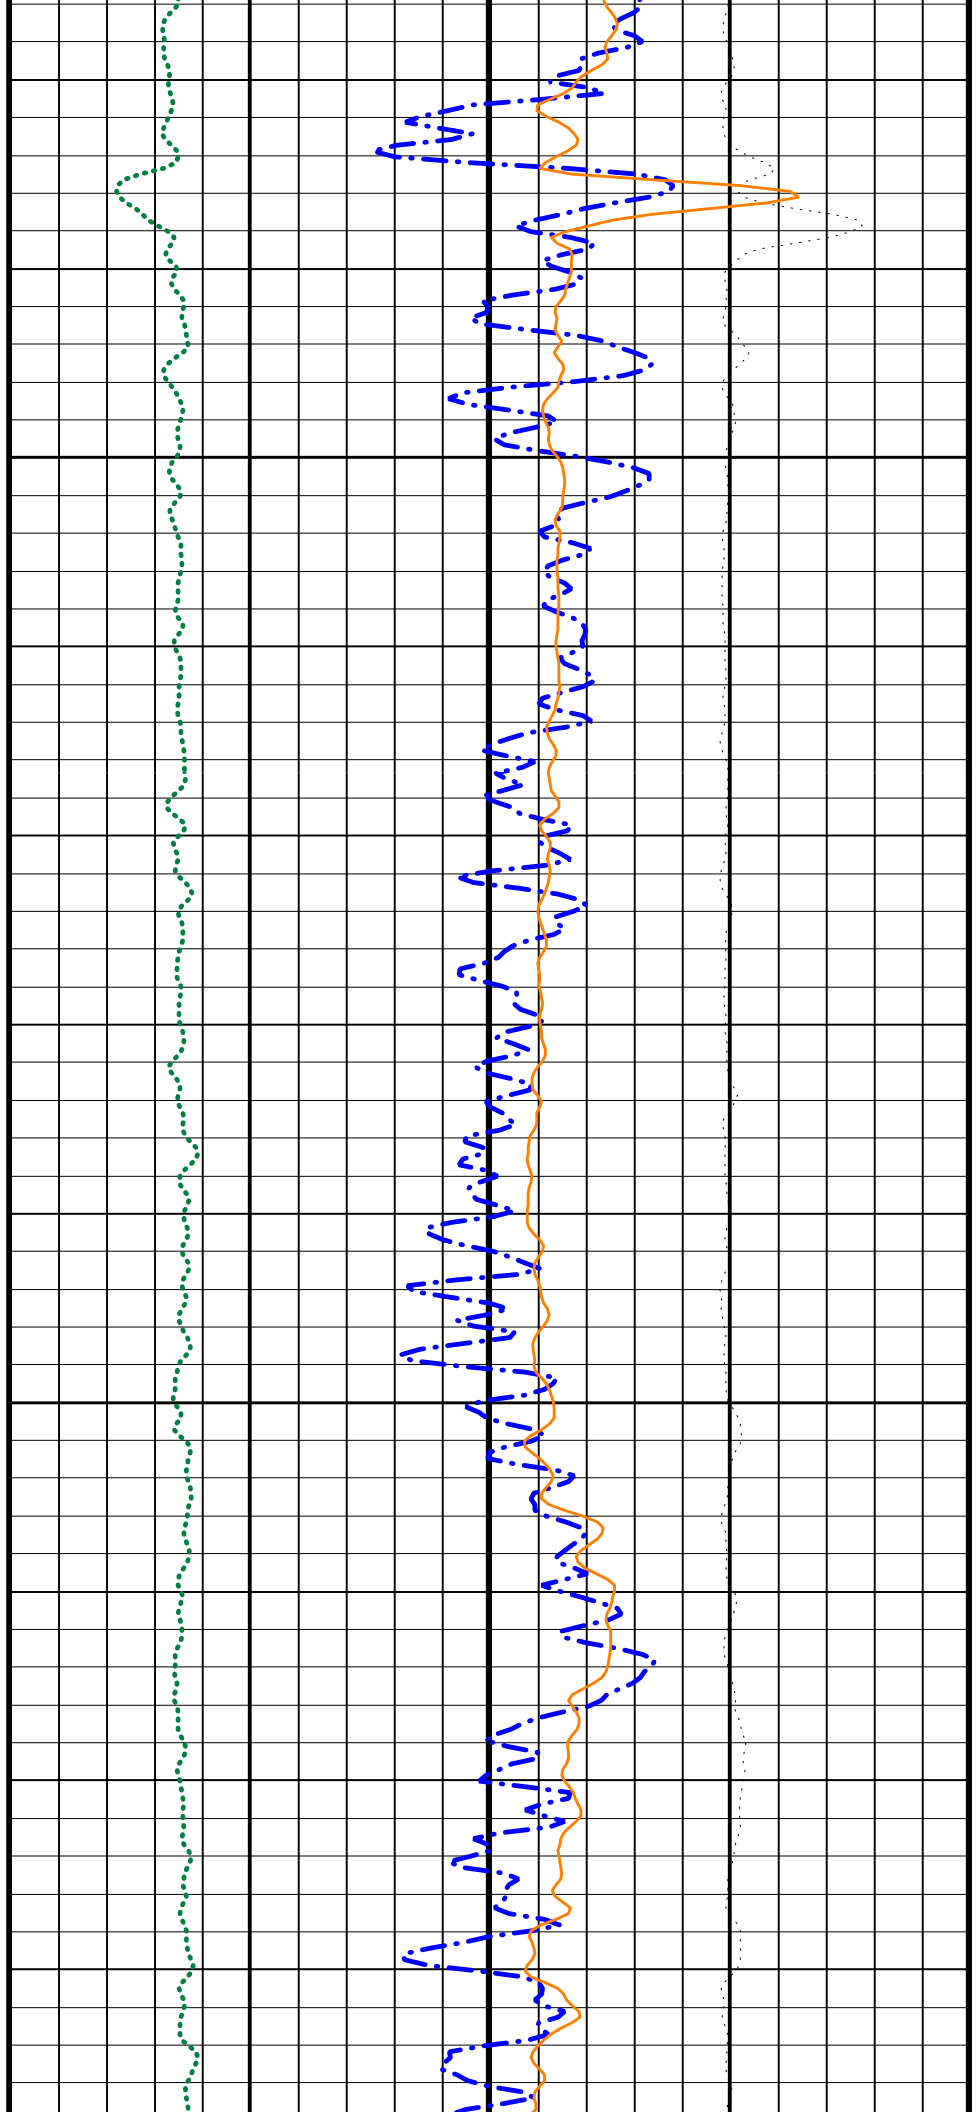


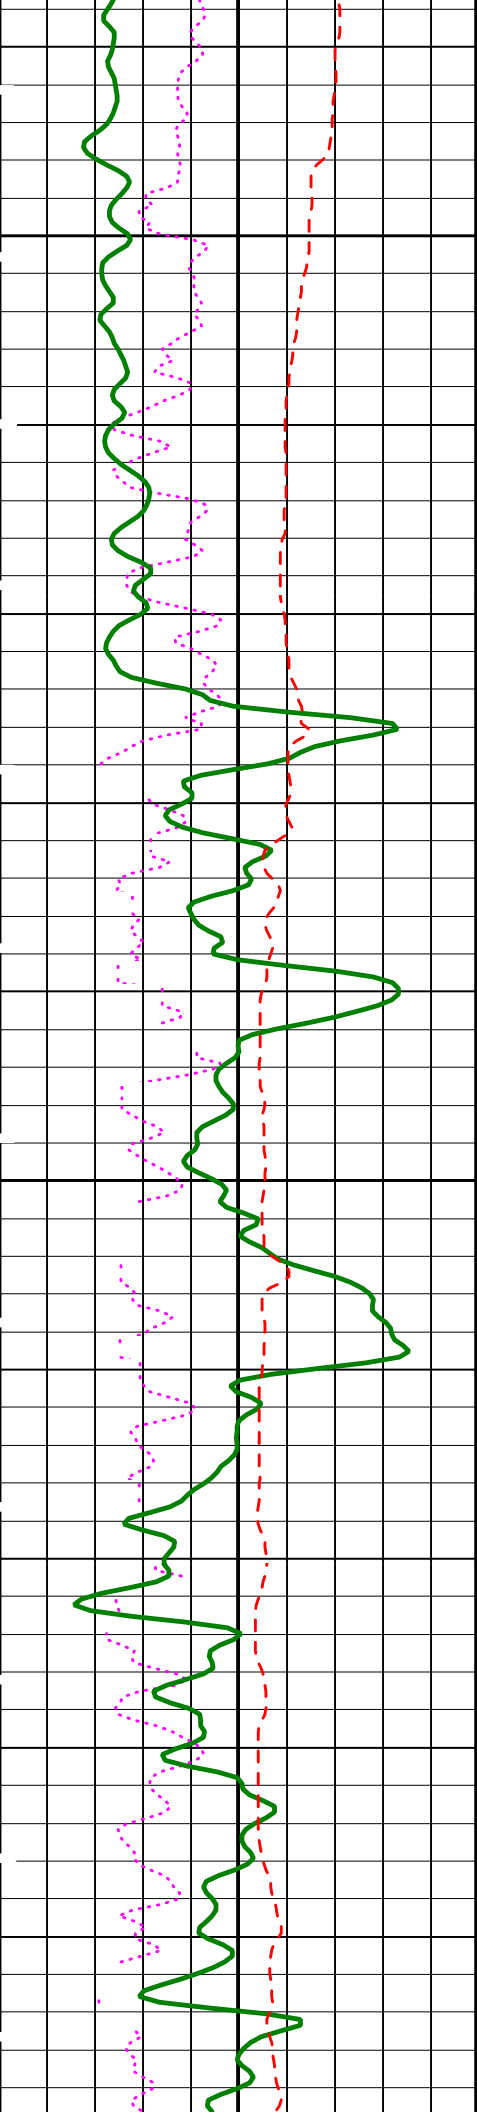



3125

3150

3175

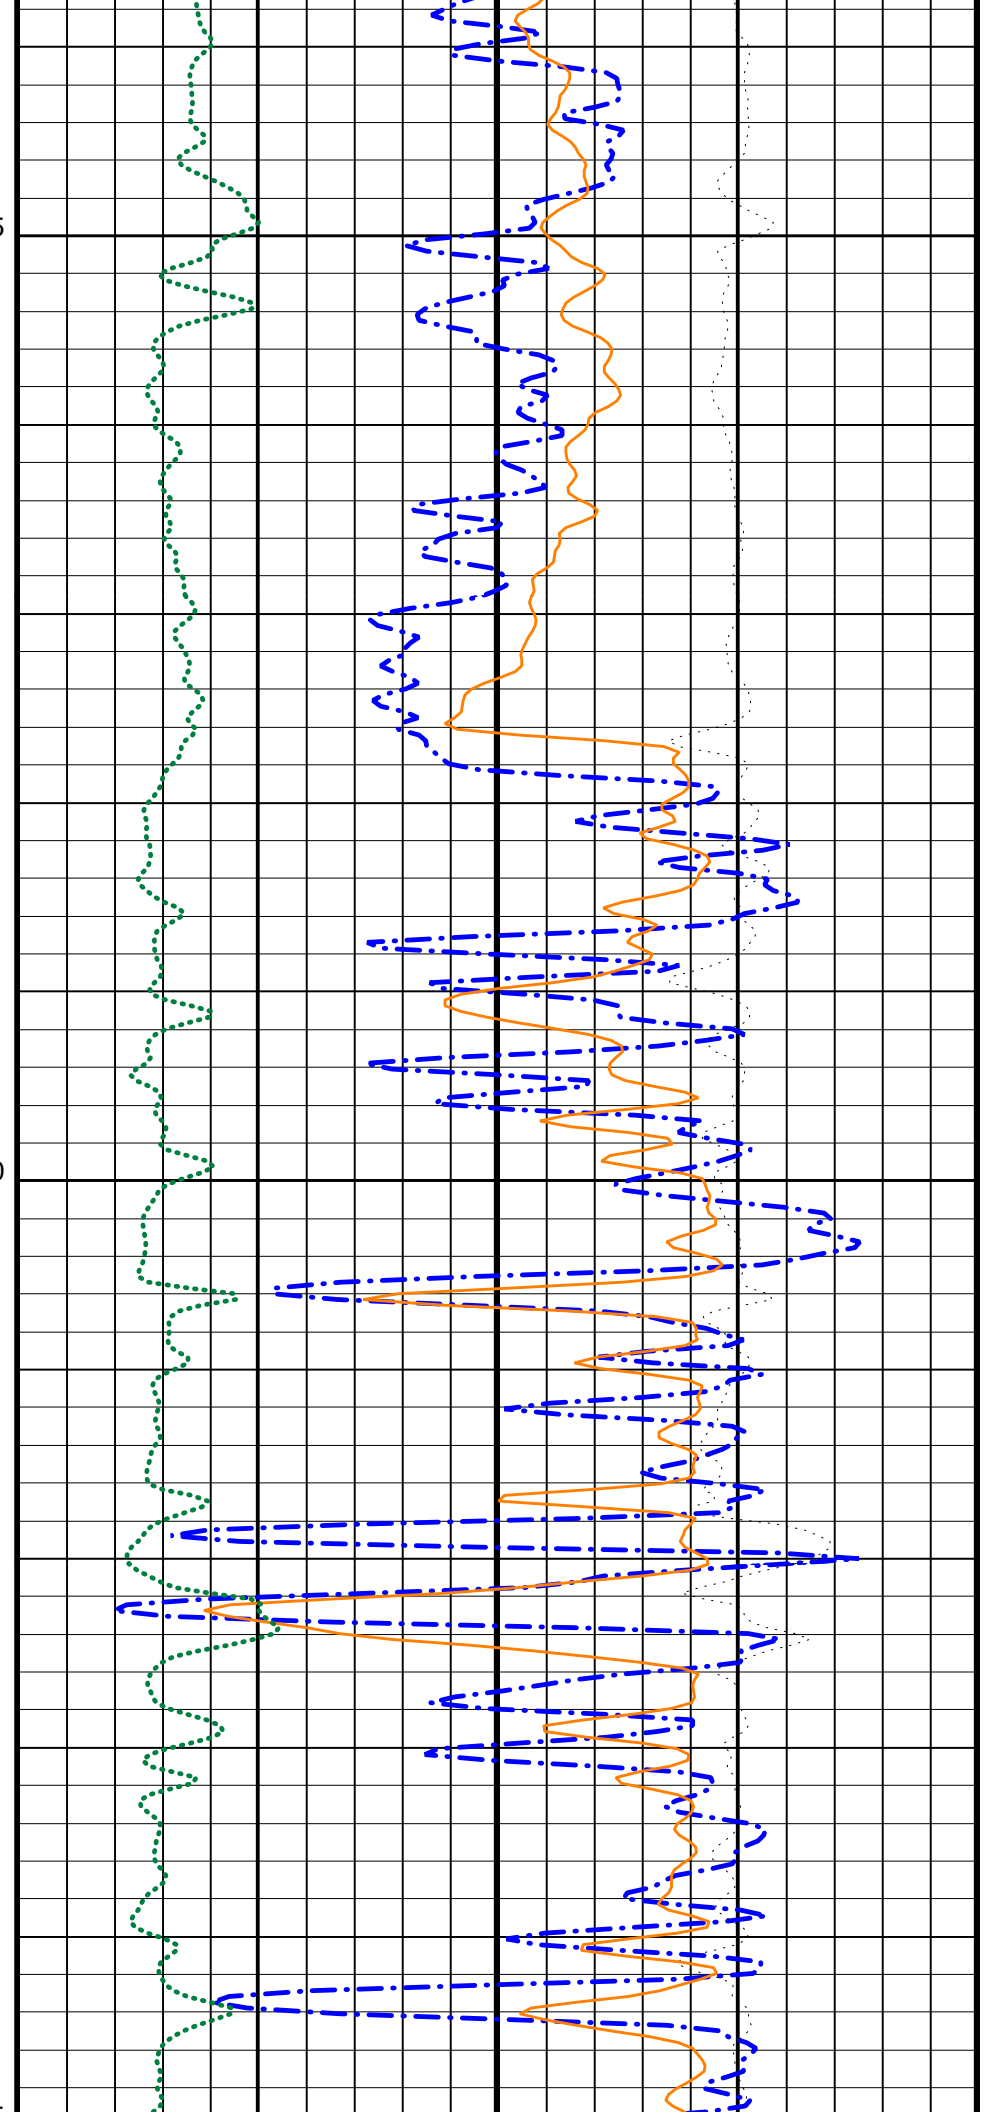

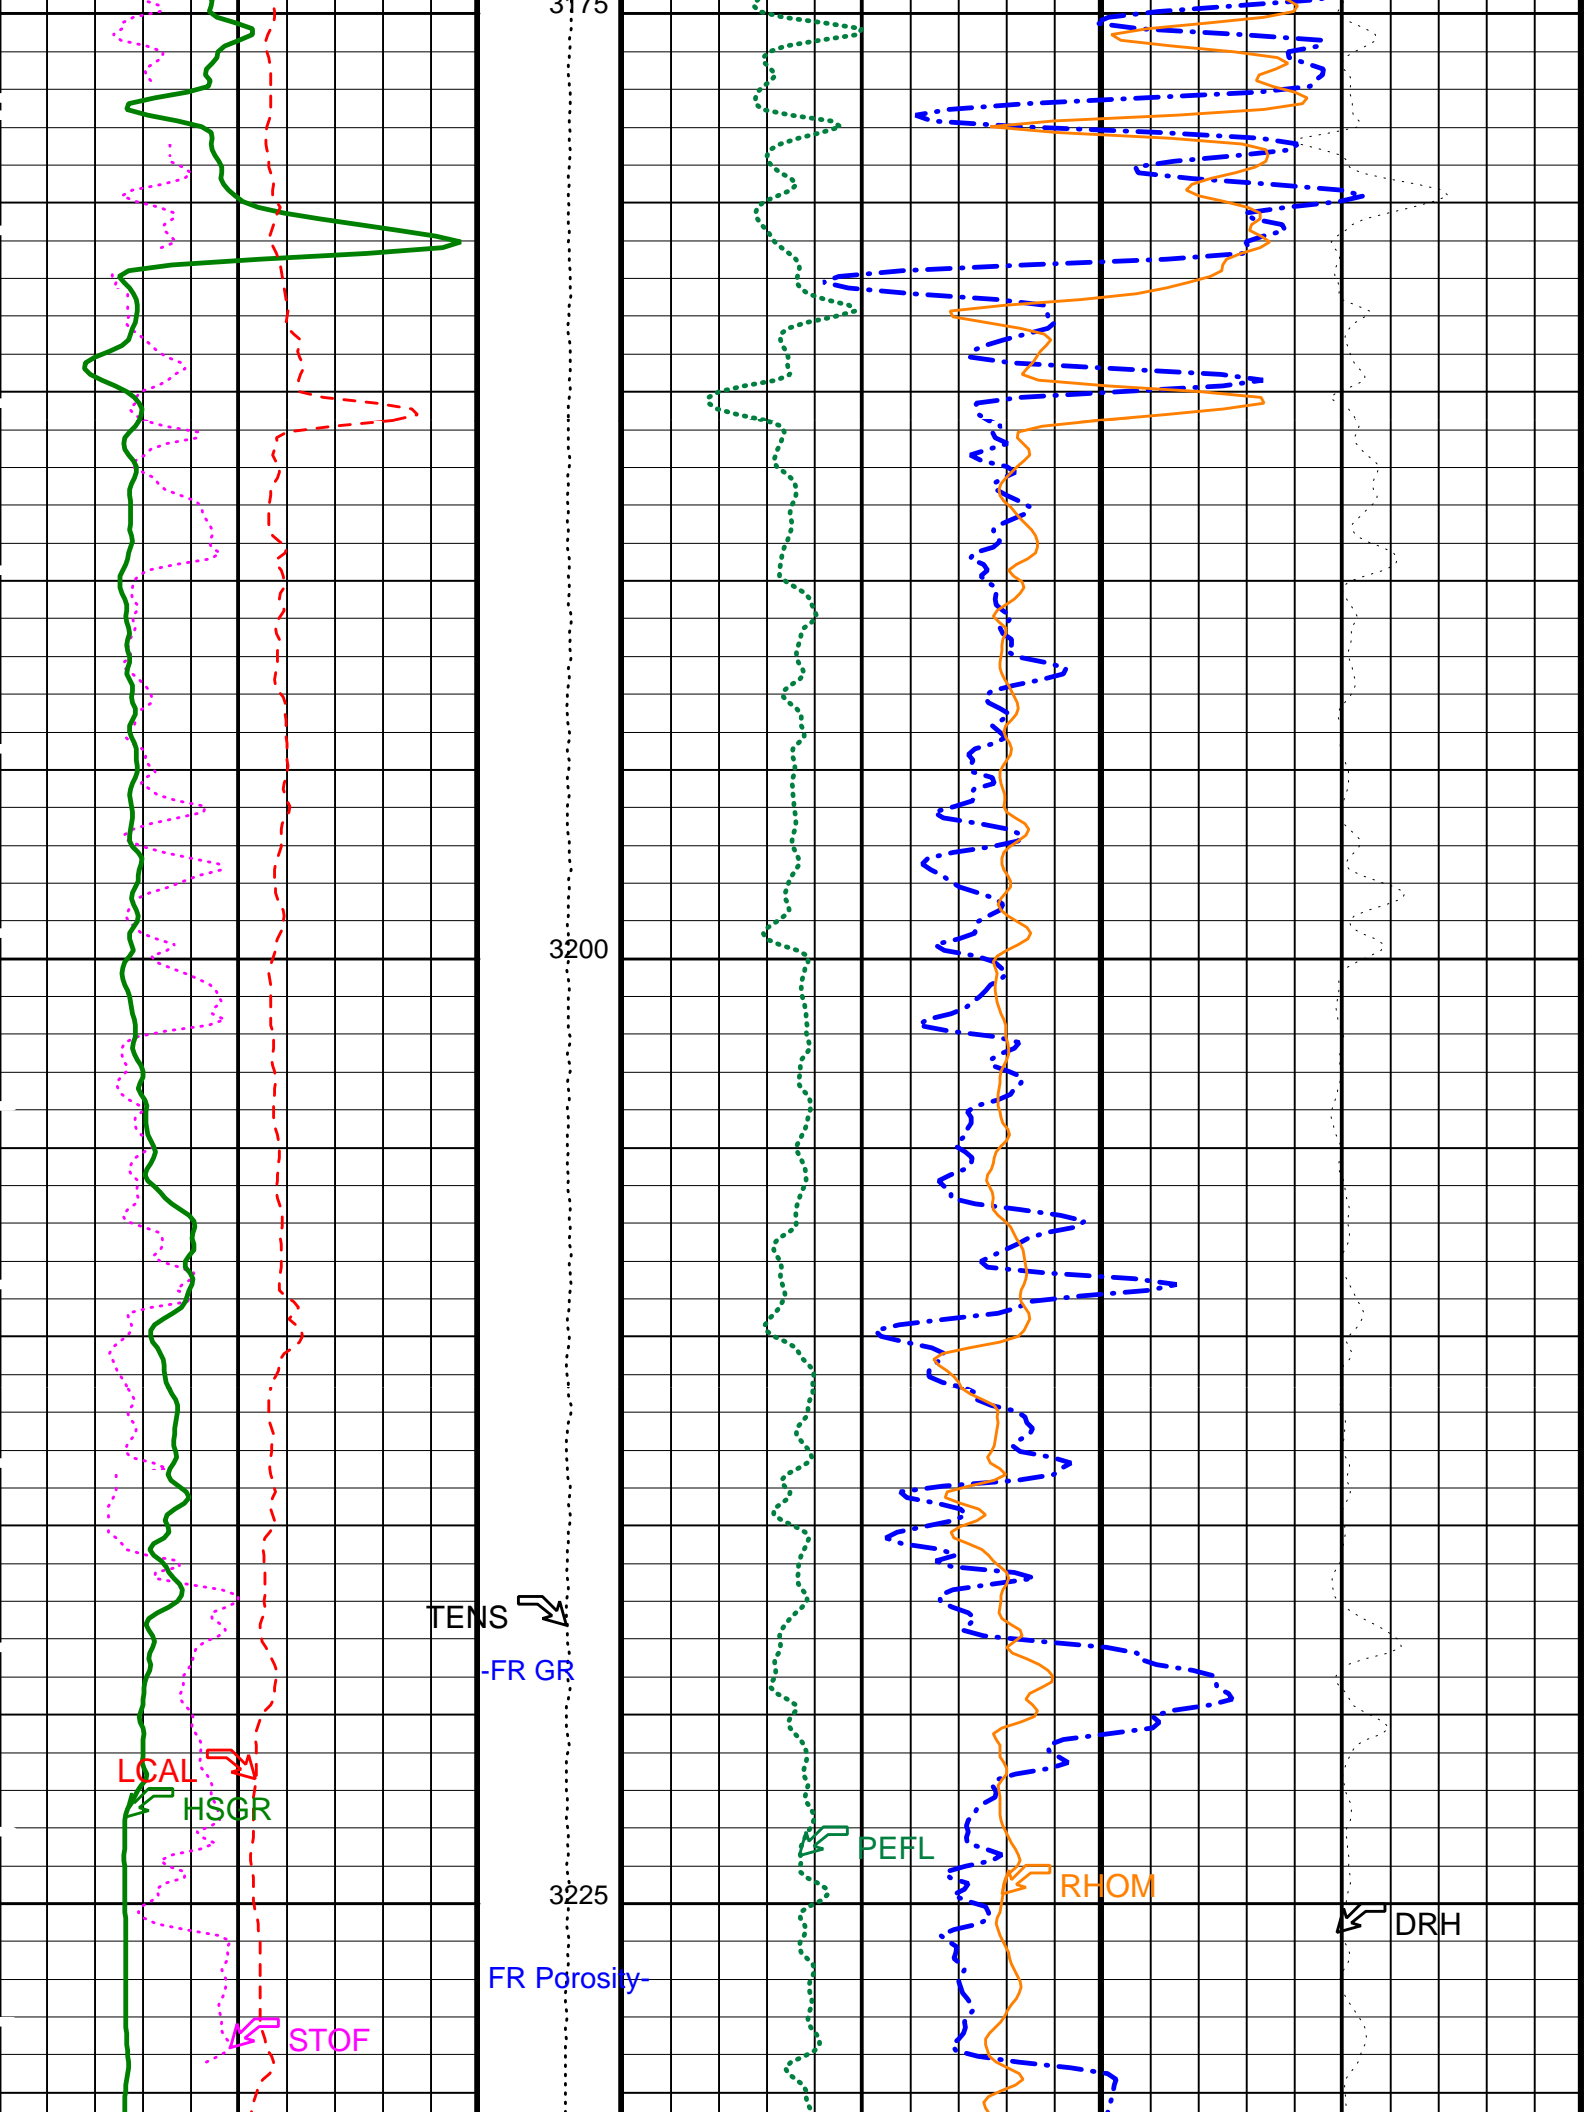

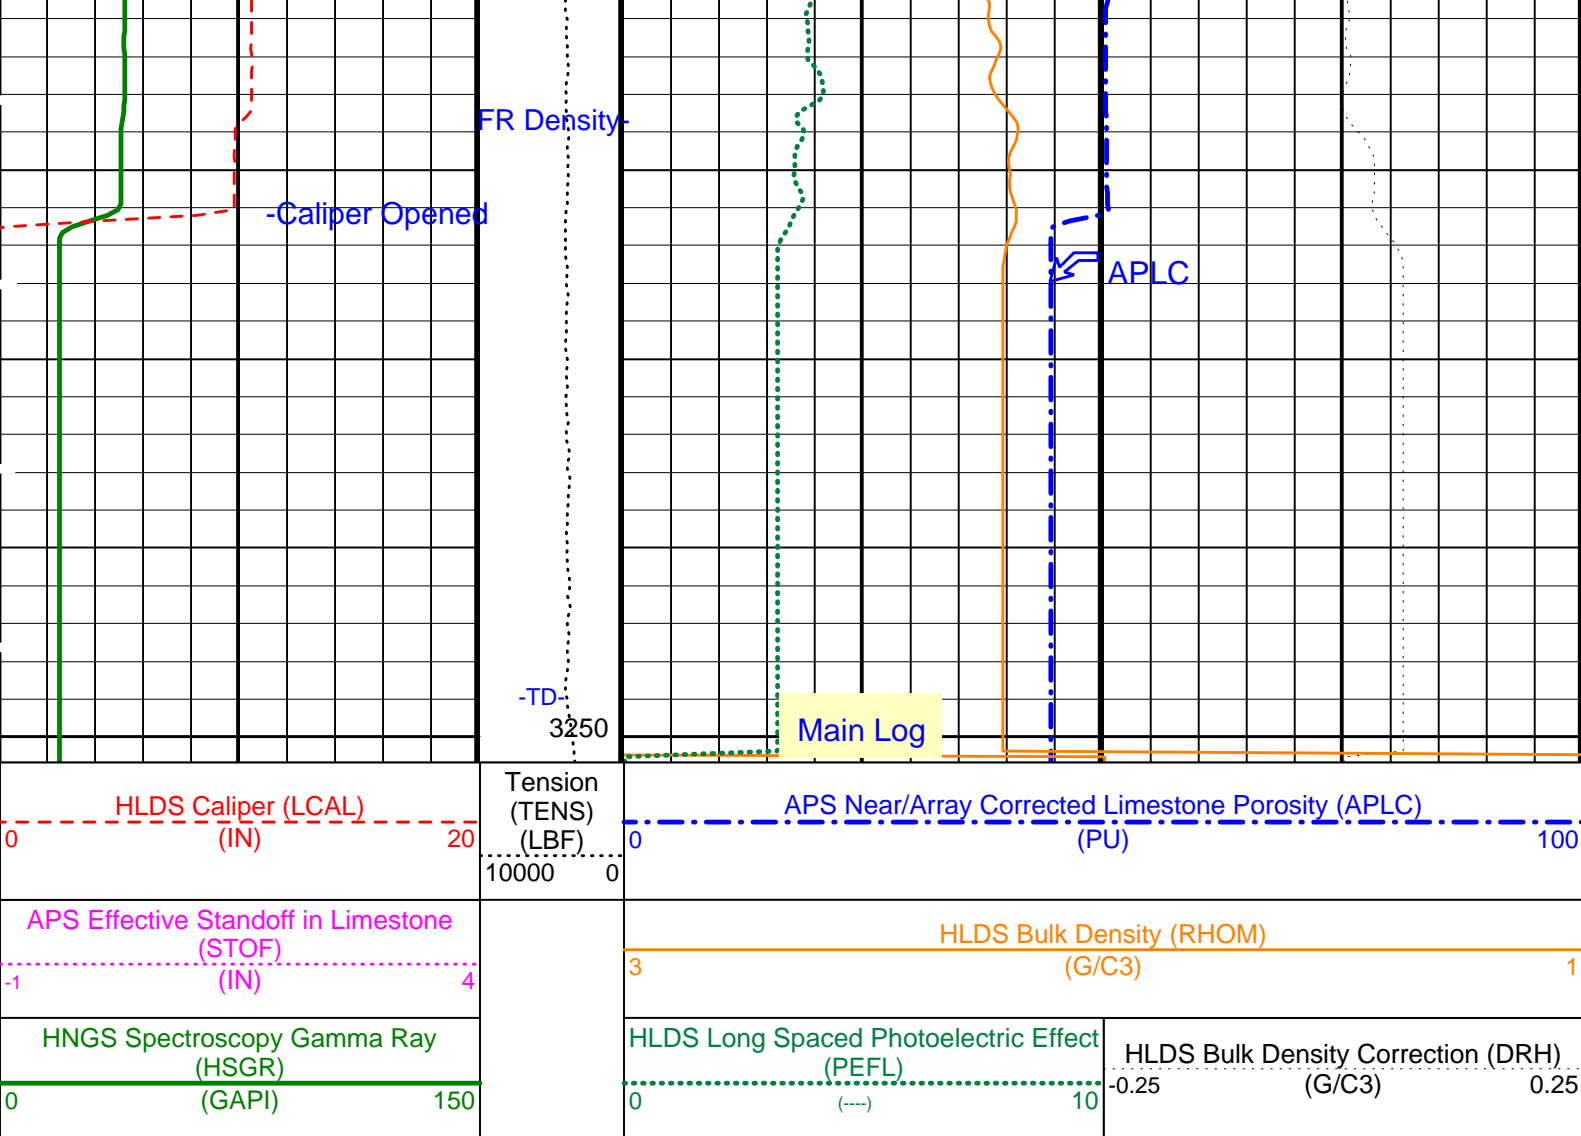

PIP SUMMARY

Time Mark Every 60 S

Parameters

DLIS Name	Description	Value	
DIT-E: Dual Induction - E			
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
DGF2	Deep 20 kHz Gain Factor	1.00789	
DPH2	Deep 20 kHz Phase Shift	-0.152394	DEG
DRE2	Deep Real 20 kHz Sonde Error Correction	16.357	MM/M
DSR2	Deep Sigma Reference (20 kHz)	1843	MM/M
DXE2	Deep Quad 20 kHz Sonde Error Correction	64.6326	MM/M
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
IFRS	DIT-E Induction Frequency Selector	20	
IPHA	DIT-E Phasor Processing Mode	ALL	
IPRO	DIT-E Induction Processing Selector	PHASOR	
ITEN	DIT-E Temperature Enable	ENABLE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
MGF2	Medium 20 kHz Gain Factor	1.02964	
MPH2	Medium 20 kHz Phase Shift	-0.933067	DEG
MRE2	Medium Real 20 kHz Sonde Error Correction	-1.78642	MM/M
MSR2	Medium Sigma Reference (20 kHz)	3250	MM/M
MXE2	Medium Quad 20 kHz Sonde Error Correction	-34.2041	MM/M
SBR	Shoulder Bed Resistivity Factor	1	OHMM
SFCR	SFL Channel Ratio	1000	
SFLE	SFL Enable	ENABLE	
SHT	Surface Hole Temperature	20	DEGC
SPAE	DIT-E SPARC Processing Enable	ENABLE	
SPNV	SP Next Value	0	MV
HLDS: Hostile Litho-Density Sonde			

CLCL	HLDS LS Control Loop Controller Mode	AUTO_DEFAULT	
CLCS	HLDS SS Control Loop Controller Mode	AUTO	
CLLS	HLDS Mode Loop Long Spacing	AUTO	
CLSS	HLDS Mode Loop Short Spacing	AUTO	
DHC	Density Hole Correction	BS	
DPPM	Density Porosity Processing Mode	HIRS	
FD	Fluid Density	1	G/C3
LATC	HLDS Activation Correction	ON	
LLDL	HLDS LS Low Level Discriminator DAC	14000	
LLDS	HLDS SS Low Level Discriminator DAC	14000	
LLML	HLDS LS Low Level Discriminator Mode	AUTO	
LLMS	HLDS SS Low Level Discriminator Mode	AUTO	
MDEN	Matrix Density	2.71	G/C3
PHVL	HLDS Long Spacing High Voltage Setting	1000	V
PHVS	HLDS Short Spacing High Voltage Setting	1000	V
PSDL	HLDS LS Pulse Shape Compensation DAC	16000	
PSDS	HLDS SS Pulse Shape Compensation DAC	16000	
PSML	HLDS LS Pulse Shape Compensation Mode	AUTO	
PSMS	HLDS SS Pulse Shape Compensation Mode	AUTO	
NPLC-B: Nuclear Porosity Lithology Cartridge - B			
NOTS	NPLC Old Temperature Sensor	NO	
APS-BA: Accelerator-Porosity Tool			
	APS Software Version	5	
AASD	APS Thermal and Array Detectors High Voltage Setting	1958.44	V
ADSO	APS Array Detectors Data Source Switch	Both	
AFSD	APS Far Detector High Voltage Setting	2072.71	V
AHCS	APS Holesize Correction Source	GCSE	
AHSS	APS Holesize Correction Switch	ON	
AMTY	APS Environmental Corrections Mud Type	WaterBaseBarite	
ANSD	APS Near Detector High Voltage Setting	1727.99	V
AOTS	APS Old Temperature Sensor Switch	NO	
ASOS	APS Standoff Correction Switch	ON	
ATSS	APS Temperature-Pressure-Salinity Correction Switch	OFF	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
DPPM	Density Porosity Processing Mode	HIRS	
FSAL	Formation Salinity	-50000	PPM
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
NARC	APS Near/Array Calibration Ratio	1.05147	
NFRC	APS Near/Far Calibration Ratio	0.886931	
SHT	Surface Hole Temperature	20	DEGC
HNGS-BA: Hostile Natural Gamma Ray Sonde			
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.000331568	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	NATU	
HNPE	HNGS Processing Enable	YES	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	-999.25	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	-999.25	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	ECCE	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.734507	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.776573	

System and Miscellaneous

ALDTPCHAN	Name of alternate depth channel	SpeedCorrectedDepth	
BS	Bit Size	11.438	IN
BSAL	Borehole Salinity	-50000.00	PPM
CSIZ	Current Casing Size	0.000	IN
CWEI	Casing Weight	0.00	LB/F
DFD	Drilling Fluid Density	1.10	G/C3
MST	Mud Sample Temperature	32.00	DEGC

PBVSADP	Use alternate depth channel for playback	NO	
RMFS	Resistivity of Mud Filtrate Sample	-50000.0000	OHMM
RW	Resistivity of Connate Water	1.0000	OHMM
TD	Total Depth	-50000	M
TDD	Total Depth - Driller	-50000.00	M
TDL	Total Depth - Logger	-50000.00	M
TWS	Temperature of Connate Water Sample	37.78	DEGC

Format: APSLiquidPorosity_1 Vertical Scale: 1:200 Graphics File Created: 18-Jan-2003 18:53

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	DTA-A	10C0-306
HLDS	SPC-2277-NUCL_b	NPLC-B	OP10-KP1
APS-BA	SPC-2277-NUCL_b	HNGS-BA	SPC-2277-NUCL_b
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_011LUP	FN:13	PRODUCER	18-Jan-2003 18:53
REDUCE	PI_LDL_APS_NGS_011LUP	FN:14	PRODUCER	18-Jan-2003 18:53

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_012LUP	FN:15	PRODUCER	18-Jan-2003 20:20	3248.4 M	3023.3 M
REDUCE	PI_LDL_APS_NGS_012LUP	FN:16	PRODUCER	18-Jan-2003 20:20	3248.4 M	3023.3 M


OP System Version: 10C0-306


MCM

DIT-E	10C0-306	DTA-A	10C0-306
HLDS	SPC-2277-NUCL_b	NPLC-B	OP10-KP1
APS-BA	SPC-2277-NUCL_b	HNGS-BA	SPC-2277-NUCL_b
DTC-H	10C0-306		

PIP SUMMARY


Time Mark Every 60 S		HNGS Spectroscopy Gamma Ray (HSGR) (GAPI) 0 150		HLDS Long Spaced Photoelectric Effect (PEFL) (---) 0 10		HLDS Bulk Density Correction (DRH) (G/C3) -0.25 0.25	
APS Effective Standoff in Limestone (STOF) (IN) -1 4		HLDS Bulk Density (RHOM) (G/C3) 3 1					
HLDS Caliper (LCAL) (IN) 0 20		Tension (TENS) (LBF) 10000 0		APS Near/Array Corrected Limestone Porosity (APLC) (PU) 0 100			


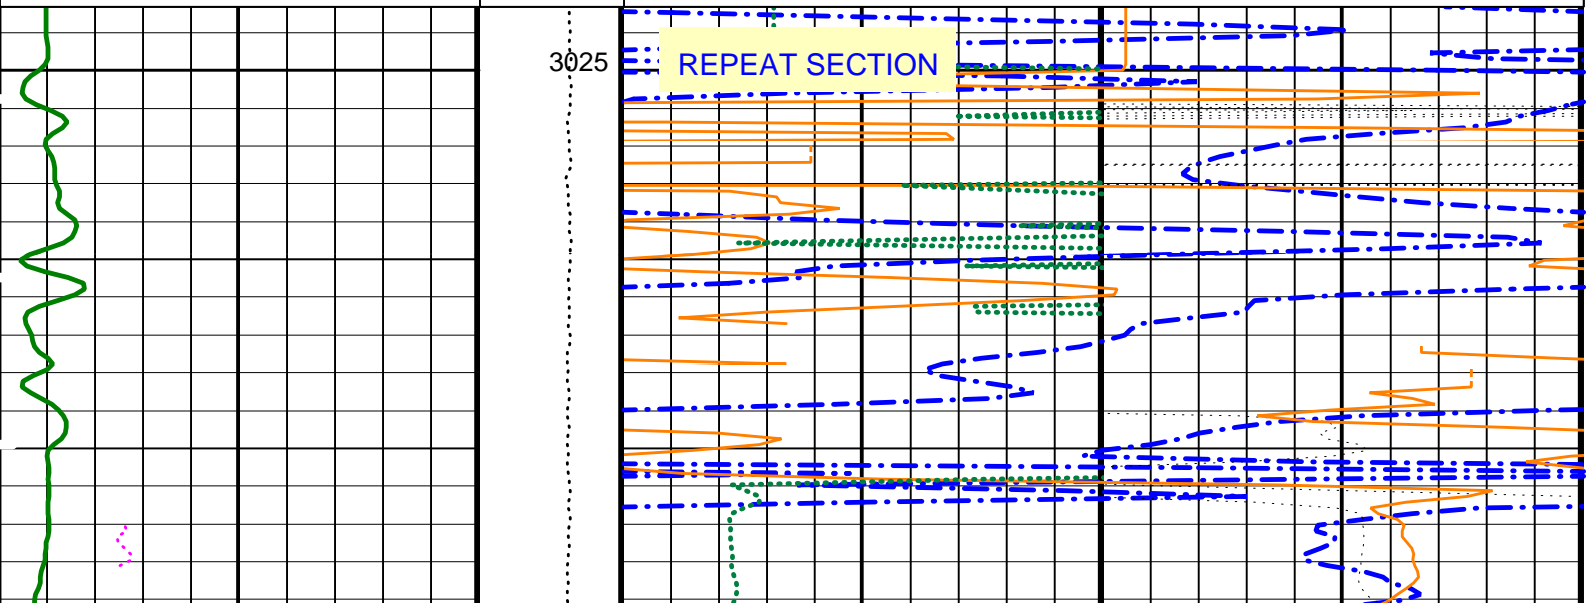



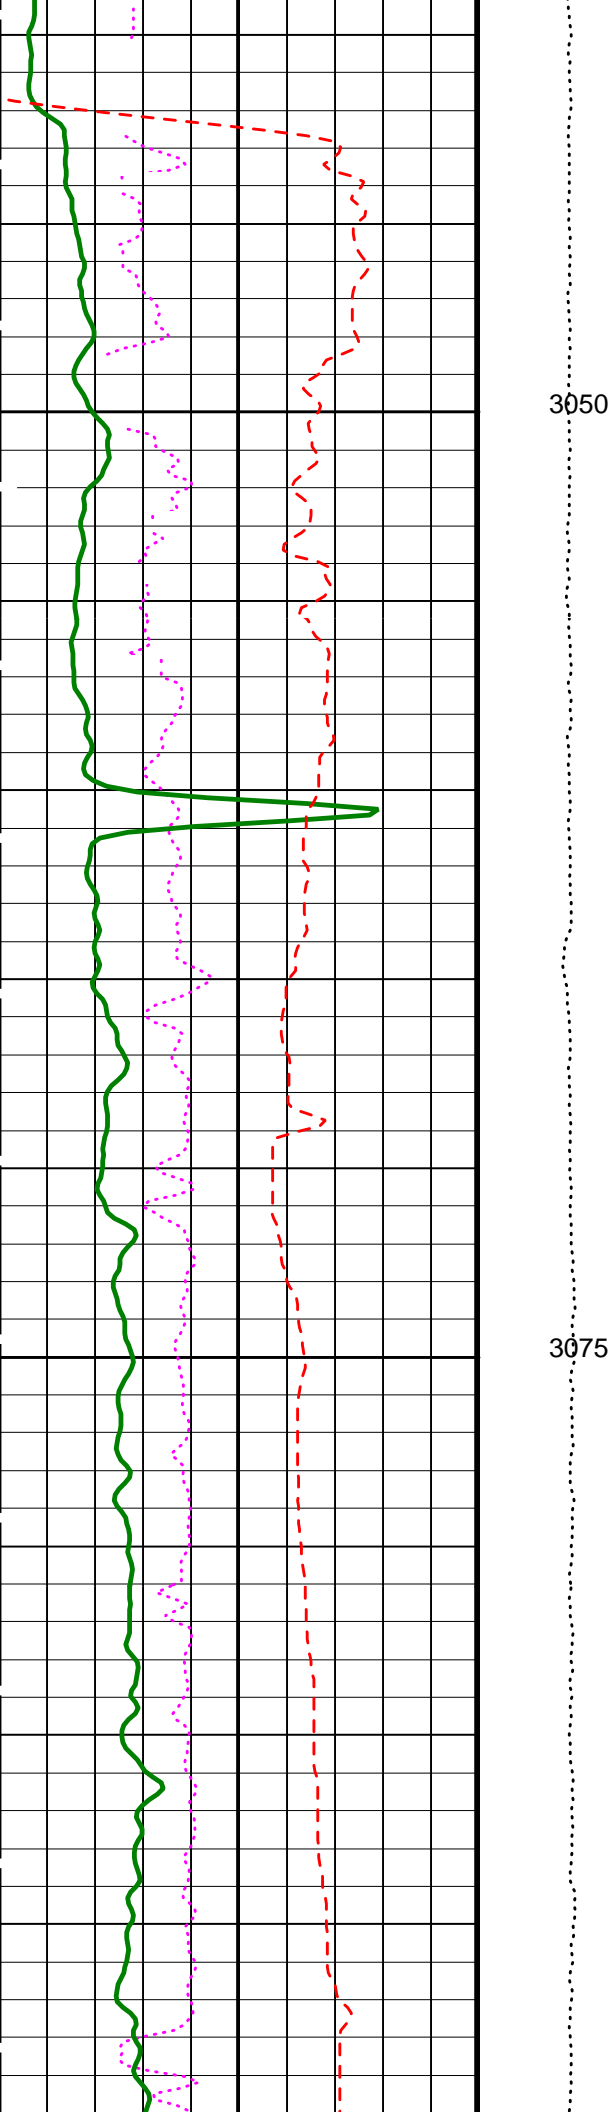



3050

3075

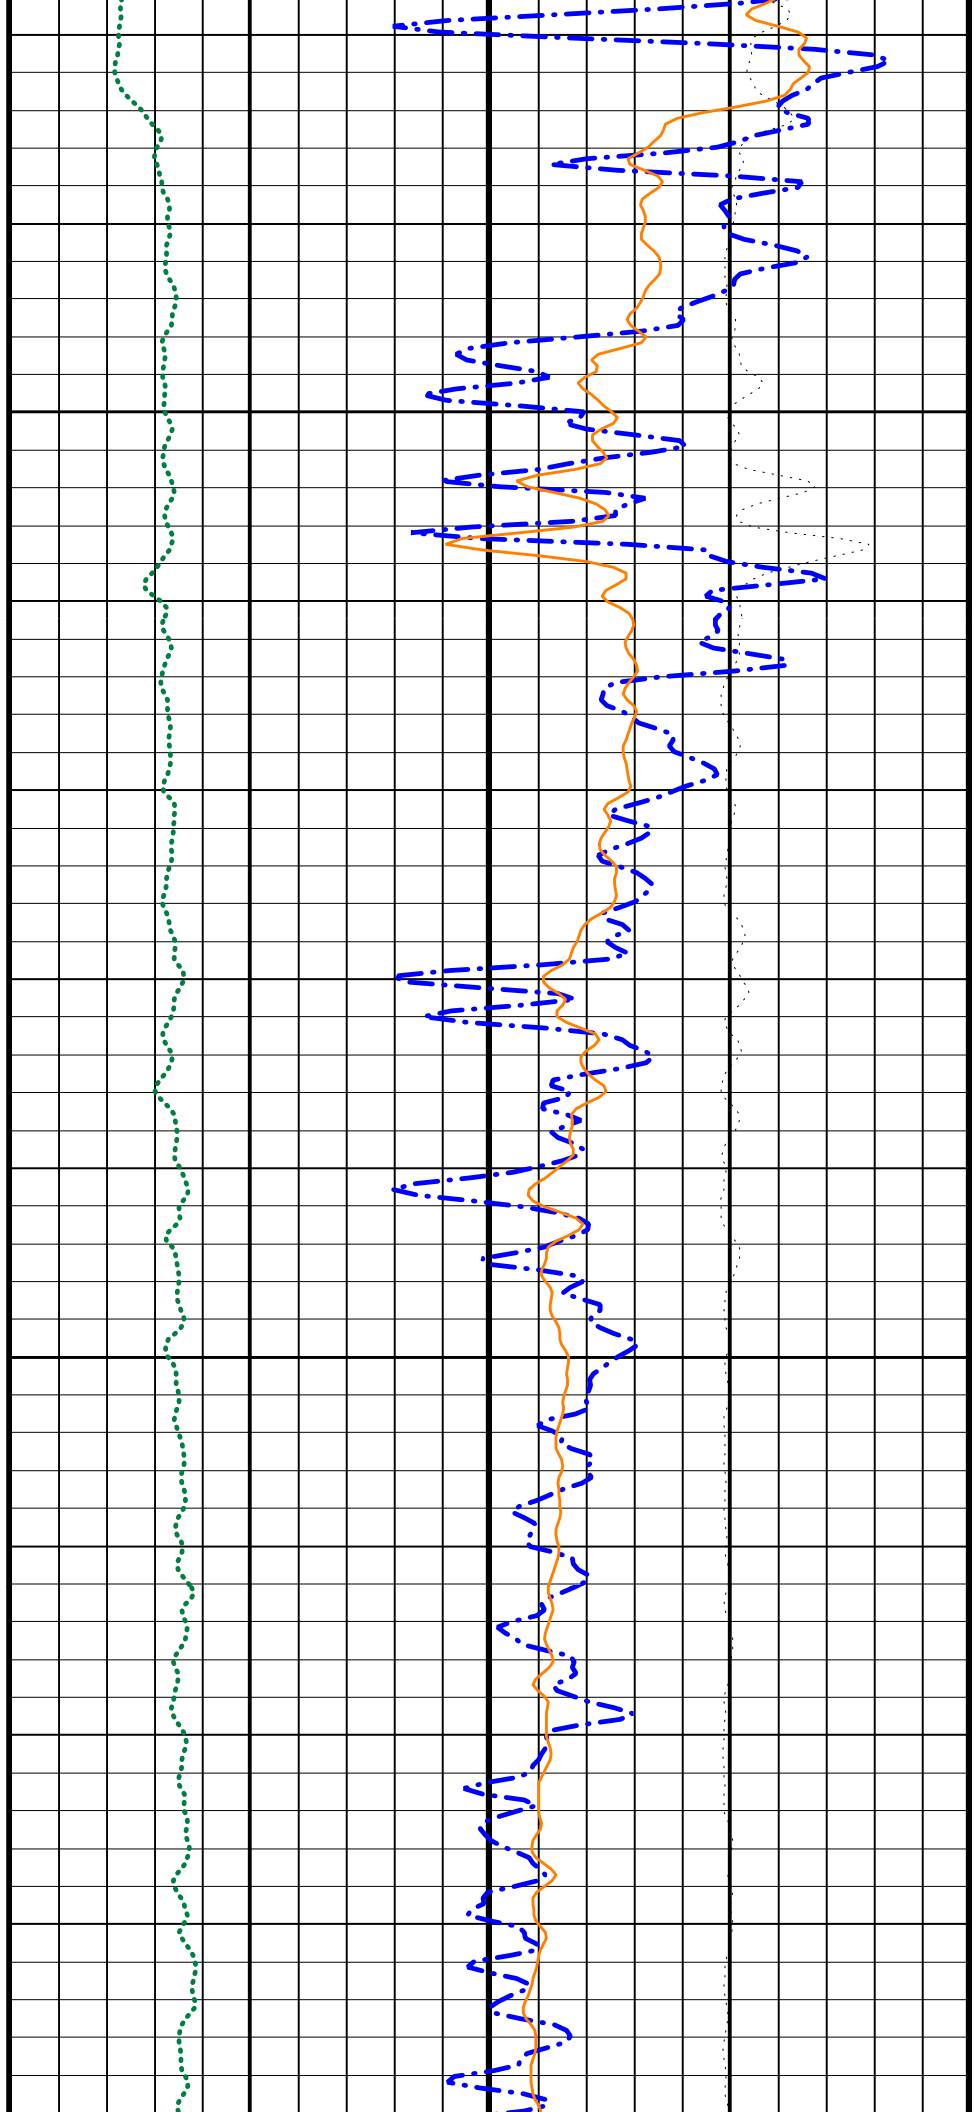

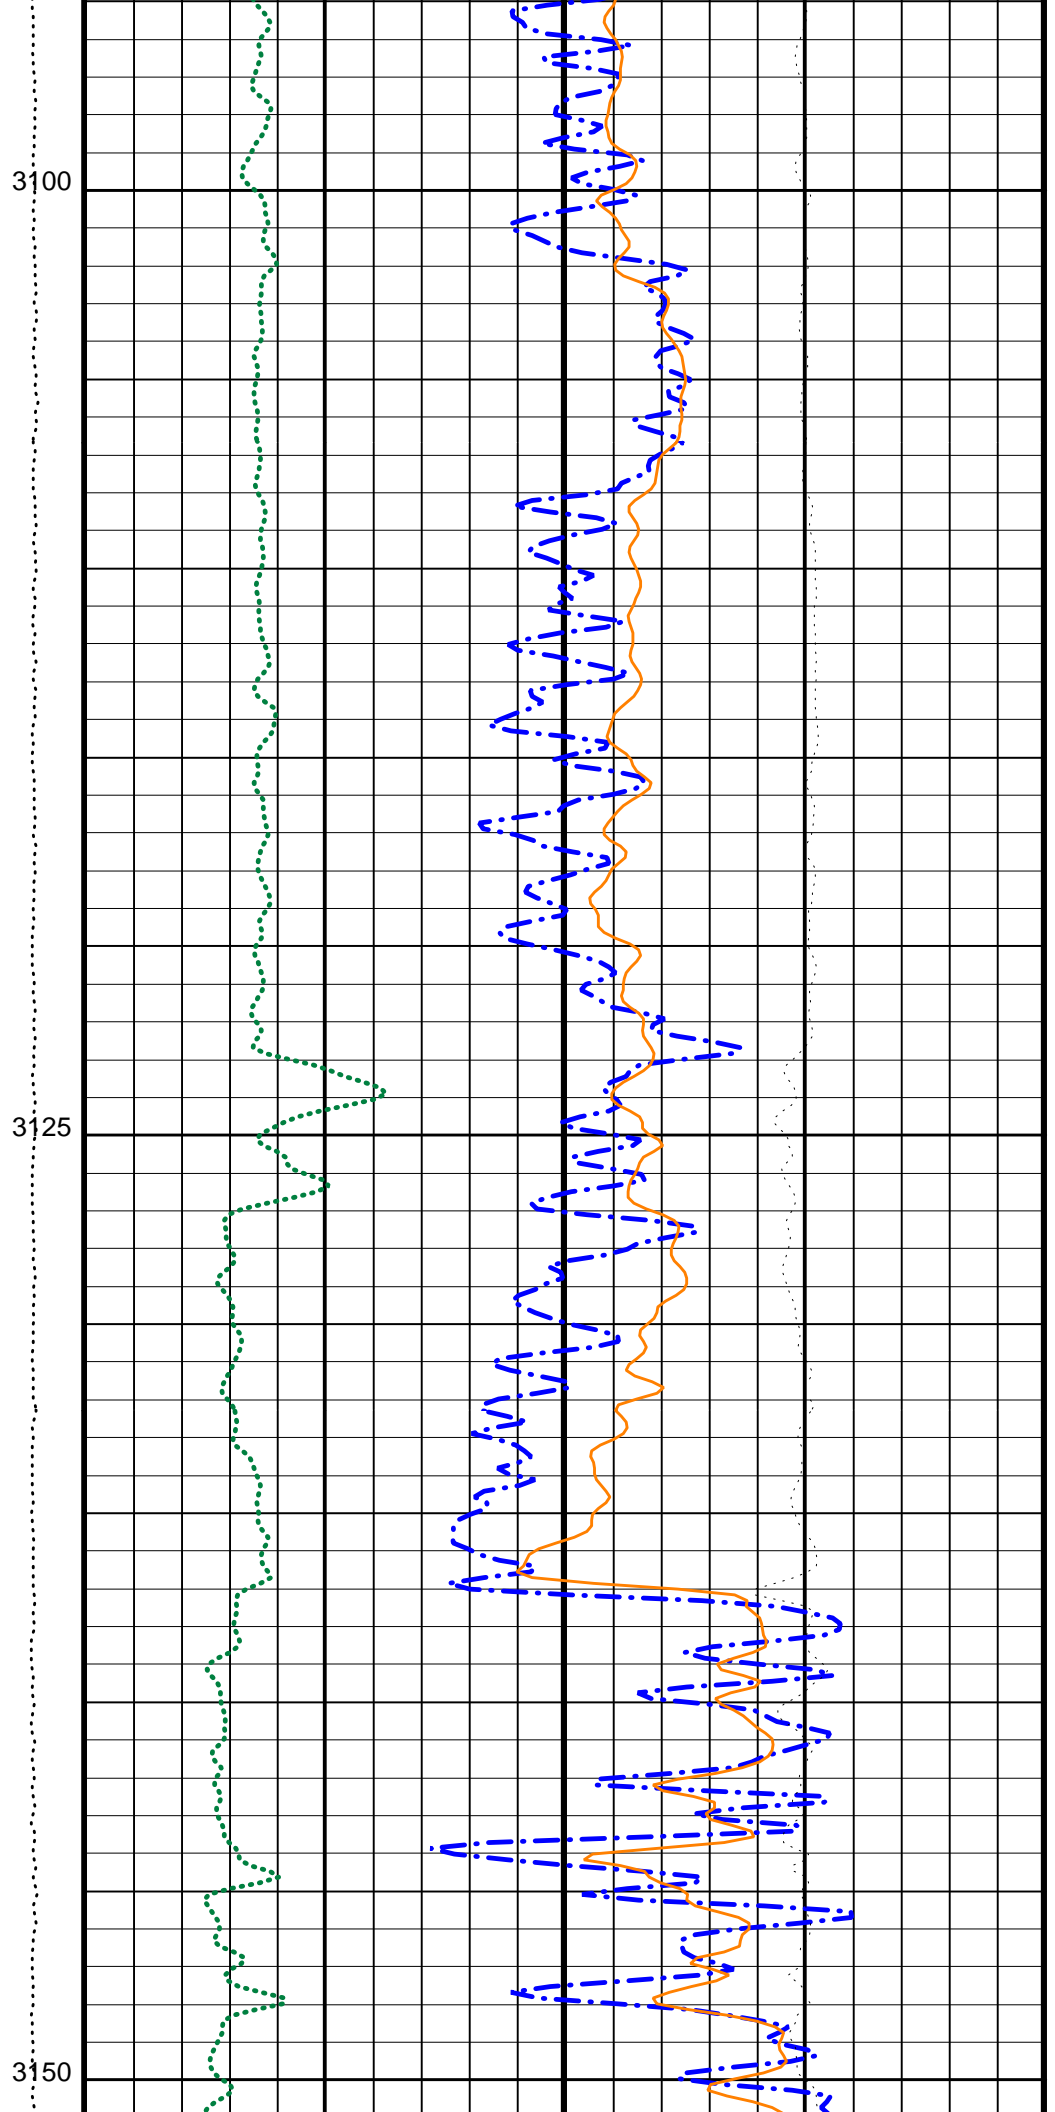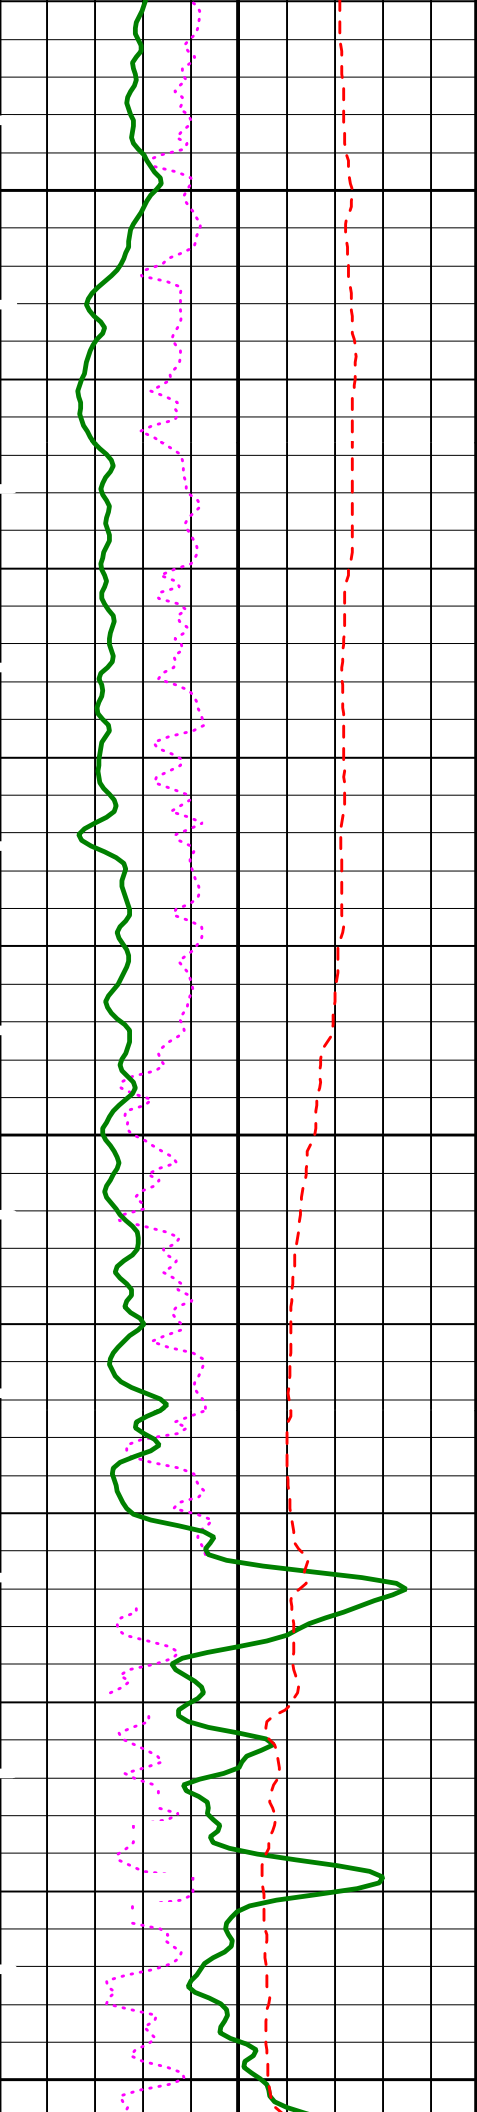

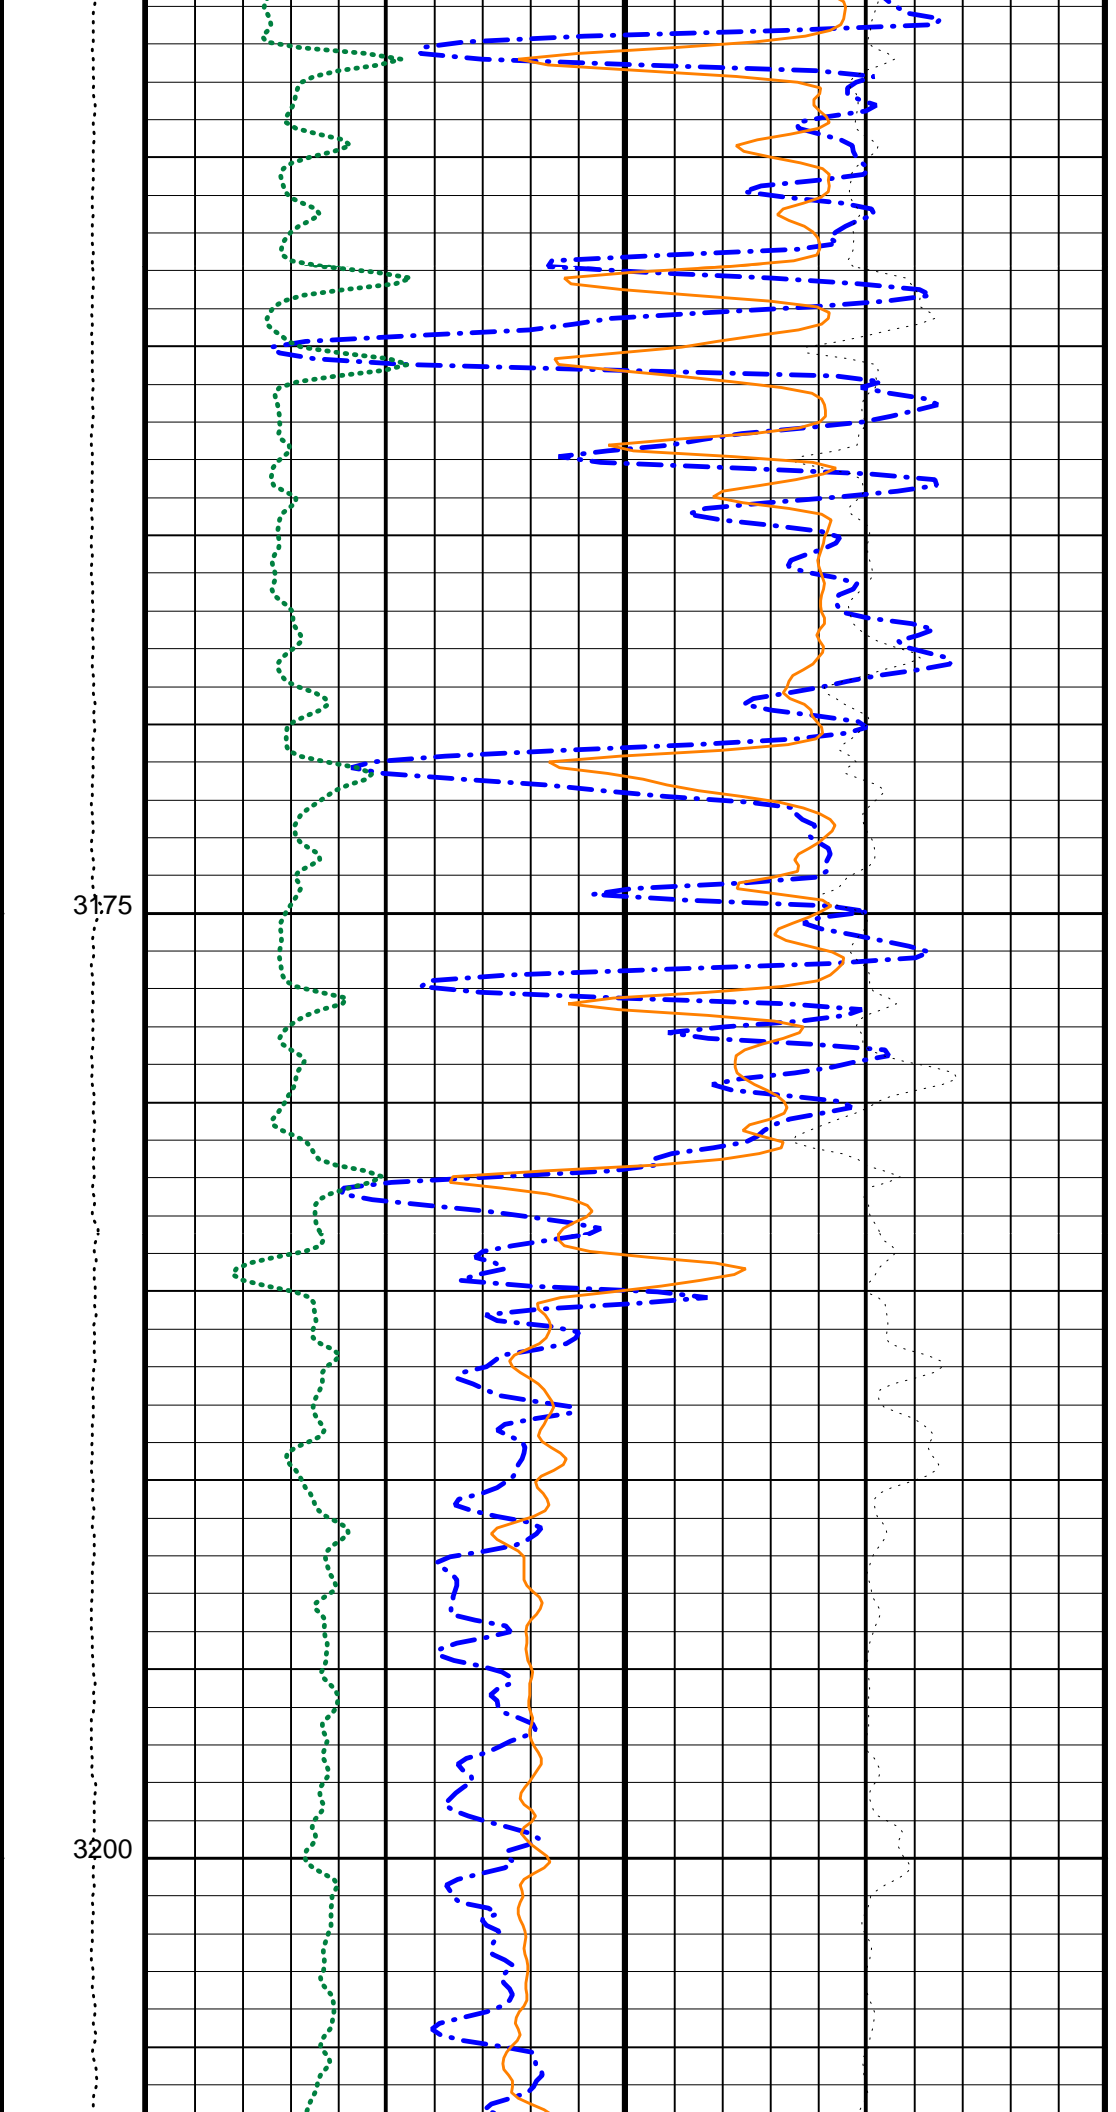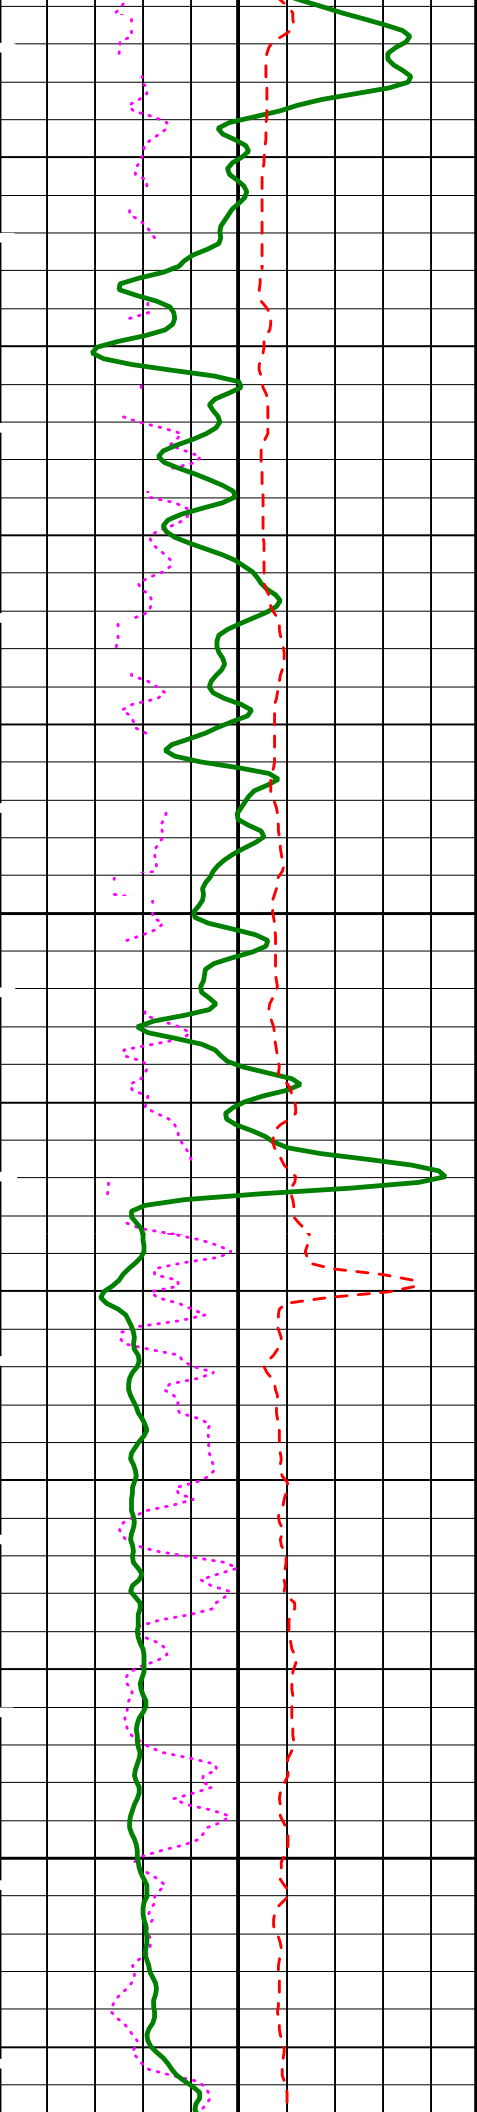

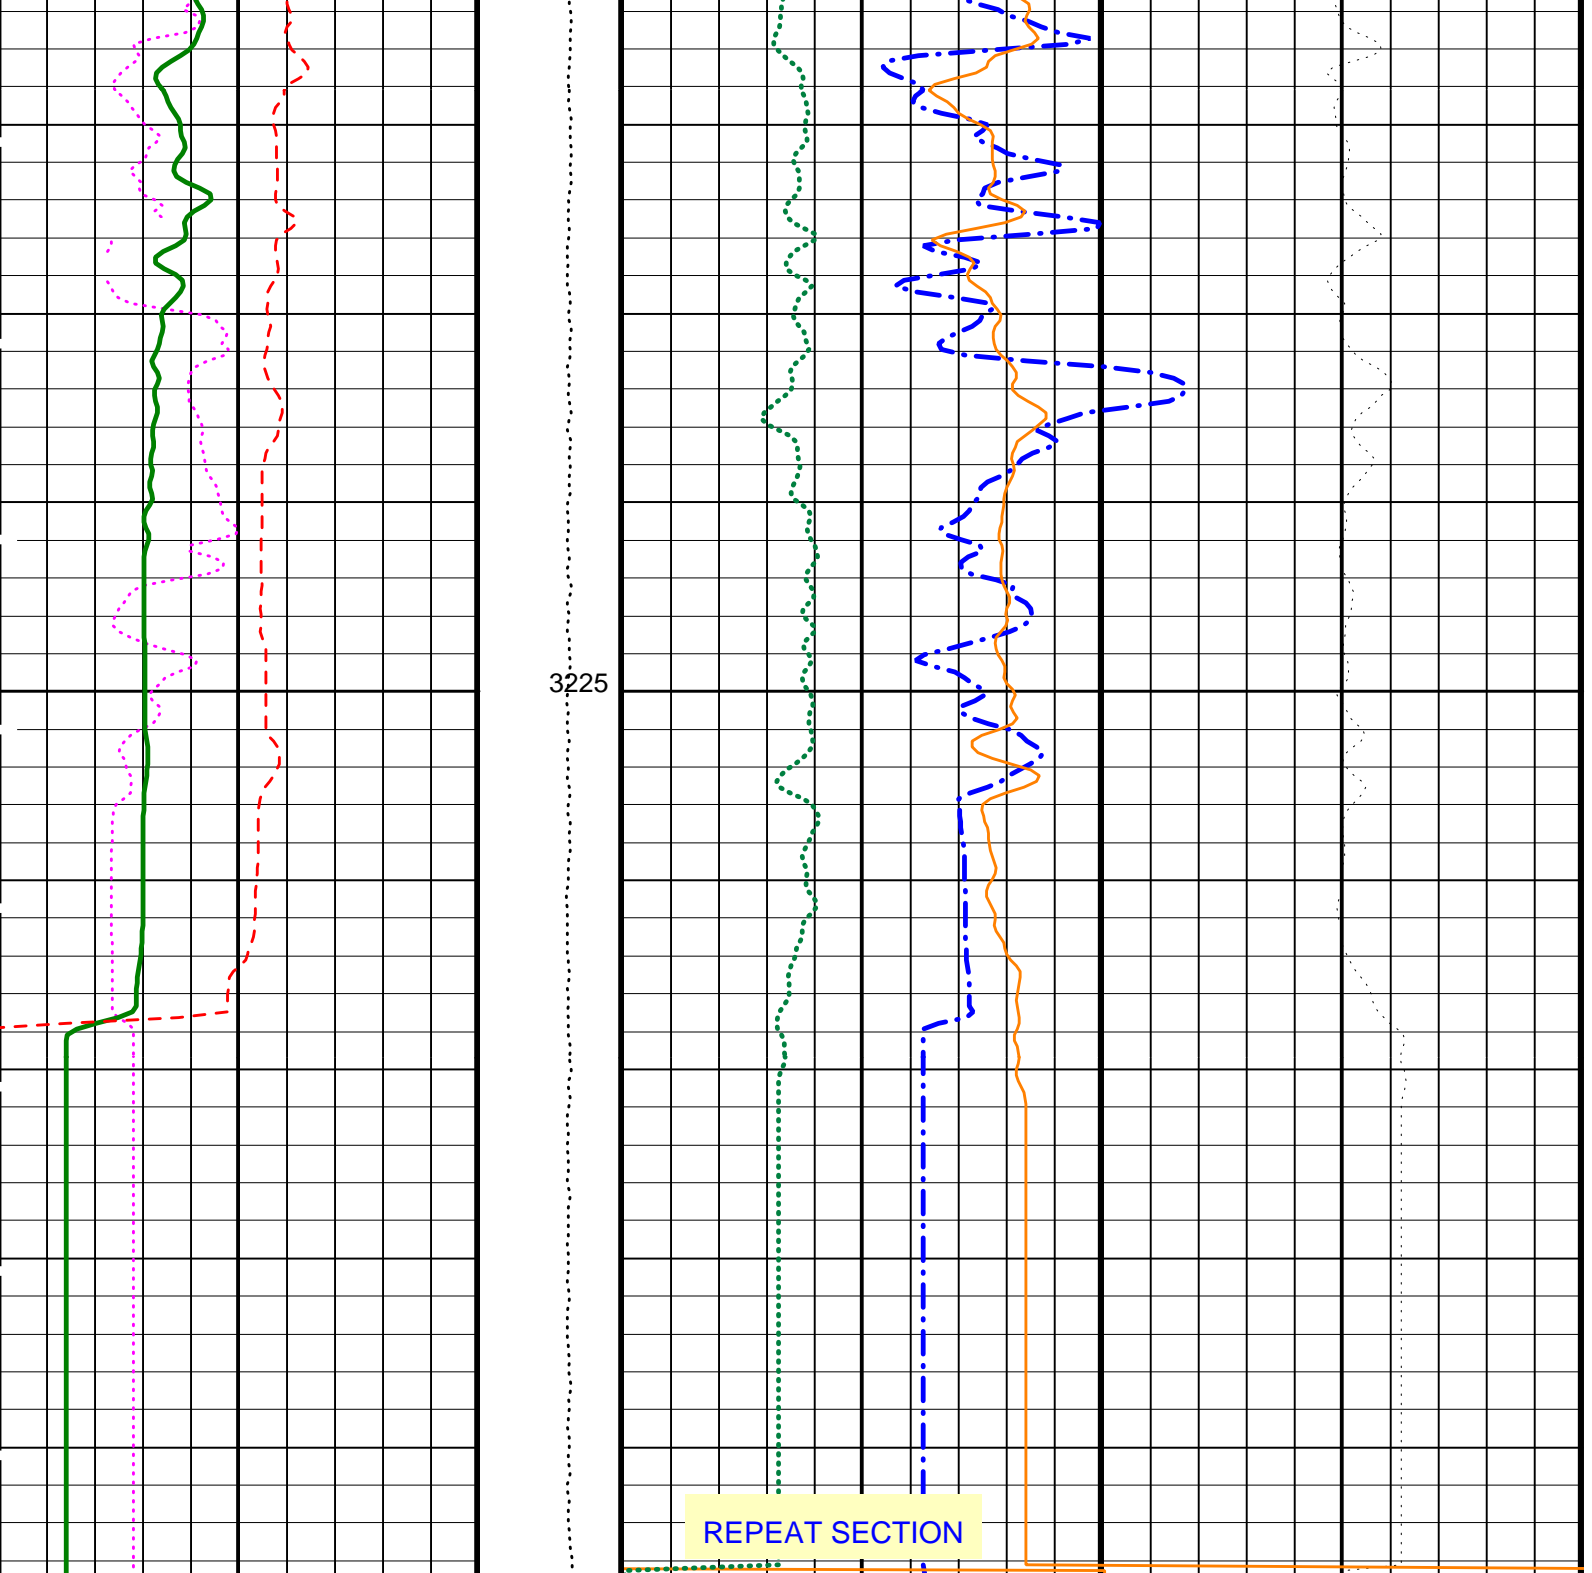

3225

REPEAT SECTION

<p>HLDS Caliper (LCAL) (IN)</p> <p>0 20</p>	<p>Tension (TENS) (LBF)</p> <p>10000 0</p>	<p>APS Near/Array Corrected Limestone Porosity (APLC) (PU)</p> <p>0 100</p>
<p>APS Effective Standoff in Limestone (STOF) (IN)</p> <p>-1 4</p>	<p>HLDS Bulk Density (RHOM) (G/C3)</p> <p>3 1</p>	
<p>HNGS Spectroscopy Gamma Ray (HSGR) (GAPI)</p> <p>0 150</p>	<p>HLDS Long Spaced Photoelectric Effect (PEFL) (---)</p> <p>0 10</p>	<p>HLDS Bulk Density Correction (DRH) (G/C3)</p> <p>-0.25 0.25</p>

PIP SUMMARY

▶ Time Mark Every 60 S

Parameters

DLIS Name	Description	Value	
	DIT-E: Dual Induction - E		
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
DGF2	Deep 20 kHz Gain Factor	1.00789	
DPH2	Deep 20 kHz Phase Shift	-0.152394	DEG
DRE2	Deep Real 20 kHz Sonde Error Correction	16.357	MM/M
DSR2	Deep Sigma Reference (20 kHz)	1843	MM/M
DXE2	Deep Quad 20 kHz Sonde Error Correction	64.6326	MM/M
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
IFRS	DIT-E Induction Frequency Selector	20	
IPHA	DIT-E Phasor Processing Mode	ALL	
IPRO	DIT-E Induction Processing Selector	PHASOR	
ITEN	DIT-E Temperature Enable	ENABLE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
MGF2	Medium 20 kHz Gain Factor	1.02964	
MPH2	Medium 20 kHz Phase Shift	-0.933067	DEG
MRE2	Medium Real 20 kHz Sonde Error Correction	-1.78642	MM/M
MSR2	Medium Sigma Reference (20 kHz)	3250	MM/M
MXE2	Medium Quad 20 kHz Sonde Error Correction	-34.2041	MM/M
SBR	Shoulder Bed Resistivity Factor	1	OHMM
SFCR	SFL Channel Ratio	1000	
SFLE	SFL Enable	ENABLE	
SHT	Surface Hole Temperature	20	DEGC
SPAE	DIT-E SPARC Processing Enable	ENABLE	
SPNV	SP Next Value	0	MV
	HLDS: Hostile Litho-Density Sonde		
CLCL	HLDS LS Control Loop Controller Mode	AUTO_DEFAULT	
CLCS	HLDS SS Control Loop Controller Mode	AUTO_DEFAULT	
CLLS	HLDS Mode Loop Long Spacing	AUTO	
CLSS	HLDS Mode Loop Short Spacing	AUTO	
DHC	Density Hole Correction	BS	
DPPM	Density Porosity Processing Mode	HIRS	
FD	Fluid Density	1	G/C3
LATC	HLDS Activation Correction	ON	
LLDL	HLDS LS Low Level Discriminator DAC	14000	
LLDS	HLDS SS Low Level Discriminator DAC	14000	
LLML	HLDS LS Low Level Discriminator Mode	AUTO	
LLMS	HLDS SS Low Level Discriminator Mode	AUTO	
MDEN	Matrix Density	2.71	G/C3
PHVL	HLDS Long Spacing High Voltage Setting	1000	V
PHVS	HLDS Short Spacing High Voltage Setting	1000	V
PSDL	HLDS LS Pulse Shape Compensation DAC	16000	
PSDS	HLDS SS Pulse Shape Compensation DAC	16000	
PSML	HLDS LS Pulse Shape Compensation Mode	AUTO	
PSMS	HLDS SS Pulse Shape Compensation Mode	AUTO	
	NPLC-B: Nuclear Porosity Lithology Cartridge - B		
NOTS	NPLC Old Temperature Sensor	NO	
	APS-BA: Accelerator-Porosity Tool		
	APS Software Version	5	
AASD	APS Thermal and Array Detectors High Voltage Setting	1958.44	V
ADSO	APS Array Detectors Data Source Switch	Both	
AFSD	APS Far Detector High Voltage Setting	2072.71	V
AHCS	APS Holesize Correction Source	GCSE	
AHSS	APS Holesize Correction Switch	ON	
AMTY	APS Environmental Corrections Mud Type	WaterBaseBarite	
ANSD	APS Near Detector High Voltage Setting	1727.99	V
AOTS	APS Old Temperature Sensor Switch	NO	
ASOS	APS Standoff Correction Switch	ON	
ATSS	APS Temperature-Pressure-Salinity Correction Switch	OFF	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC
DPPM	Density Porosity Processing Mode	HIRS	
FSAL	Formation Salinity	-50000	PPM
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
NARC	APS Near/Array Calibration Ratio	1.05147	
NFRC	APS Near/Far Calibration Ratio	0.886931	
SHT	Surface Hole Temperature	20	DEGC
	HNGS-BA: Hostile Natural Gamma Ray Sonde		
BAR1	HNGS Detector 1 Barite Constant	1	
BAR2	HNGS Detector 2 Barite Constant	1	
BHK	HNGS Borehole Potassium Correction Concentration	0	
BHS	Borehole Status	OPEN	
BHT	Bottom Hole Temperature (used in calculations)	100	DEGC

CSD1	Inner Casing Outer Diameter	0	IN
CSD2	Outer Casing Outer Diameter	0	IN
CSW1	Inner Casing Weight	0	LB/F
CSW2	Outer Casing Weight	0	LB/F
DBCC	HNGS Barite Constant Correction Flag	NONE	
GCSE	Generalized Caliper Selection	LCAL	
GDEV	Average Angular Deviation of Borehole from Normal	0	DEG
GGRD	Geothermal Gradient	0.018227	DC/M
GRSE	Generalized Mud Resistivity Selection	CHART_GEN_9	
GTSE	Generalized Temperature Selection	LINEAR_ESTIMATE	
H1P	HNGS Detector 1 Allow/Disallow In Processing	ALLOW	
H2P	HNGS Detector 2 Allow/Disallow In Processing	ALLOW	
HABK	HNGS Borehole Potassium Running Average	-0.0178137	
HALF	HNGS Alpha Filter Length	60	IN
HCRB	HNGS Apply Borehole Potassium Correction	NONE	
HMWM	Mud Weighting Material	NATU	
HNPE	HNGS Processing Enable	YES	
MATR	Rock Matrix for Neutron Porosity Corrections	LIMESTONE	
S1BI	HNGS Detector 1 Calibration Bismuth Count Rate	-999.25	CPS
S2BI	HNGS Detector 2 Calibration Bismuth Count Rate	-999.25	CPS
SGRC	HNGS Standard Gamma-Ray Correction Flag	YES	
SHT	Surface Hole Temperature	20	DEGC
TPOS	Tool Position	ECCE	
VBA1	HNGS Detector 1 Variable Barite Factor Running Average	0.96088	
VBA2	HNGS Detector 2 Variable Barite Factor Running Average	0.5297	
System and Miscellaneous			
ALTDPCCHAN	Name of alternate depth channel	SpeedCorrectedDepth	
BS	Bit Size	11.438	IN
BSAL	Borehole Salinity	-50000.00	PPM
CSIZ	Current Casing Size	0.000	IN
CWEI	Casing Weight	0.00	LB/F
DFD	Drilling Fluid Density	1.10	G/C3
MST	Mud Sample Temperature	32.00	DEGC
PBVSADP	Use alternate depth channel for playback	NO	
RMFS	Resistivity of Mud Filtrate Sample	-50000.0000	OHMM
RW	Resistivity of Connate Water	1.0000	OHMM
TD	Total Depth	-50000	M
TDD	Total Depth - Driller	-50000.00	M
TDL	Total Depth - Logger	-50000.00	M
TWS	Temperature of Connate Water Sample	37.78	DEGC

Format: APSLiquidPorosity_1 Vertical Scale: 1:200 Graphics File Created: 18-Jan-2003 20:21

OP System Version: 10C0-306

MCM

DIT-E	10C0-306	DTA-A	10C0-306
HLDS	SPC-2277-NUCL_b	NPLC-B	OP10-KP1
APS-BA	SPC-2277-NUCL_b	HNGS-BA	SPC-2277-NUCL_b
DTC-H	10C0-306		

Output DLIS Files

DEFAULT	PI_LDL_APS_NGS_012LUP	FN:15	PRODUCER	18-Jan-2003 20:20
REDUCE	PI_LDL_APS_NGS_012LUP	FN:16	PRODUCER	18-Jan-2003 20:20

Calibration and Check Summary

Measurement	Nominal	Master	Before	After	Change	Limit	Units
Hostile Litho-Density Sonde Wellsite Calibration - Background Measurement							
Master: 13-Dec-2002 14:00 Before: 15-Jan-2003 11:10 After: 19-Jan-2003 2:14							
SS Cs Resolution Bkg	9.000	8.065	8.135	8.044	-0.09056	1.800	%
LS Cs Resolution Bkg	9.000	8.249	8.108	8.124	0.01535	1.800	%
LSW1 Background	100.0	86.88	86.46	86.16	-0.2965	3.000	CPS
LSW2 Background	100.0	82.90	80.84	81.32	0.4762	3.000	CPS
LSW3 Background	200.0	182.1	179.4	180.0	0.5779	6.000	CPS
LSW4 Background	250.0	221.9	216.6	220.1	3.541	7.500	CPS
LSW5 Background	600.0	510.1	505.1	504.0	-1.098	18.00	CPS
SSW1 Background	100.0	96.14	98.01	96.03	-1.977	3.000	CPS
SSW2 Background	200.0	176.7	177.3	173.7	-3.596	6.000	CPS
SSW3 Background	500.0	478.2	477.6	477.4	-0.1395	15.00	CPS
SSW4 Background	270.0	244.1	244.0	242.2	-1.773	8.100	CPS
SSW5 Background	200.0	177.5	175.7	176.8	1.105	6.000	CPS

Hostile Litho-Density Sonde Wellsite Calibration - Aluminum Measurement

Master: 13-Dec-2002 15:15

Master: 13-Dec-2002 15:13	LSW1 Aluminum	600.0	580.8	N/A	N/A	N/A	N/A	CPS
	LSW2 Aluminum	900.0	822.1	N/A	N/A	N/A	N/A	CPS
	LSW3 Aluminum	1100	985.4	N/A	N/A	N/A	N/A	CPS
	LSW4 Aluminum	580.0	489.2	N/A	N/A	N/A	N/A	CPS
	LSW5 Aluminum	570.0	453.3	N/A	N/A	N/A	N/A	CPS
	SSW1 Aluminum	2800	2597	N/A	N/A	N/A	N/A	CPS
	SSW2 Aluminum	8000	7087	N/A	N/A	N/A	N/A	CPS
	SSW3 Aluminum	11600	9849	N/A	N/A	N/A	N/A	CPS
	SSW4 Aluminum	5000	4127	N/A	N/A	N/A	N/A	CPS
	SSW5 Aluminum	660.0	537.2	N/A	N/A	N/A	N/A	CPS

Hostile Litho-Density Sonde Wellsite Calibration - Lithology Measurement

Master: 13-Dec-2002 15:11

LSW1 Iron	400.0	401.7	N/A	N/A	N/A	N/A	CPS
LSW2 Iron	730.0	683.6	N/A	N/A	N/A	N/A	CPS
LSW3 Iron	1000	900.2	N/A	N/A	N/A	N/A	CPS
LSW4 Iron	520.0	465.6	N/A	N/A	N/A	N/A	CPS
LSW5 Iron	470.0	434.8	N/A	N/A	N/A	N/A	CPS
SSW1 Iron	2100	1961	N/A	N/A	N/A	N/A	CPS
SSW2 Iron	6800	6103	N/A	N/A	N/A	N/A	CPS
SSW3 Iron	10800	9305	N/A	N/A	N/A	N/A	CPS
SSW4 Iron	4600	3921	N/A	N/A	N/A	N/A	CPS
SSW5 Iron	580.0	502.8	N/A	N/A	N/A	N/A	CPS

Hostile Litho-Density Sonde Wellsite Calibration - Caliper Calibration

Before: 15-Jan-2003 11:25

HLDS Caliper Small Ring	15.00	N/A	18.20	N/A	N/A	N/A	IN
HLDS Caliper Large Ring	17.50	N/A	20.31	N/A	N/A	N/A	IN

Accelerator-Porosity Tool Wellsite Calibration - Detector Background

Master: 28-Nov-2002 19:52 Before: 18-Jan-2003 18:09 After: 19-Jan-2003 0:35

Near Det Bkg Cntrate	30.00	32.65	61.25	31.59	-29.66	N/A	CPS
Far Det Bkg Cntrate	30.00	31.56	38.09	33.02	-5.071	N/A	CPS
Array-1 Det Bkg Cntrate	30.00	29.11	38.78	28.71	-10.07	N/A	CPS
Array-2 Det Bkg Cntrate	30.00	29.96	40.03	29.94	-10.09	N/A	CPS
Array Therm Det Bkg Cntrate	30.00	32.97	41.48	32.50	-8.981	N/A	CPS

Accelerator-Porosity Tool Wellsite Calibration - Calibration Ratios

Master: 28-Nov-2002 19:53

Near/Far Calibration Ratio	0.9250	0.8869	N/A	N/A	N/A	N/A
Near/Array Calibration Ratio	1.030	1.051	N/A	N/A	N/A	N/A
Near/Array Cal Ratio Up/Down	1.000	1.002	N/A	N/A	N/A	N/A

Accelerator-Porosity Tool Wellsite Calibration - Tank Check

Master: 28-Nov-2002 19:54

Array-1 Standoff Porosity	11.75	11.90	N/A	N/A	N/A	N/A	PU
Array-2 Standoff Porosity	11.75	11.44	N/A	N/A	N/A	N/A	PU
Average Slowing Down Time	6.000	5.850	N/A	N/A	N/A	N/A	US
Array-1 SDT Ratio Up/Down	1.000	0.9966	N/A	N/A	N/A	N/A	
Array-2 SDT Ratio Up/Down	1.000	0.9889	N/A	N/A	N/A	N/A	
Sigma Formation	27.50	27.81	N/A	N/A	N/A	N/A	CU

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 1 Check

Master: 15-Jan-2003 16:08 Before: 15-Jan-2003 16:17 After: 19-Jan-2003 2:15

Na 511 Peak Loc	40.00	40.59	40.72	40.70	-0.02711	1.000	
Na 511 Peak Res	15.50	17.05	17.42	16.61	-0.8152	2.000	%
High Voltage	1150	1212	1212	1215	2.189	30.00	V
Na 1785 Peak Loc	142.6	145.6	145.3	145.8	0.5008	7.000	
Na 1785 Peak Res	8.500	9.037	9.666	9.711	0.04524	2.000	%
Temperature	15.50	32.69	32.84	29.54	-3.307	N/A	DEGC
Na Count Rate	45.00	44.80	43.98	43.51	-0.4779	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Detector 2 Check

Master: 15-Jan-2003 16:08 Before: 15-Jan-2003 16:17 After: 19-Jan-2003 2:15

Na 511 Peak Loc	40.00	40.55	40.57	40.61	0.03738	1.000	
Na 511 Peak Res	15.50	16.60	16.91	17.25	0.3423	2.000	%
High Voltage	1150	1239	1239	1242	2.449	30.00	V
Na 1785 Peak Loc	142.6	144.7	144.4	144.4	0.07025	7.000	
Na 1785 Peak Res	8.500	9.925	9.708	9.893	0.1852	2.000	%
Temperature	15.50	32.80	32.89	29.63	-3.265	N/A	DEGC
Na Count Rate	45.00	44.45	43.98	43.50	-0.4887	8.000	CPS

Hostile Natural Gamma Ray Sonde Wellsite Calibration - Ratio Of Detector 1 To Detector 2

Master: 15-Jan-2003 16:08 Before: 15-Jan-2003 16:17 After: 19-Jan-2003 2:15

Coincidence Count Rate Ratio	1.000	1.008	1.0000	1.001	0.001407	0.05000
------------------------------	-------	-------	--------	-------	----------	---------

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 1 Calibration

Master: 15-Jan-2003 16:01

Na 511 Peak Set Point	40.00	41.00	--	--	--	--
Th Peak Loc	209.6	209.3	--	--	--	--
Th Peak Res	7.000	8.207	--	--	--	%

Background Count Rate	142.5	23.15	--	--	--	--	CPS
Gain Ratio	1.000	0.9810	--	--	--	--	

Hostile Natural Gamma Ray Sonde Master Calibration - Detector 2 Calibration

Master: 15-Jan-2003 16:01

Na 511 Peak Set Point	40.00	41.00	--	--	--	--	
Th Peak Loc	209.6	209.3	--	--	--	--	
Th Peak Res	7.000	7.848	--	--	--	--	%
Background Count Rate	142.5	21.80	--	--	--	--	CPS
Gain Ratio	1.000	0.9821	--	--	--	--	

Accelerator-Porosity Tool - Detector Plateau Settings :

Near Detector Plateau Setting	1728 V
Far Detector Plateau Setting	2073 V
Array Detector Plateau Setting	1958 V

Dual Induction - E / Equipment Identification

Primary Equipment:		
Dual Induction Sonde	DIS - HB	442
Dual Induction Cartridge	DIC - EB	438
Auxiliary Equipment:		
Mass Isolated Housing	MIH - ZA	

Hostile Litho-Density Sonde / Equipment Identification

Primary Equipment:		
Hostile Litho Density Sonde	HLDS - D	45
Hostile Litho Density High Voltage	HLDV - D	35
Gamma Source Radioactive	GSR - Z	1846
Auxiliary Equipment:		
Hostile Litho Density Pad	HLDP - C	45
Hostile Litho Density High Voltage Housi	HEH - H	35

Hostile Litho-Density Sonde Wellsite Calibration

Background Measurement

Phase	SS Cs Resolution Bkg %	Value	Phase	LS Cs Resolution Bkg %	Value	Phase	LSW1 Background CPS	Value
Master		8.065	Master		8.249	Master		86.88
Before		8.135	Before		8.108	Before		86.46
After		8.044	After		8.124	After		86.16
7.000 (Minimum) 9.000 (Nominal) 11.000 (Maximum)			7.000 (Minimum) 9.000 (Nominal) 11.000 (Maximum)			55.00 (Minimum) 100.0 (Nominal) 150.0 (Maximum)		
Phase	LSW2 Background CPS	Value	Phase	LSW3 Background CPS	Value	Phase	LSW4 Background CPS	Value
Master		82.90	Master		182.1	Master		221.9
Before		80.84	Before		179.4	Before		216.6
After		81.32	After		180.0	After		220.1
50.00 (Minimum) 100.0 (Nominal) 140.0 (Maximum)			110.0 (Minimum) 200.0 (Nominal) 290.0 (Maximum)			140.0 (Minimum) 250.0 (Nominal) 360.0 (Maximum)		
Phase	LSW5 Background CPS	Value	Phase	SSW1 Background CPS	Value	Phase	SSW2 Background CPS	Value
Master		510.1	Master		96.14	Master		176.7
Before		505.1	Before		98.01	Before		177.3
After		504.0	After		96.03	After		173.7
330.0 (Minimum) 600.0 (Nominal) 830.0 (Maximum)			55.00 (Minimum) 100.0 (Nominal) 150.0 (Maximum)			100.0 (Minimum) 200.0 (Nominal) 260.0 (Maximum)		
Phase	SSW3 Background CPS	Value	Phase	SSW4 Background CPS	Value	Phase	SSW5 Background CPS	Value
Master		478.2	Master		244.1	Master		177.5
Before		477.6	Before		244.0	Before		175.7
After		477.1	After		243.2	After		173.0
330.0 (Minimum) 600.0 (Nominal) 830.0 (Maximum)			55.00 (Minimum) 100.0 (Nominal) 150.0 (Maximum)			100.0 (Minimum) 200.0 (Nominal) 260.0 (Maximum)		

After		477.4	After		242.2	After		176.8	
	280.0 (Minimum)	500.0 (Nominal)	700.0 (Maximum)	150.0 (Minimum)	270.0 (Nominal)	380.0 (Maximum)	110.0 (Minimum)	200.0 (Nominal)	270.0 (Maximum)
Master: 13-Dec-2002 14:00			Before: 15-Jan-2003 11:10			After: 19-Jan-2003 2:14			

Hostile Litho-Density Sonde Master Calibration											
Detector Background Measurement											
Phase	LSW1 Background CPS		Value	Phase	LSW2 Background CPS		Value	Phase	LSW3 Background CPS		Value
Master			86.88	Master			82.90	Master			182.1
	55.00 (Minimum)	100.0 (Nominal)	150.0 (Maximum)		50.00 (Minimum)	100.0 (Nominal)	140.0 (Maximum)		110.0 (Minimum)	200.0 (Nominal)	290.0 (Maximum)
Phase	LSW4 Background CPS		Value	Phase	LSW5 Background CPS		Value	Phase	LS Cs Resolution Bkg %		Value
Master			221.9	Master			510.1	Master			8.249
	140.0 (Minimum)	250.0 (Nominal)	360.0 (Maximum)		330.0 (Minimum)	600.0 (Nominal)	830.0 (Maximum)		7.000 (Minimum)	9.000 (Nominal)	11.00 (Maximum)
Phase	SSW1 Background CPS		Value	Phase	SSW2 Background CPS		Value	Phase	SSW3 Background CPS		Value
Master			96.14	Master			176.7	Master			478.2
	55.00 (Minimum)	100.0 (Nominal)	150.0 (Maximum)		100.0 (Minimum)	200.0 (Nominal)	260.0 (Maximum)		280.0 (Minimum)	500.0 (Nominal)	700.0 (Maximum)
Phase	SSW4 Background CPS		Value	Phase	SSW5 Background CPS		Value	Phase	SS Cs Resolution Bkg %		Value
Master			244.1	Master			177.5	Master			8.065
	150.0 (Minimum)	270.0 (Nominal)	380.0 (Maximum)		110.0 (Minimum)	200.0 (Nominal)	270.0 (Maximum)		7.000 (Minimum)	9.000 (Nominal)	11.00 (Maximum)
Master: 13-Dec-2002 14:00											

Hostile Litho-Density Sonde Master Calibration											
Detector Aluminum Measurement (bkqd-subtracted)											
Phase	LSW1 Aluminum CPS		Value	Phase	LSW2 Aluminum CPS		Value	Phase	LSW3 Aluminum CPS		Value
Master			580.8	Master			822.1	Master			985.4
	420.0 (Minimum)	600.0 (Nominal)	700.0 (Maximum)		650.0 (Minimum)	900.0 (Nominal)	1050 (Maximum)		800.0 (Minimum)	1100 (Nominal)	1300 (Maximum)
Phase	LSW4 Aluminum CPS		Value	Phase	LSW5 Aluminum CPS		Value	Phase	SSW1 Aluminum CPS		Value
Master			489.2	Master			453.3	Master			2597
	410.0 (Minimum)	580.0 (Nominal)	670.0 (Maximum)		410.0 (Minimum)	570.0 (Nominal)	660.0 (Maximum)		2000 (Minimum)	2800 (Nominal)	3200 (Maximum)
Phase	SSW2 Aluminum CPS		Value	Phase	SSW3 Aluminum CPS		Value	Phase	SSW4 Aluminum CPS		Value
Master			7087	Master			9849	Master			4127
	5800 (Minimum)	8000 (Nominal)	9300 (Maximum)		8300 (Minimum)	11600 (Nominal)	13500 (Maximum)		3500 (Minimum)	5000 (Nominal)	5800 (Maximum)
Phase	SSW5 Aluminum CPS		Value								
Master			537.2								
	470.0 (Minimum)	660.0 (Nominal)	770.0 (Maximum)								
Master: 13-Dec-2002 15:15											

Hostile Litho-Density Sonde Master Calibration											
Detector Litholog Measurement (bkqd-subtracted)											
Phase	LSW1 Iron CPS		Value	Phase	LSW2 Iron CPS		Value	Phase	LSW3 Iron CPS		Value
Master			401.7	Master			683.6	Master			900.2
	290.0 (Minimum)	400.0 (Nominal)	470.0 (Maximum)		520.0 (Minimum)	730.0 (Nominal)	850.0 (Maximum)		720.0 (Minimum)	1000 (Nominal)	1160 (Maximum)
Phase	LSW4 Iron CPS		Value	Phase	LSW5 Iron CPS		Value	Phase	SSW1 Iron CPS		Value
Master			465.6	Master			434.8	Master			1961
	370.0 (Minimum)	520.0 (Nominal)	600.0 (Maximum)		340.0 (Minimum)	470.0 (Nominal)	550.0 (Maximum)		1500 (Minimum)	2100 (Nominal)	2400 (Maximum)
Phase	SSW2 Iron CPS		Value	Phase	SSW3 Iron CPS		Value	Phase	SSW4 Iron CPS		Value
Master			6103	Master			9305	Master			3921
	4900 (Minimum)	6800 (Nominal)	7900 (Maximum)		7800 (Minimum)	10800 (Nominal)	12600 (Maximum)		3300 (Minimum)	4600 (Nominal)	5400 (Maximum)
Phase	SSW5 Iron CPS		Value								
Master			502.8								
	420.0 (Minimum)	580.0 (Nominal)	680.0 (Maximum)								
Master: 13-Dec-2002 15:11											

Hostile Litho-Density Sonde Master Calibration

Quality Ratios

Phase	AL CALIBRATION RATIO 1	Value	Phase	AL CALIBRATION RATIO 2	Value	Phase	AL CALIBRATION RATIO 3	Value
Master		1.046	Master		2.112	Master		0.6163
	0.9000 (Minimum) 1.000 (Nominal) 1.100 (Maximum)			1.800 (Minimum) 2.000 (Nominal) 2.200 (Maximum)			0.4500 (Minimum) 0.5500 (Nominal) 0.6500 (Maximum)	
Phase	AL CALIBRATION RATIO 4	Value	Phase	Pad-Wear SS Ratio	Value	Phase	Pad-Wear LS Ratio	Value
Master		0.5569	Master		0.9905	Master		0.9885
	0.4000 (Minimum) 0.5000 (Nominal) 0.6000 (Maximum)			0.9800 (Minimum) 0.9880 (Nominal) 0.9960 (Maximum)			0.9800 (Minimum) 0.9880 (Nominal) 0.9960 (Maximum)	
Phase	Pad-Position SS Ratio	Value	Phase	Pad-Position LS Ratio	Value			
Master		0.9979	Master	EXCEEDS LIMIT	0.9509			
	0.9900 (Minimum) 0.9940 (Nominal) 1.015 (Maximum)			0.9850 (Minimum) 0.9940 (Nominal) 1.010 (Maximum)				

Master: 14-Dec-2002 14:24

Nuclear Porosity Lithology Cartridge - B / Equipment Identification

Primary Equipment:	NPLC Cartridge	NPLC - B	79
Auxiliary Equipment:	NPLC Housing	NPH - B	82

Accelerator-Porosity Tool / Equipment Identification

Primary Equipment:	Accelerator-Porosity Sonde	APS - BA	22
	APS Minitron	MNTR - F	4185
Auxiliary Equipment:	Accelerator-Porosity Housing	APH - AC	22
	APS Calibration Water Tank	SFT - 178	4722
	APS Aluminium Calibrator Sleeve	SFT - 281	24

Accelerator-Porosity Tool Wellsite Calibration

Detector Background

Phase	Near Det Bkg Cntrate CPS	Value	Phase	Far Det Bkg Cntrate CPS	Value	Phase	Array-1 Det Bkg Cntrate CPS	Value
Master		32.65	Master		31.56	Master		29.11
Before	EXCEEDS LIMIT	61.25	Before		38.09	Before		38.78
After		31.59	After		33.02	After		28.71
	1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)			1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)			1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)	
Phase	Array-2 Det Bkg Cntrate CPS	Value	Phase	Array Therm Det Bkg Cntrate CPS	Value			
Master		29.96	Master		32.97			
Before		40.03	Before		41.48			
After		29.94	After		32.50			
	1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)			1.000 (Minimum) 30.00 (Nominal) 50.00 (Maximum)				

Master: 28-Nov-2002 19:52 Before: 18-Jan-2003 18:09 After: 19-Jan-2003 0:35

Accelerator-Porosity Tool Wellsite Calibration

Calibration Ratios

Phase	Near/Far Calibration Ratio	Value	Phase	Near/Array Calibration Ratio	Value	Phase	Near/Array Cal Ratio Up/Down	Value
Master		0.8869	Master		1.051	Master		1.002
	0.8000 (Minimum) 0.9250 (Nominal) 1.050 (Maximum)			0.9000 (Minimum) 1.030 (Nominal) 1.170 (Maximum)			0.9700 (Minimum) 1.000 (Nominal) 1.030 (Maximum)	

Master: 28-Nov-2002 19:53

Accelerator-Porosity Tool Wellsite Calibration

Tank Check

Phase	Array-1 Standoff Porosity PU	Value	Phase	Array-2 Standoff Porosity PU	Value	Phase	Average Slowing Down Time US	Value

Master	9.900 (Minimum)	11.75 (Nominal)	13.60 (Maximum)	11.90	Master	9.900 (Minimum)	11.75 (Nominal)	13.60 (Maximum)	11.44	Master	5.500 (Minimum)	6.000 (Nominal)	6.250 (Maximum)	5.850
Phase	Array-1 SDT Ratio Up/Down			Value	Phase	Array-2 SDT Ratio Up/Down			Value	Phase	Sigma Formation CU			Value
Master				0.9966	Master				0.9889	Master				27.81
	0.9500 (Minimum)	1.000 (Nominal)	1.050 (Maximum)			0.9500 (Minimum)	1.000 (Nominal)	1.050 (Maximum)			20.00 (Minimum)	27.50 (Nominal)	35.00 (Maximum)	

Master: 28-Nov-2002 19:54

Accelerator-Porosity Tool Master Calibration														
Detector Calibration														
Phase	Near/Far Calibration Ratio			Value	Phase	Near/Array Calibration Ratio			Value	Phase	Near/Array Cal Ratio Up/Down			Value
Master				0.8869	Master				1.051	Master				1.002
	0.8000 (Minimum)	0.9250 (Nominal)	1.050 (Maximum)			0.9000 (Minimum)	1.030 (Nominal)	1.170 (Maximum)			0.9700 (Minimum)	1.000 (Nominal)	1.030 (Maximum)	

Master: 28-Nov-2002 19:53

Accelerator-Porosity Tool Master Calibration														
Tank Check														
Phase	Array-1 Standoff Porosity PU			Value	Phase	Array-2 Standoff Porosity PU			Value	Phase	Average Slowing Down Time US			Value
Master				11.90	Master				11.44	Master				5.850
	9.900 (Minimum)	11.75 (Nominal)	13.60 (Maximum)			9.900 (Minimum)	11.75 (Nominal)	13.60 (Maximum)			5.500 (Minimum)	6.000 (Nominal)	6.250 (Maximum)	
Phase	Array-1 SDT Ratio Up/Down			Value	Phase	Array-2 SDT Ratio Up/Down			Value	Phase	Sigma Formation CU			Value
Master				0.9966	Master				0.9889	Master				27.81
	0.9500 (Minimum)	1.000 (Nominal)	1.050 (Maximum)			0.9500 (Minimum)	1.000 (Nominal)	1.050 (Maximum)			20.00 (Minimum)	27.50 (Nominal)	35.00 (Maximum)	

Master: 28-Nov-2002 19:54

Hostile Natural Gamma Ray Sonde / Equipment Identification			
Primary Equipment:	HNGS Sonde	HNGS - BA	77
Auxiliary Equipment:	HNGS Sonde Housing	HNSH - BA	79
	Gamma Source Radioactive	GSR - U	135

Hostile Natural Gamma Ray Sonde Wellsite Calibration														
Detector 1 Check														
Phase	Na 511 Peak Loc			Value	Phase	Na 511 Peak Res %			Value	Phase	High Voltage V			Value
Master				40.59	Master				17.05	Master				1212
Before				40.72	Before				17.42	Before				1212
After				40.70	After				16.61	After				1215
	37.50 (Minimum)	40.00 (Nominal)	42.50 (Maximum)			12.00 (Minimum)	15.50 (Nominal)	19.00 (Maximum)			900.0 (Minimum)	1150 (Nominal)	1600 (Maximum)	
Phase	Na 1785 Peak Loc			Value	Phase	Na 1785 Peak Res %			Value	Phase	Temperature DEGC			Value
Master				145.6	Master				9.037	Master				32.69
Before				145.3	Before				9.666	Before				32.84
After				145.8	After				9.711	After				29.54
	135.0 (Minimum)	142.6 (Nominal)	150.3 (Maximum)			7.000 (Minimum)	8.500 (Nominal)	11.00 (Maximum)			-28.89 (Minimum)	15.50 (Nominal)	60.00 (Maximum)	
Phase	Na Count Rate CPS			Value										
Master				44.80										
Before				43.98										
After				43.51										
	10.00 (Minimum)	45.00 (Nominal)	100.0 (Maximum)											

Master: 15-Jan-2003 16:08

Before: 15-Jan-2003 16:17

After: 19-Jan-2003 2:15

Hostile Natural Gamma Ray Sonde Wellsite Calibration													
Detector 2 Check													

Na 511 Peak Loc			Na 511 Peak Res %			High Voltage V		
Phase		Value	Phase		Value	Phase		Value
Master		40.55	Master		16.60	Master		1239
Before		40.57	Before		16.91	Before		1239
After		40.61	After		17.25	After		1242
	37.50 (Minimum) 40.00 (Nominal) 42.50 (Maximum)			12.00 (Minimum) 15.50 (Nominal) 19.00 (Maximum)			900.0 (Minimum) 1150 (Nominal) 1600 (Maximum)	
Na 1785 Peak Loc			Na 1785 Peak Res %			Temperature DEGC		
Master		144.7	Master		9.925	Master		32.80
Before		144.4	Before		9.708	Before		32.89
After		144.4	After		9.893	After		29.63
	135.0 (Minimum) 142.6 (Nominal) 150.3 (Maximum)			7.000 (Minimum) 8.500 (Nominal) 11.00 (Maximum)			-28.89 (Minimum) 15.50 (Nominal) 60.00 (Maximum)	
Na Count Rate CPS								
Master		44.45						
Before		43.98						
After		43.50						
	10.00 (Minimum) 45.00 (Nominal) 100.0 (Maximum)							
Master: 15-Jan-2003 16:08			Before: 15-Jan-2003 16:17			After: 19-Jan-2003 2:15		

Hostile Natural Gamma Ray Sonde Wellsite Calibration		
Ratio Of Detector 1 To Detector 2		
Phase	Coincidence Count Rate Ratio	Value
Master		1.008
Before		1.0000
After		1.001
	0.9500 (Minimum) 1.000 (Nominal) 1.050 (Maximum)	
Master: 15-Jan-2003 16:08		
Before: 15-Jan-2003 16:17		
After: 19-Jan-2003 2:15		

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 1 Calibration								
Na 511 Peak Set Point			Th Peak Loc			Th Peak Res %		
Phase		Value	Phase		Value	Phase		Value
Master		41.00	Master		209.3	Master		8.207
	38.00 (Minimum) 40.00 (Nominal) 42.00 (Maximum)			201.0 (Minimum) 209.6 (Nominal) 218.3 (Maximum)			5.000 (Minimum) 7.000 (Nominal) 9.000 (Maximum)	
Background Count Rate CPS			Gain Ratio					
Master		23.15	Master		0.9810			
	20.00 (Minimum) 142.5 (Nominal) 265.0 (Maximum)			0.9400 (Minimum) 1.000 (Nominal) 1.060 (Maximum)				
Master: 15-Jan-2003 16:01								

Hostile Natural Gamma Ray Sonde Master Calibration								
Detector 2 Calibration								
Na 511 Peak Set Point			Th Peak Loc			Th Peak Res %		
Phase		Value	Phase		Value	Phase		Value
Master		41.00	Master		209.3	Master		7.848
	38.00 (Minimum) 40.00 (Nominal) 42.00 (Maximum)			201.0 (Minimum) 209.6 (Nominal) 218.3 (Maximum)			5.000 (Minimum) 7.000 (Nominal) 9.000 (Maximum)	
Background Count Rate CPS			Gain Ratio					
Master		21.80	Master		0.9821			
	20.00 (Minimum) 142.5 (Nominal) 265.0 (Maximum)			0.9400 (Minimum) 1.000 (Nominal) 1.060 (Maximum)				
Master: 15-Jan-2003 16:01								

Company: Lamont Doherty

Schlumberger

Well: ODP Leg 207 Site 1257A

Field: Demarara Rise

Country: Venezuela

Ocean: Atlantic

HLDS/APS Porosity
Natural Gamma Ray